

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022223.D
 Acq On : 04 Oct 2024 10:46
 Operator : RC/JU
 Sample : P4018-09MEDL 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DDCB5MEDL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/04/2024
 Supervised By :mohammad ahmed 10/05/2024

Quant Time: Oct 04 11:46:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 05:25:28 2024
 Response via : Initial Calibration

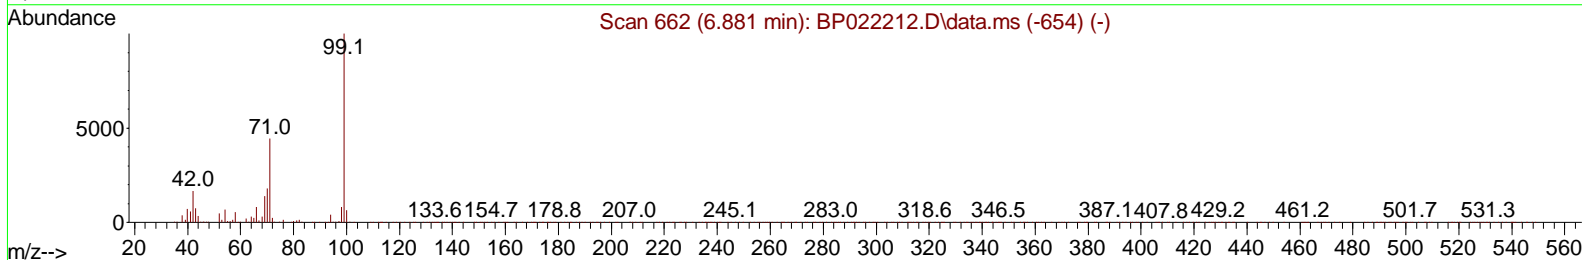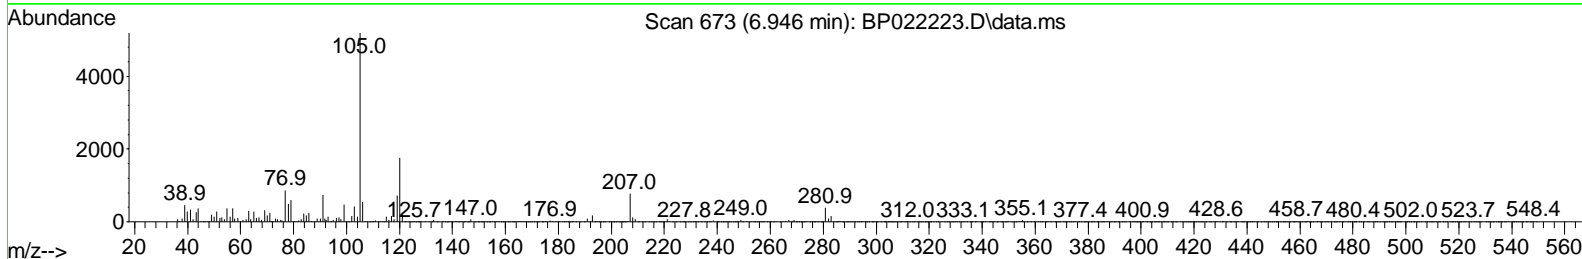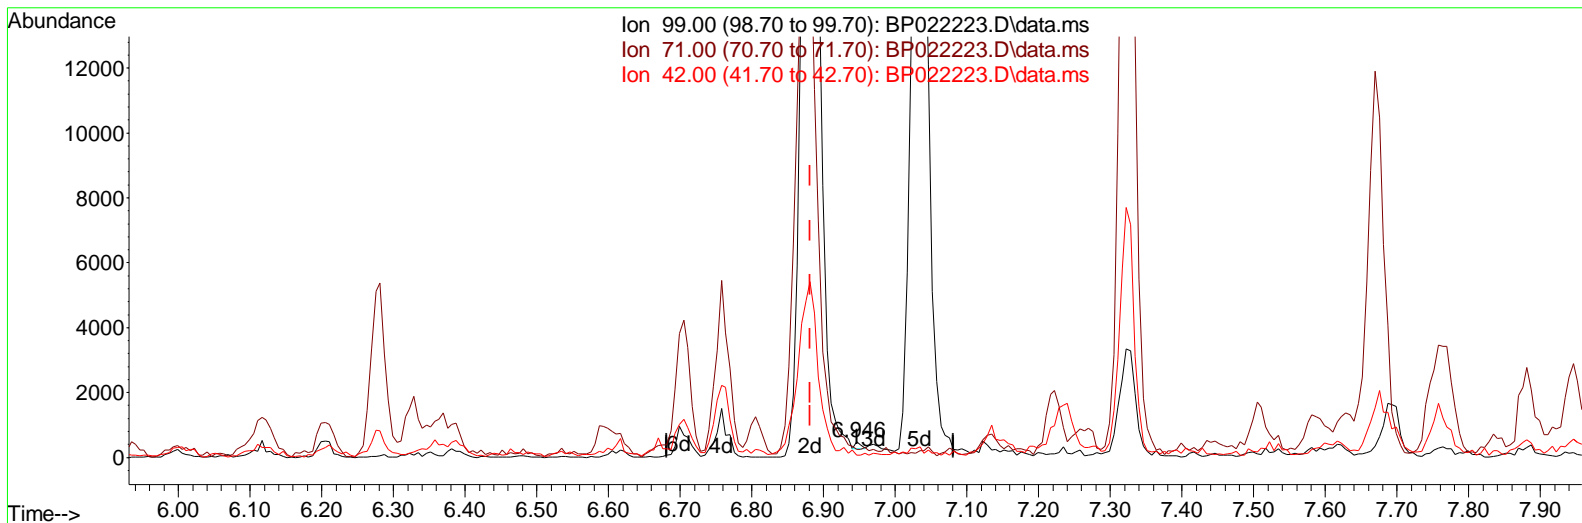

TIC: BP022223.D\data.ms

(7) Phenol-d5 (S)

6.946min (+ 0.065) 0.01 ng/ul

response 130

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	44.50	50.83
42.00	17.90	16.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022223.D
 Acq On : 04 Oct 2024 10:46
 Operator : RC/JU
 Sample : P4018-09MEDL 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DDCB5MEDL

Manual Integrations APPROVED

Quant Time: Oct 04 11:46:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 05:25:28 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 10/04/2024
 Supervised By :mohammad ahmed 10/05/2024

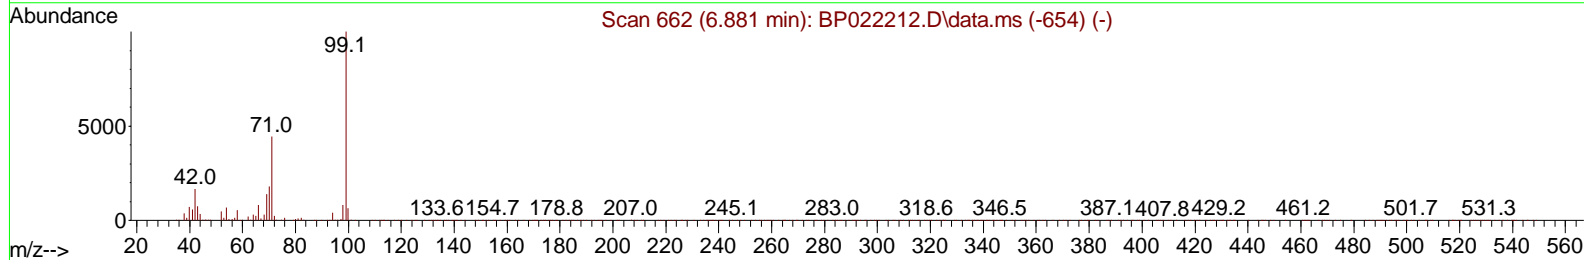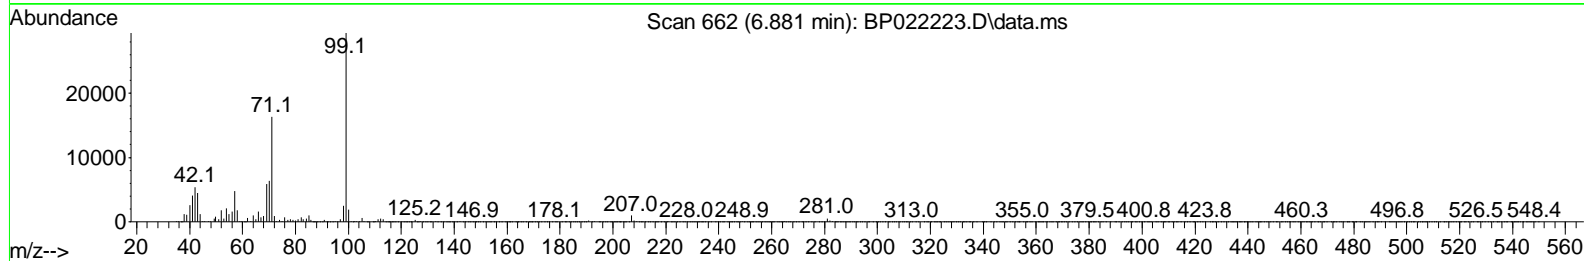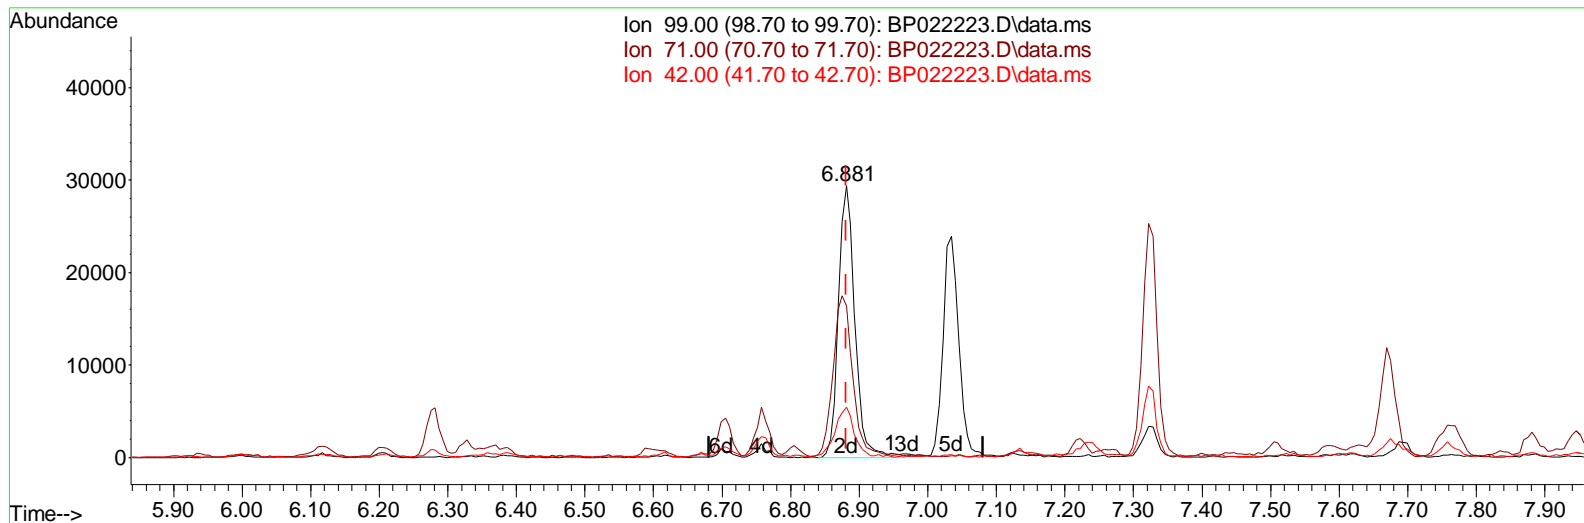

TIC: BP022223.D\data.ms

(7) Phenol-d5 (S)

6.881min (+ 0.000) 3.90 ng/ul m

response 48816

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	44.50	55.75#
42.00	17.90	18.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022223.D
 Acq On : 04 Oct 2024 10:46
 Operator : RC/JU
 Sample : P4018-09MEDL 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 DDCB5MEDL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 10/04/2024
 Supervised By :mohammad ahmed 10/05/2024

Quant Time: Oct 05 02:24:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALI BRATI ON
 QLast Update : Fri Oct 04 05:25:28 2024
 Response via : Initial Calibration

Compound	R. T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Di chl orobenzene-d4	7.693	152	153030	20.000	ng/ul	0.00
20) Naphthal ene-d8	10.452	136	568869	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164	433839	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.104	188	1037438	20.000	ng/ul	0.01
79) Chrysene-d12	21.533	240	1125926	20.000	ng/ul	0.00
88) Peryl ene-d12	24.804	264	1301190	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Di oxane-d8	3.223	96	2668	0.683	ng/uL	0.00
4) Pyri di ne-d5	3.640	84	36616	3.279	ng/ul	0.01
7) Phenol -d5	6.881	99	48816m	3.900	ng/ul	0.00
9) Bi s-(2-Chl oroethyl)eth. . .	7.034	67	32091	4.163	ng/ul	0.00
11) 2-Chl orophenol -d4	7.234	132	38797	4.284	ng/ul	0.00
15) 4-Methyl phenol -d8	8.393	113	39466	3.979	ng/ul	0.00
21) Ni trobenzene-d5	8.828	128	19014	4.466	ng/ul	0.00
24) 2-Ni trophenol -d4	9.540	143	19573	4.054	ng/ul	0.00
28) 2,4-Di chl orophenol -d3	10.087	165	44318	4.227	ng/ul	0.00
31) 4-Chl oroani li ne-d4	10.587	131	51100	4.085	ng/ul	0.00
46) Di methyl phthal ate-d6	13.710	166	165304	4.929	ng/ul	0.00
49) Acenaphthyl ene-d8	13.993	160	169190	4.765	ng/ul	0.00
54) 4-Ni trophenol -d4	0.000	143	Od	0.000	ng/ul	
60) Fl uorene-d10	15.310	176	143582	4.840	ng/ul	0.00
65) 4,6-Di ni tro-2-methyl ph. . .	15.434	200	14304	2.221	ng/ul	0.00
73) Anthracene-d10	17.198	188	243814	5.034	ng/ul	0.00
81) Pyrene-d10	19.581	212	304157	5.214	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.580	264	332673	4.861	ng/ul	0.00
Target Compounds						
58) 2,3,4,6-Tetrachl orophenol	14.940	232	111060	11.080	ng/ul	97
71) Pentachl orophenol	16.751	266	1218144	120.693	ng/ul	99

(#) = qual i fi er out of range (m) = manual i ntegrati on (+) = signal s summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022223.D
 Acq On : 04 Oct 2024 10:46
 Operator : RC/JU
 Sample : P4018-09MEDL 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :

BNA_P

ClientSampleId :

DDCB5MEDL

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay 10/04/2024
 Supervised By : mohammad ahmed 10/05/2024

Quant Time: Oct 05 02:24:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 05:25:28 2024
 Response via : Initial Calibration

