

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022161.D
 Acq On : 02 Oct 2024 14:06
 Operator : RC/JU
 Sample : P4016-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCVT2

Quant Time: Oct 02 15:00:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	148072	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.451	136	558166	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.316	164	425903	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.110	188	997666	20.000	ng/u1	0.00
79) Chrysene-d12	21.551	240	1037469	20.000	ng/u1	0.01
88) Perylene-d12	24.845	264	1240316	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	8504	2.250	ng/uL	0.00
4) Pyridine-d5	3.634	84	124701	11.540	ng/u1	0.00
7) Phenol-d5	6.887	99	173938	14.360	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.034	67	99368	13.323	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.240	132	134597	15.359	ng/u1	0.00
15) 4-Methylphenol-d8	8.399	113	146358	15.249	ng/u1	0.00
21) Nitrobenzene-d5	8.834	128	63698	15.247	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.552	143	80725	17.042	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.081	165	158095	15.369	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.587	131	179519	14.626	ng/u1	-0.02
46) Dimethylphthalate-d6	13.710	166	519235	15.771	ng/u1	-0.01
49) Acenaphthylene-d8	13.998	160	540627	15.510	ng/u1	0.00
54) 4-Nitrophenol-d4	14.534	143	64924	11.529	ng/u1	0.00
60) Fluorene-d10	15.322	176	449536	15.436	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.434	200	61173	9.876	ng/u1	-0.01
73) Anthracene-d10	17.204	188	760666	16.332	ng/u1	-0.01
81) Pyrene-d10	19.598	212	923052	17.173	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.615	264	1078905	16.538	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.757	266	30306	3.122	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022161.D
Acq On : 02 Oct 2024 14:06
Operator : RC/JU
Sample : P4016-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVT2

Quant Time: Oct 02 15:00:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

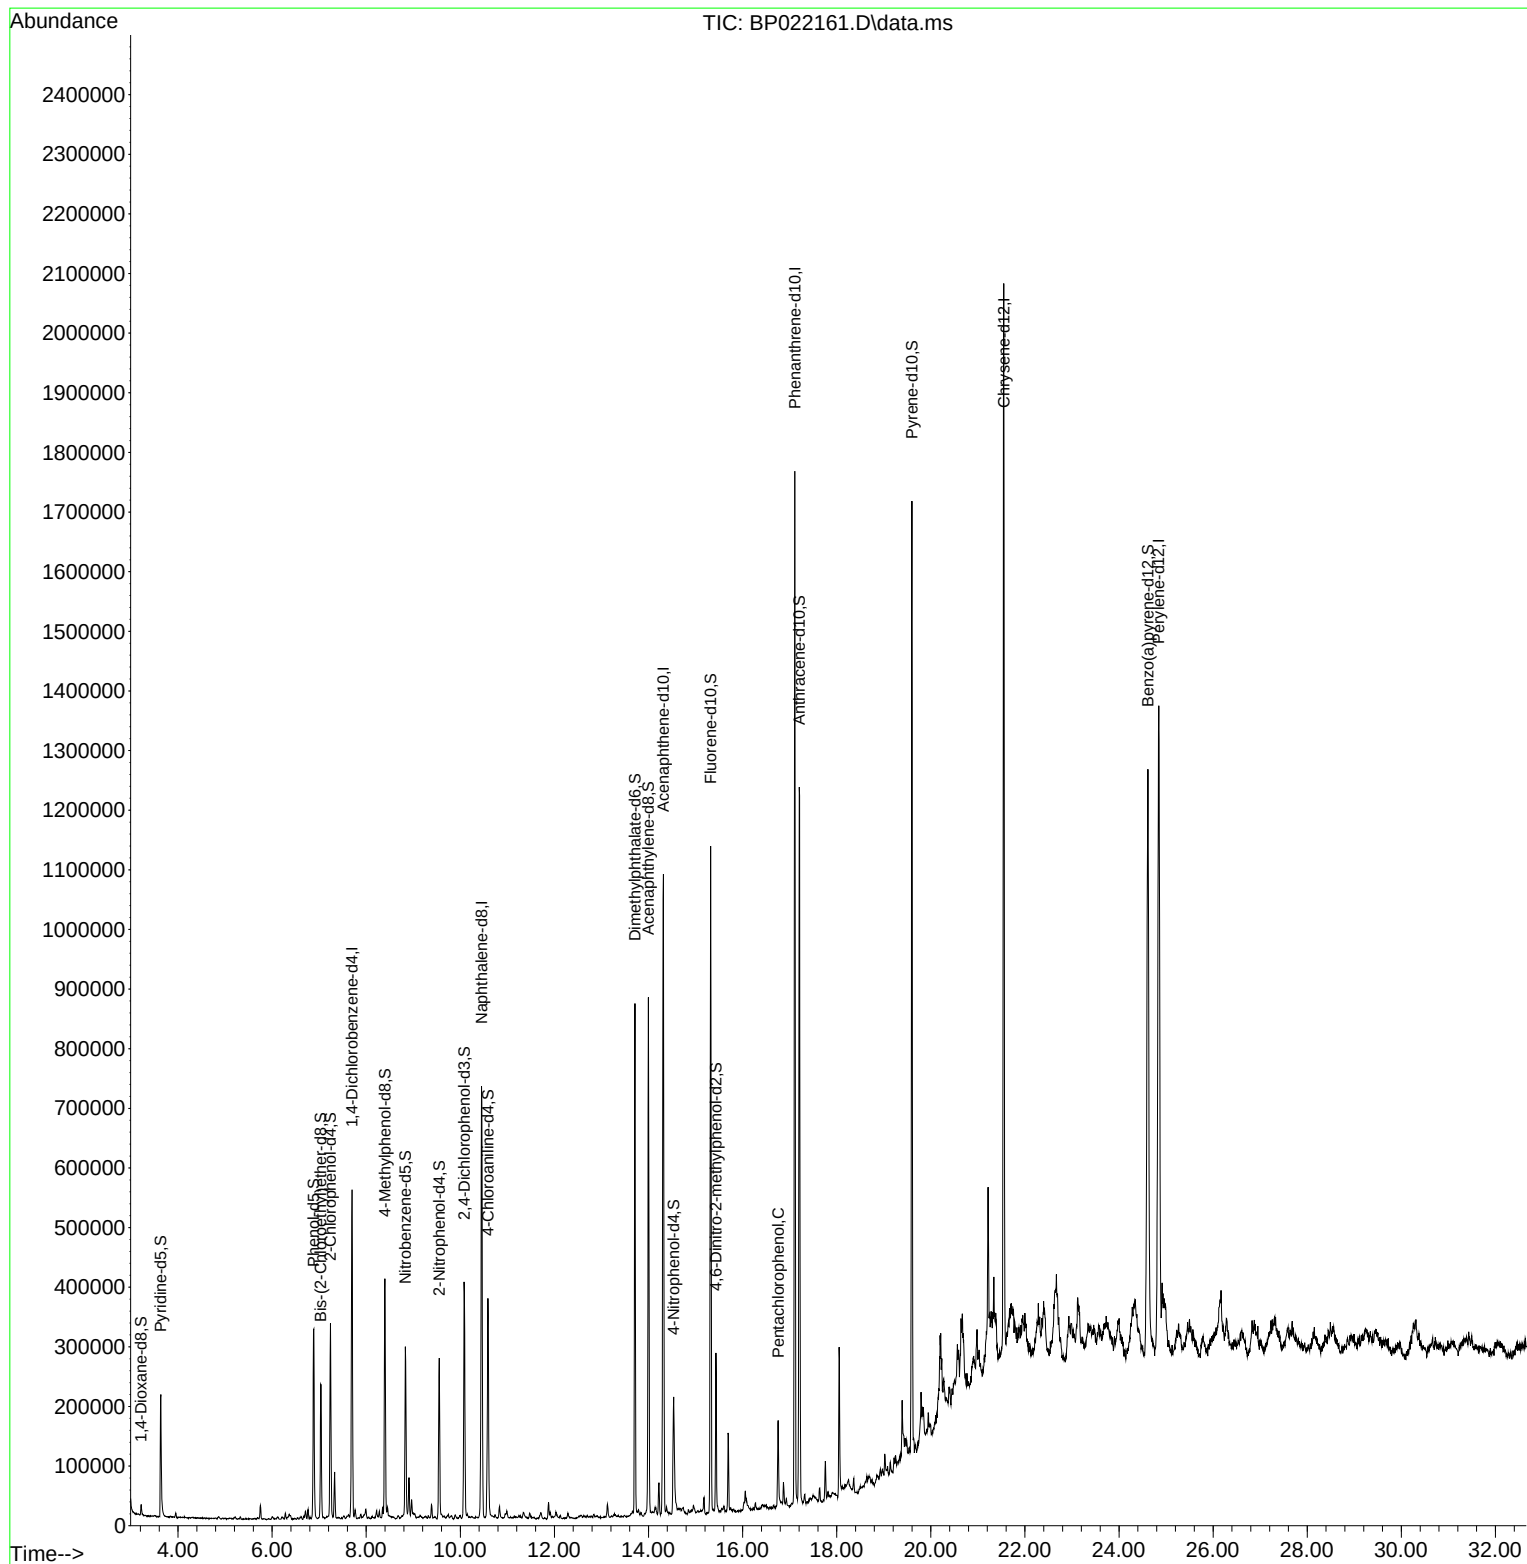

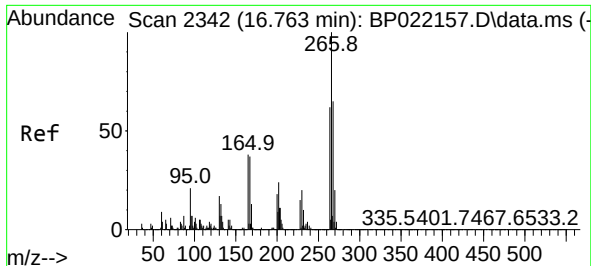

#71
 Pentachlorophenol
 Concen: 3.122 ng/ul
 RT: 16.757 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP022161.D
 Acq: 02 Oct 2024 14:06

Instrument :
 BNA_P
 ClientSampleId :
 DCVT2

Tgt Ion:266 Resp: 30306
 Ion Ratio Lower Upper
 266 100
 264 64.7 50.2 75.4
 268 69.8 51.4 77.0

