

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022162.D
 Acq On : 02 Oct 2024 14:47
 Operator : RC/JU
 Sample : P4016-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCVT3

Quant Time: Oct 02 15:23:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	168519	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.457	136	657193	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.310	164	503960	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.098	188	1178137	20.000	ng/u1	-0.02
79) Chrysene-d12	21.533	240	1232048	20.000	ng/u1	0.00
88) Perylene-d12	24.827	264	1400423	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	12096	2.812	ng/uL	0.00
4) Pyridine-d5	3.634	84	181676	14.773	ng/u1	0.00
7) Phenol-d5	6.887	99	250361	18.162	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	144035	16.969	ng/u1	0.00
11) 2-Chlorophenol-d4	7.240	132	196390	19.691	ng/u1	0.00
15) 4-Methylphenol-d8	8.399	113	210899	19.307	ng/u1	0.00
21) Nitrobenzene-d5	8.840	128	92501	18.805	ng/u1	0.00
24) 2-Nitrophenol-d4	9.552	143	120858	21.670	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.081	165	239545	19.778	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.593	131	260555	18.030	ng/u1	-0.01
46) Dimethylphthalate-d6	13.716	166	752668	19.321	ng/u1	0.00
49) Acenaphthylene-d8	13.998	160	781942	18.958	ng/u1	0.00
54) 4-Nitrophenol-d4	14.528	143	102177	15.334	ng/u1	0.00
60) Fluorene-d10	15.316	176	660986	19.181	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.439	200	105042	14.361	ng/u1	0.00
73) Anthracene-d10	17.204	188	1113257	20.241	ng/u1	-0.01
81) Pyrene-d10	19.586	212	1364064	21.370	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.598	264	1487444	20.194	ng/u1	-0.01
Target Compounds						
71) Pentachlorophenol	16.745	266	33141	2.891	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022162.D
Acq On : 02 Oct 2024 14:47
Operator : RC/JU
Sample : P4016-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVT3

Quant Time: Oct 02 15:23:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

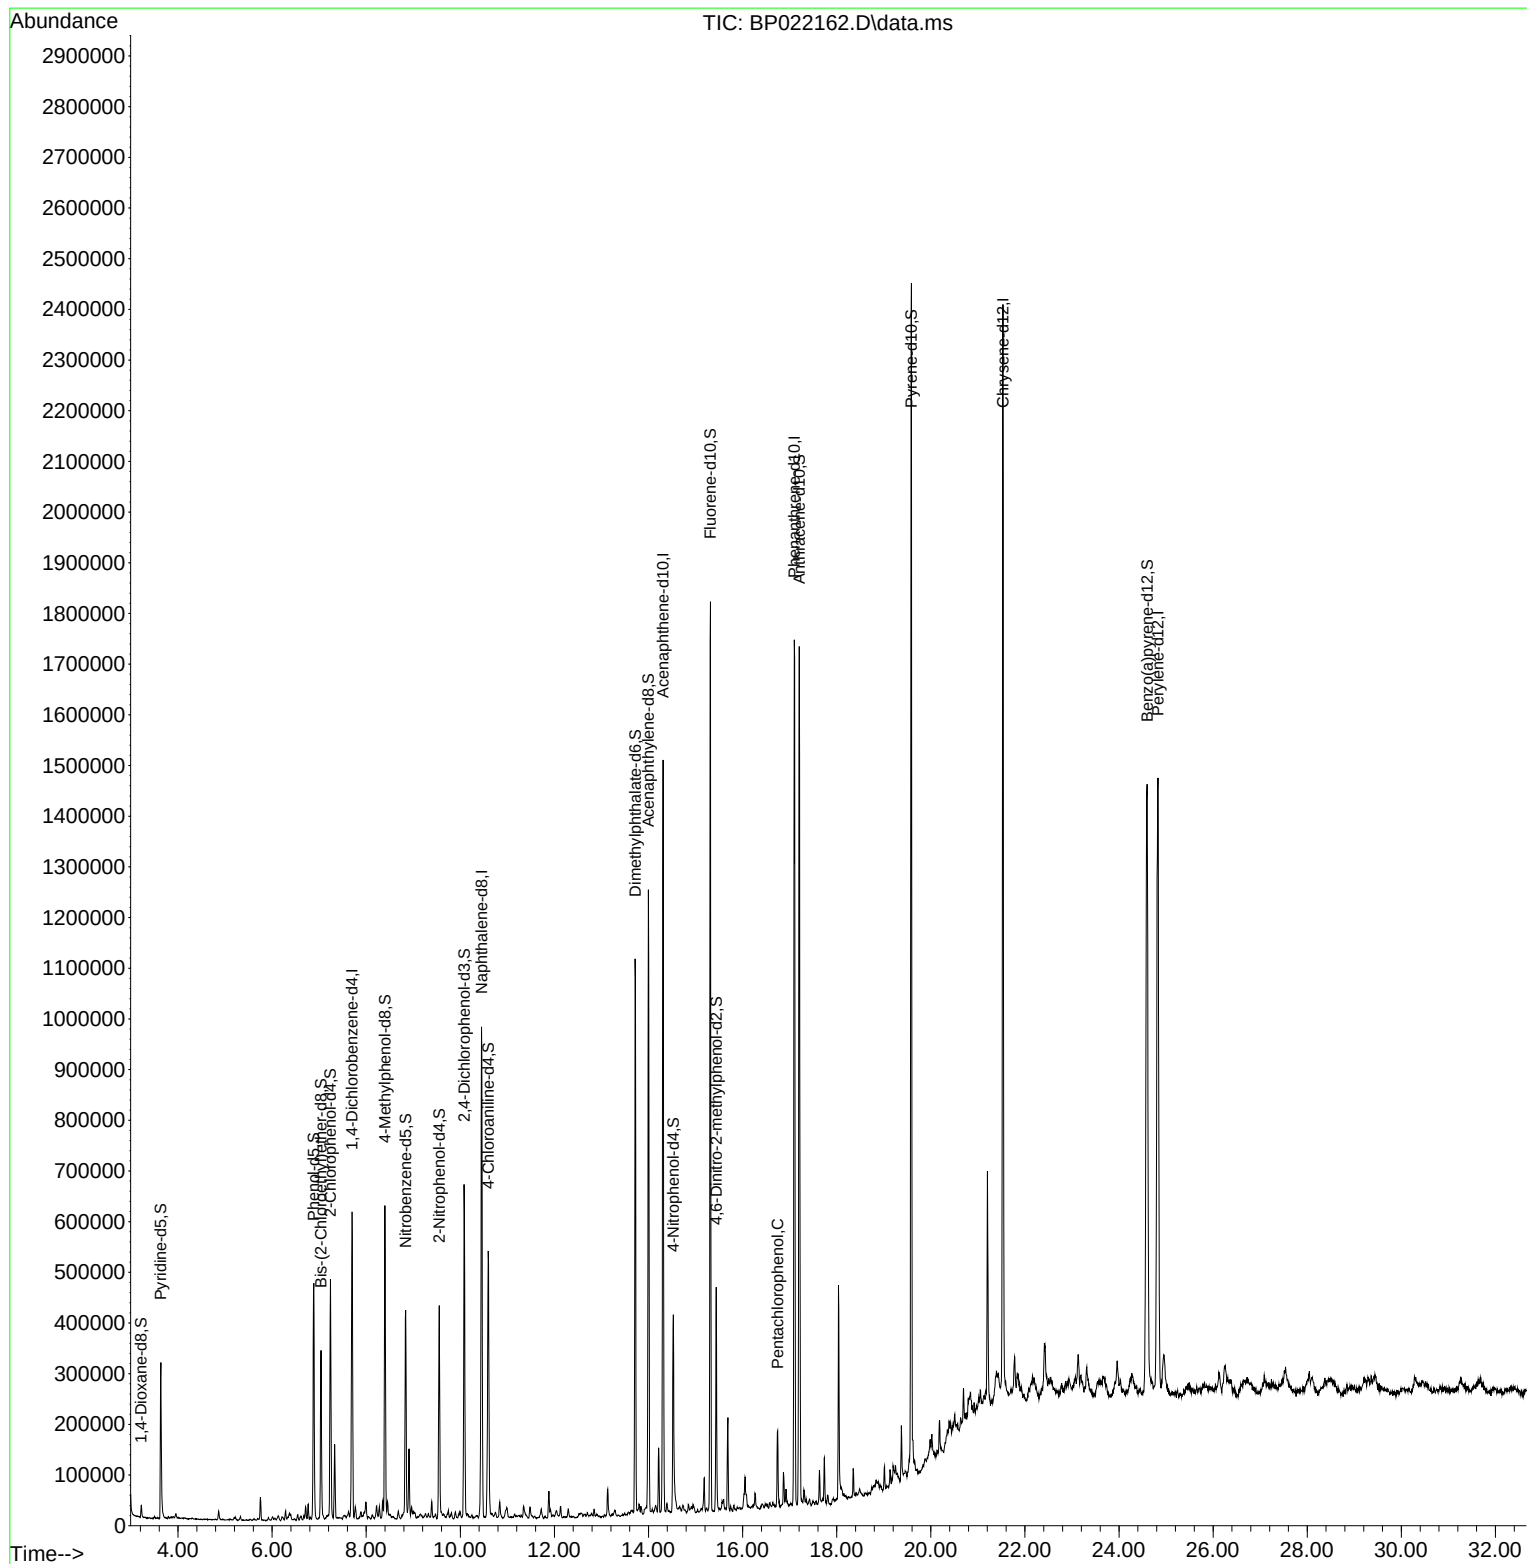

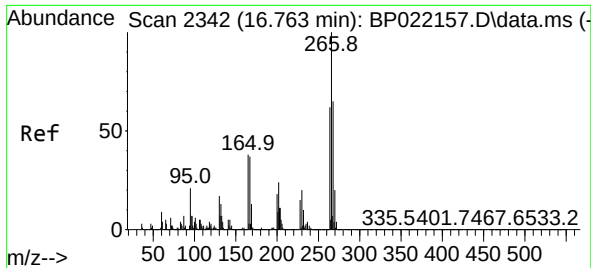

#71
 Pentachlorophenol
 Concen: 2.891 ng/ul
 RT: 16.745 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP022162.D
 Acq: 02 Oct 2024 14:47

Instrument :
 BNA_P
 ClientSampleId :
 DCVT3

Tgt Ion:266 Resp: 33141
 Ion Ratio Lower Upper
 266 100
 264 62.8 50.2 75.4
 268 66.8 51.4 77.0

