

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022163.D
 Acq On : 02 Oct 2024 15:27
 Operator : RC/JU
 Sample : P4016-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCVT4

Quant Time: Oct 02 15:59:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	152016	20.000	ng/u1	-0.02
20) Naphthalene-d8	10.458	136	593724	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.310	164	449932	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.110	188	1048073	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	1144650	20.000	ng/u1	0.00
88) Perylene-d12	24.839	264	1334719	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	10594	2.730	ng/uL	0.00
4) Pyridine-d5	3.634	84	152207	13.720	ng/u1	0.00
7) Phenol-d5	6.881	99	225686	18.149	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.034	67	123373	16.112	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.234	132	167601	18.629	ng/u1	-0.01
15) 4-Methylphenol-d8	8.393	113	185960	18.872	ng/u1	-0.01
21) Nitrobenzene-d5	8.834	128	79232	17.830	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.546	143	101019	20.049	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.081	165	204698	18.707	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.587	131	229797	17.601	ng/u1	-0.02
46) Dimethylphthalate-d6	13.716	166	693643	19.944	ng/u1	0.00
49) Acenaphthylene-d8	13.999	160	713261	19.370	ng/u1	0.00
54) 4-Nitrophenol-d4	14.528	143	96498	16.220	ng/u1	0.00
60) Fluorene-d10	15.316	176	601197	19.541	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.445	200	100391	15.428	ng/u1	0.00
73) Anthracene-d10	17.222	188	1028877	21.028	ng/u1	0.00
81) Pyrene-d10	19.592	212	1256435	21.187	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.604	264	1445403	20.589	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.757	266	187321	18.371	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022163.D
Acq On : 02 Oct 2024 15:27
Operator : RC/JU
Sample : P4016-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVT4

Quant Time: Oct 02 15:59:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

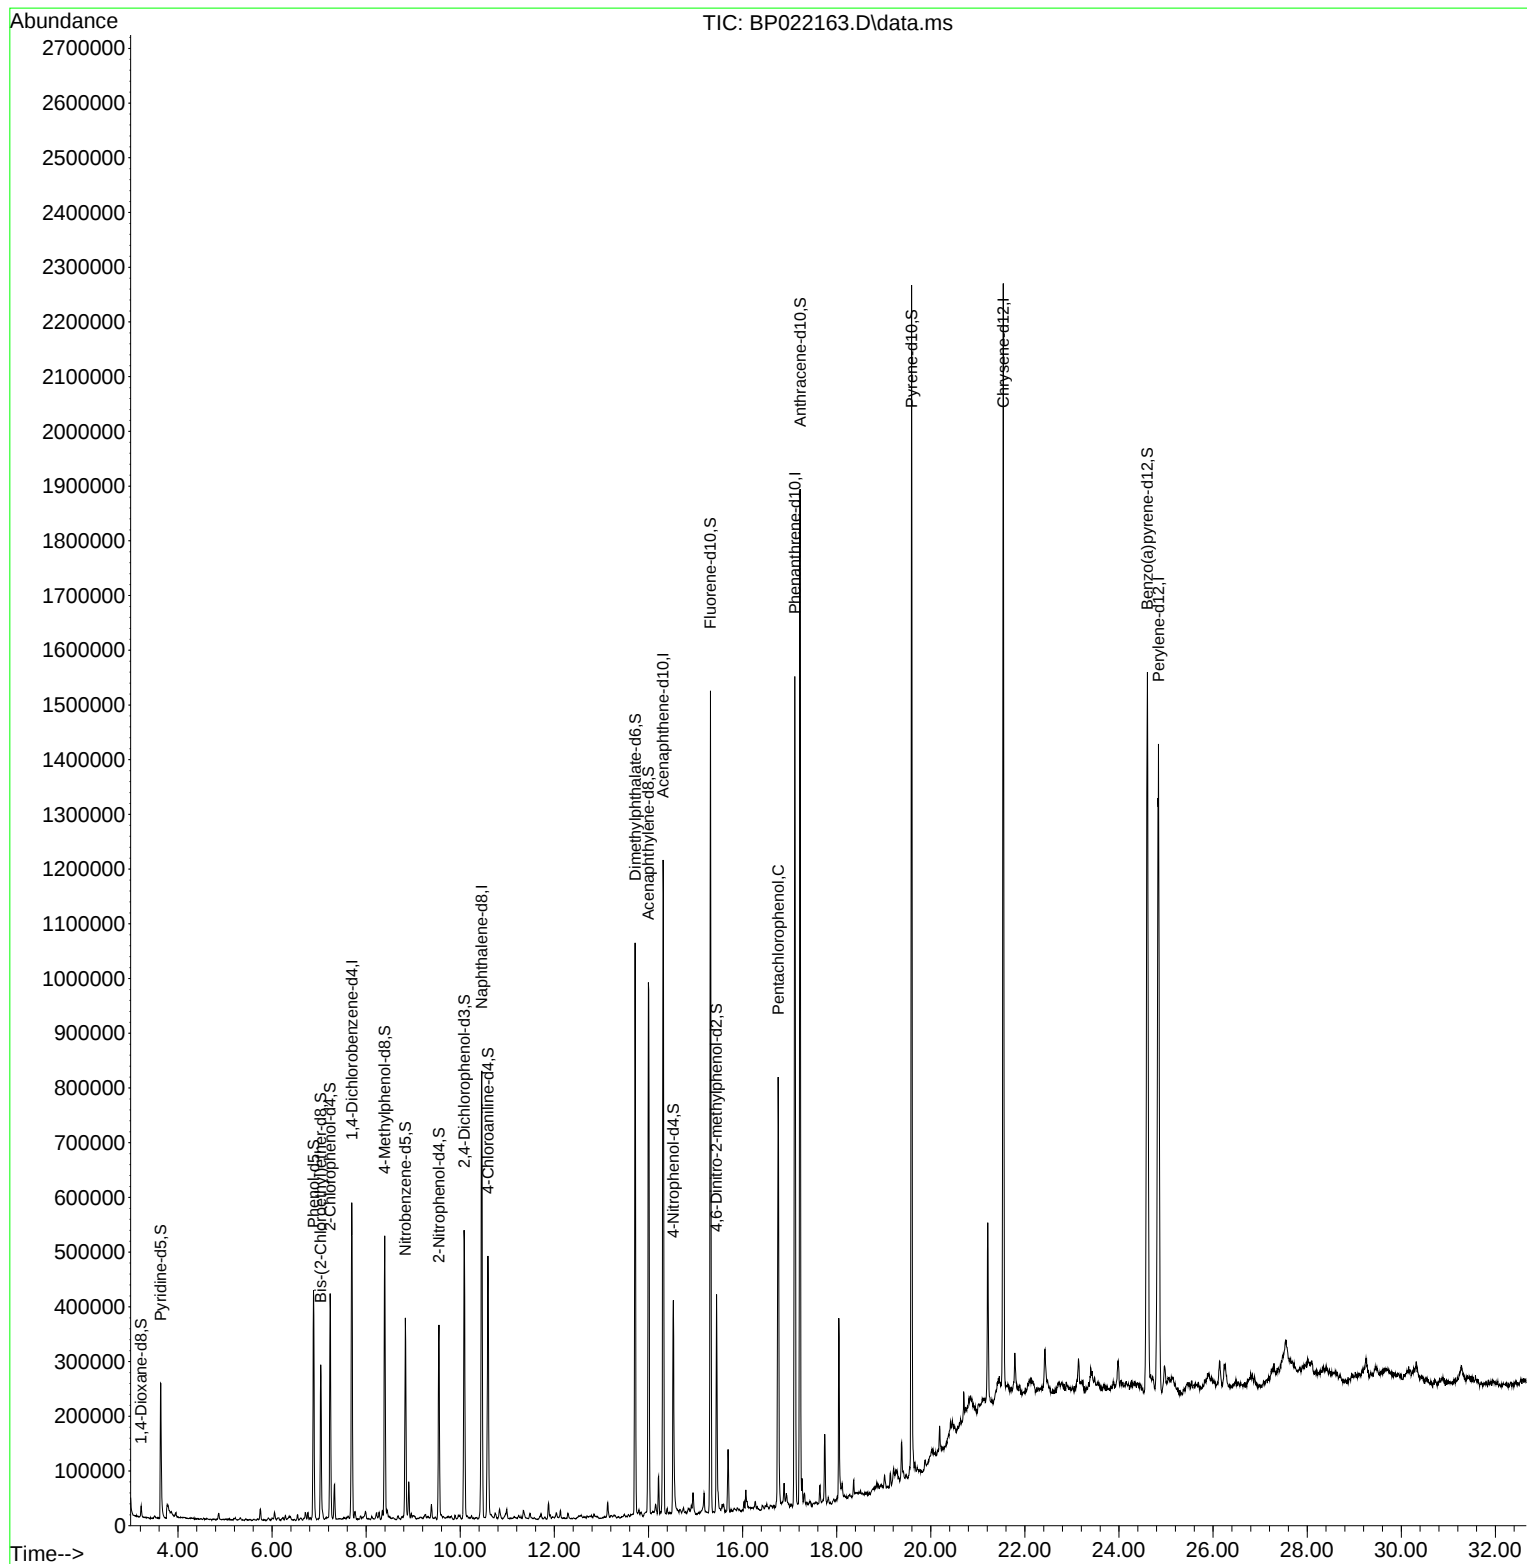

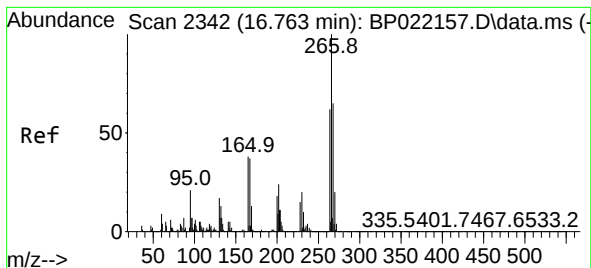

#71

Pentachlorophenol

Concen: 18.371 ng/ul

RT: 16.757 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP022163.D


Acq: 02 Oct 2024 15:27

Instrument :

BNA_P

ClientSampleId :

DCVT4

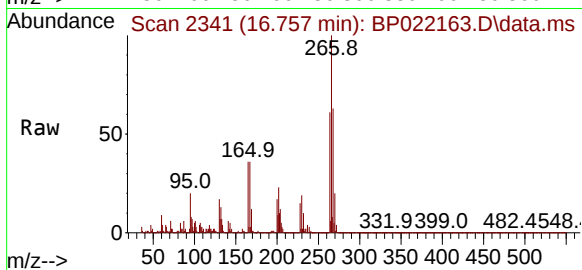

Tgt Ion:266 Resp: 187321

Ion Ratio Lower Upper

266 100

264 60.5 50.2 75.4

268 63.4 51.4 77.0

