

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022169.D
 Acq On : 02 Oct 2024 19:32
 Operator : RC/JU
 Sample : P4016-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCVT9

Quant Time: Oct 02 23:17:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 24 15:23:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	133030	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.452	136	533307	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.304	164	418229	20.000	ng/u1	-0.02
64) Phenanthrene-d10	17.098	188	994120	20.000	ng/u1	-0.02
79) Chrysene-d12	21.533	240	1061553	20.000	ng/u1	0.00
88) Perylene-d12	24.804	264	1235264	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	8925	2.628	ng/uL	0.00
4) Pyridine-d5	3.634	84	137911	14.206	ng/u1	0.00
7) Phenol-d5	6.881	99	190343	17.492	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.034	67	110965	16.560	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.234	132	144355	18.335	ng/u1	-0.01
15) 4-Methylphenol-d8	8.399	113	163702	18.985	ng/u1	0.00
21) Nitrobenzene-d5	8.828	128	65788	16.482	ng/u1	-0.02
24) 2-Nitrophenol-d4	9.546	143	75634	16.711	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.081	165	176771	17.985	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.587	131	208878	17.811	ng/u1	-0.02
46) Dimethylphthalate-d6	13.704	166	621078	19.211	ng/u1	-0.02
49) Acenaphthylene-d8	13.993	160	647800	18.925	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.522	143	64306	11.629	ng/u1	0.00
60) Fluorene-d10	15.310	176	543495	19.005	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.428	200	55484	8.990	ng/u1	-0.02
73) Anthracene-d10	17.198	188	925763	19.948	ng/u1	-0.02
81) Pyrene-d10	19.586	212	1126741	20.487	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.586	264	1281622	19.726	ng/u1	-0.02
Target Compounds						
71) Pentachlorophenol	16.745	266	63062	6.520	ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022169.D
Acq On : 02 Oct 2024 19:32
Operator : RC/JU
Sample : P4016-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVT9

Quant Time: Oct 02 23:17:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 24 15:23:13 2024
Response via : Initial Calibration

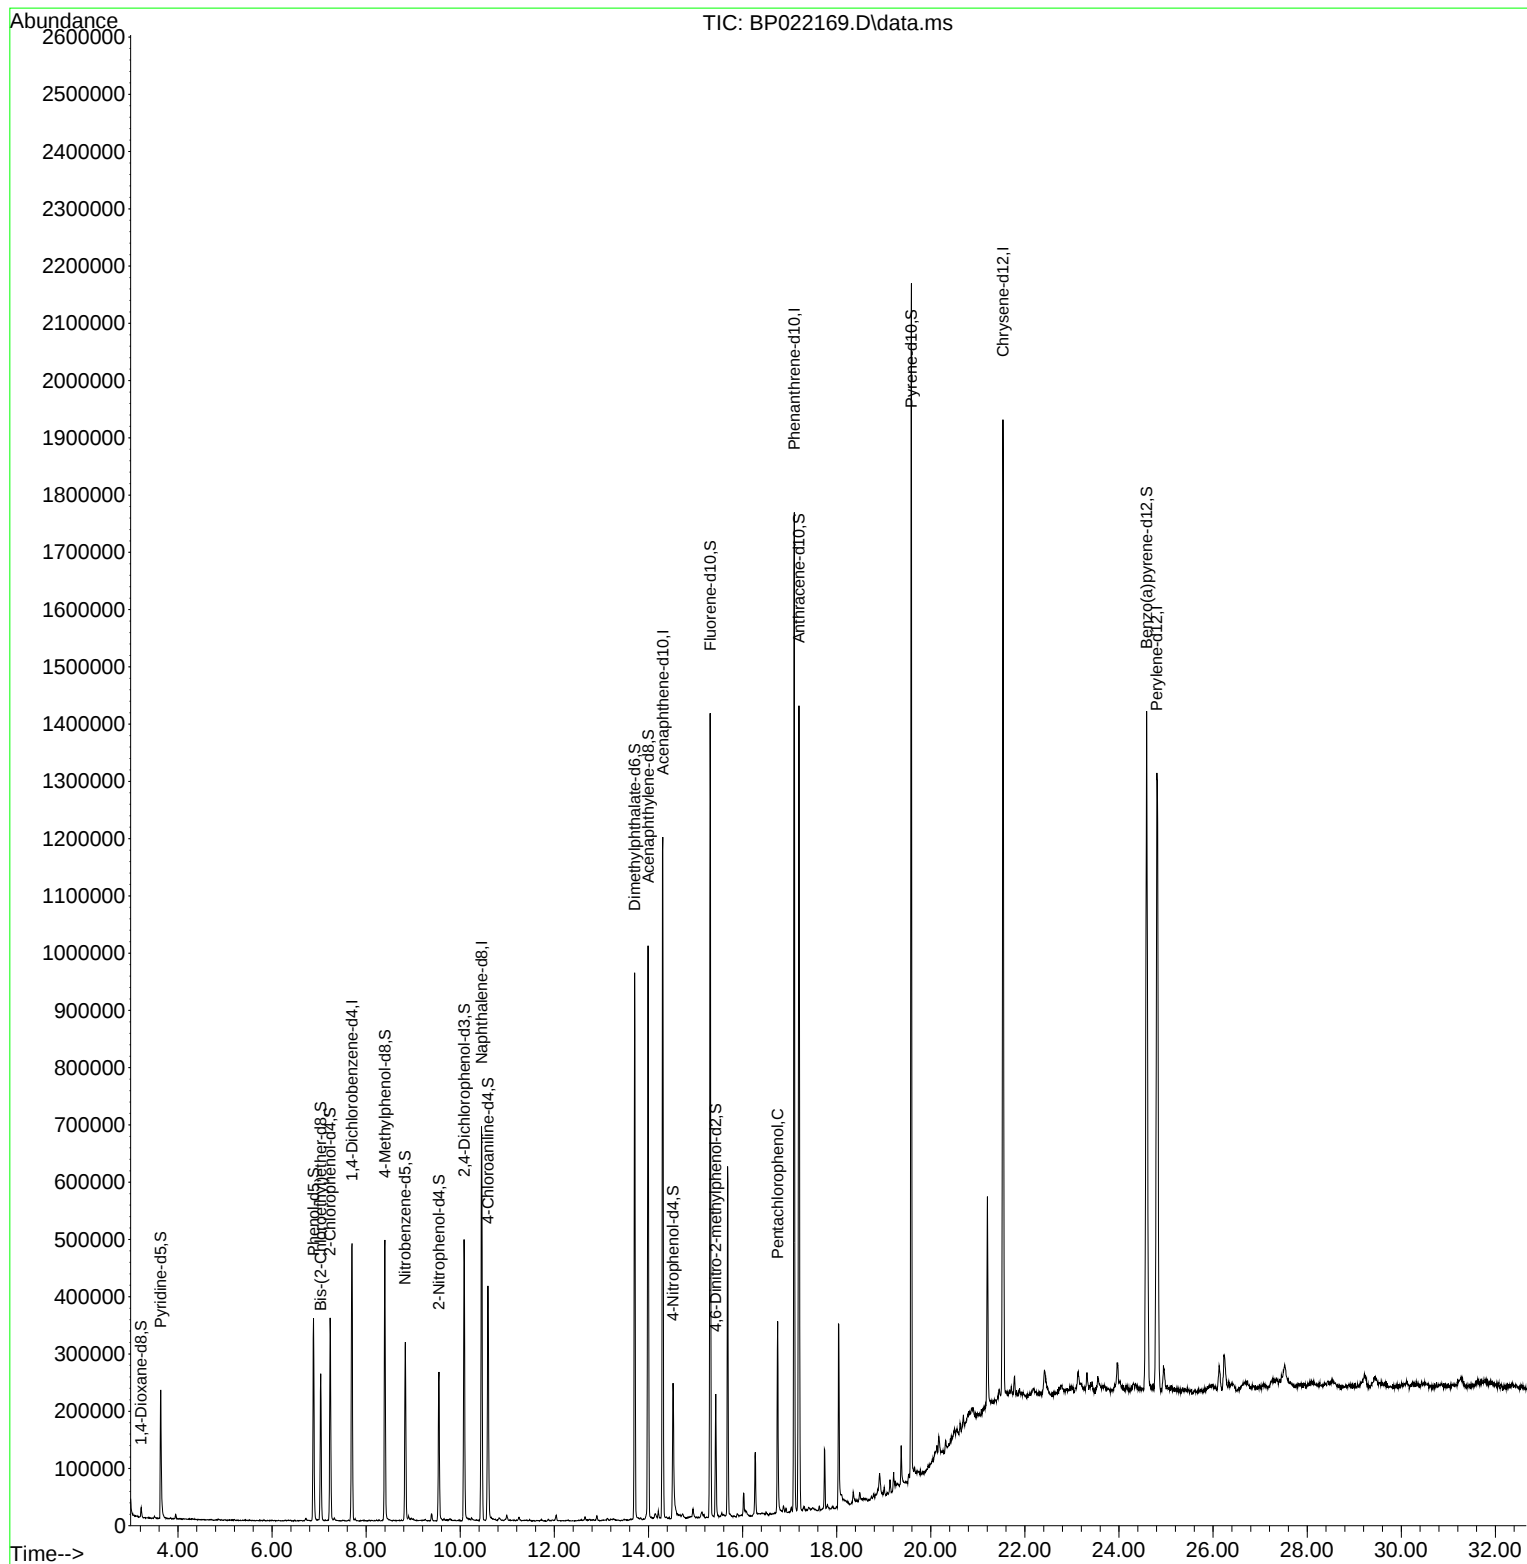

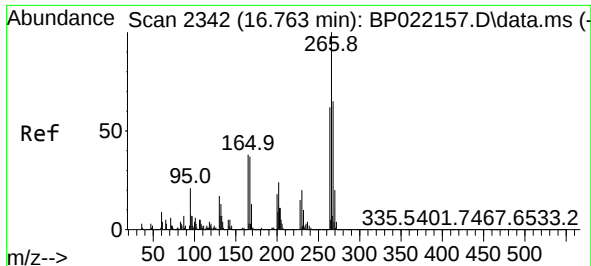

#71
 Pentachlorophenol
 Concen: 6.520 ng/ul
 RT: 16.745 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP022169.D
 Acq: 02 Oct 2024 19:32

Instrument :
 BNA_P
 ClientSampleId :
 DCVT9

Tgt Ion:266 Resp: 63062
 Ion Ratio Lower Upper
 266 100
 264 65.5 50.2 75.4
 268 67.6 51.4 77.0

