

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022215.D
 Acq On : 04 Oct 2024 05:22
 Operator : RC/JU
 Sample : P4017-17DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCD3DL

Quant Time: Oct 04 06:14:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 05:25:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	124505	20.000	ng/u1	0.00
20) Naphthalene-d8	10.457	136	465920	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.304	164	365362	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.098	188	866826	20.000	ng/u1	0.00
79) Chrysene-d12	21.521	240	971329	20.000	ng/u1	-0.01
88) Perylene-d12	24.792	264	1154480	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.887	99	2916	0.286	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	3553	0.567	ng/u1	0.00
11) 2-Chlorophenol-d4	7.245	132	3390	0.460	ng/u1	0.01
15) 4-Methylphenol-d8	0.000	113	0d	0.000	ng/u1	
21) Nitrobenzene-d5	8.840	128	1772	0.508	ng/u1	0.00
24) 2-Nitrophenol-d4	9.551	143	2065	0.522	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.098	165	2962	0.345	ng/u1	0.02
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/u1	
46) Dimethylphthalate-d6	13.710	166	20203	0.715	ng/u1	0.00
49) Acenaphthylene-d8	13.992	160	18481	0.618	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.304	176	18019	0.721	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.204	188	29219	0.722	ng/u1	0.00
81) Pyrene-d10	19.580	212	30042	0.597	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.574	264	21519	0.354	ng/u1	0.00
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	14.939	232	85219	10.096	ng/u1#	96
71) Pentachlorophenol	16.751	266	1884688	223.487	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022215.D
Acq On : 04 Oct 2024 05:22
Operator : RC/JU
Sample : P4017-17DL 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCD3DL

Quant Time: Oct 04 06:14:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 05:25:28 2024
Response via : Initial Calibration




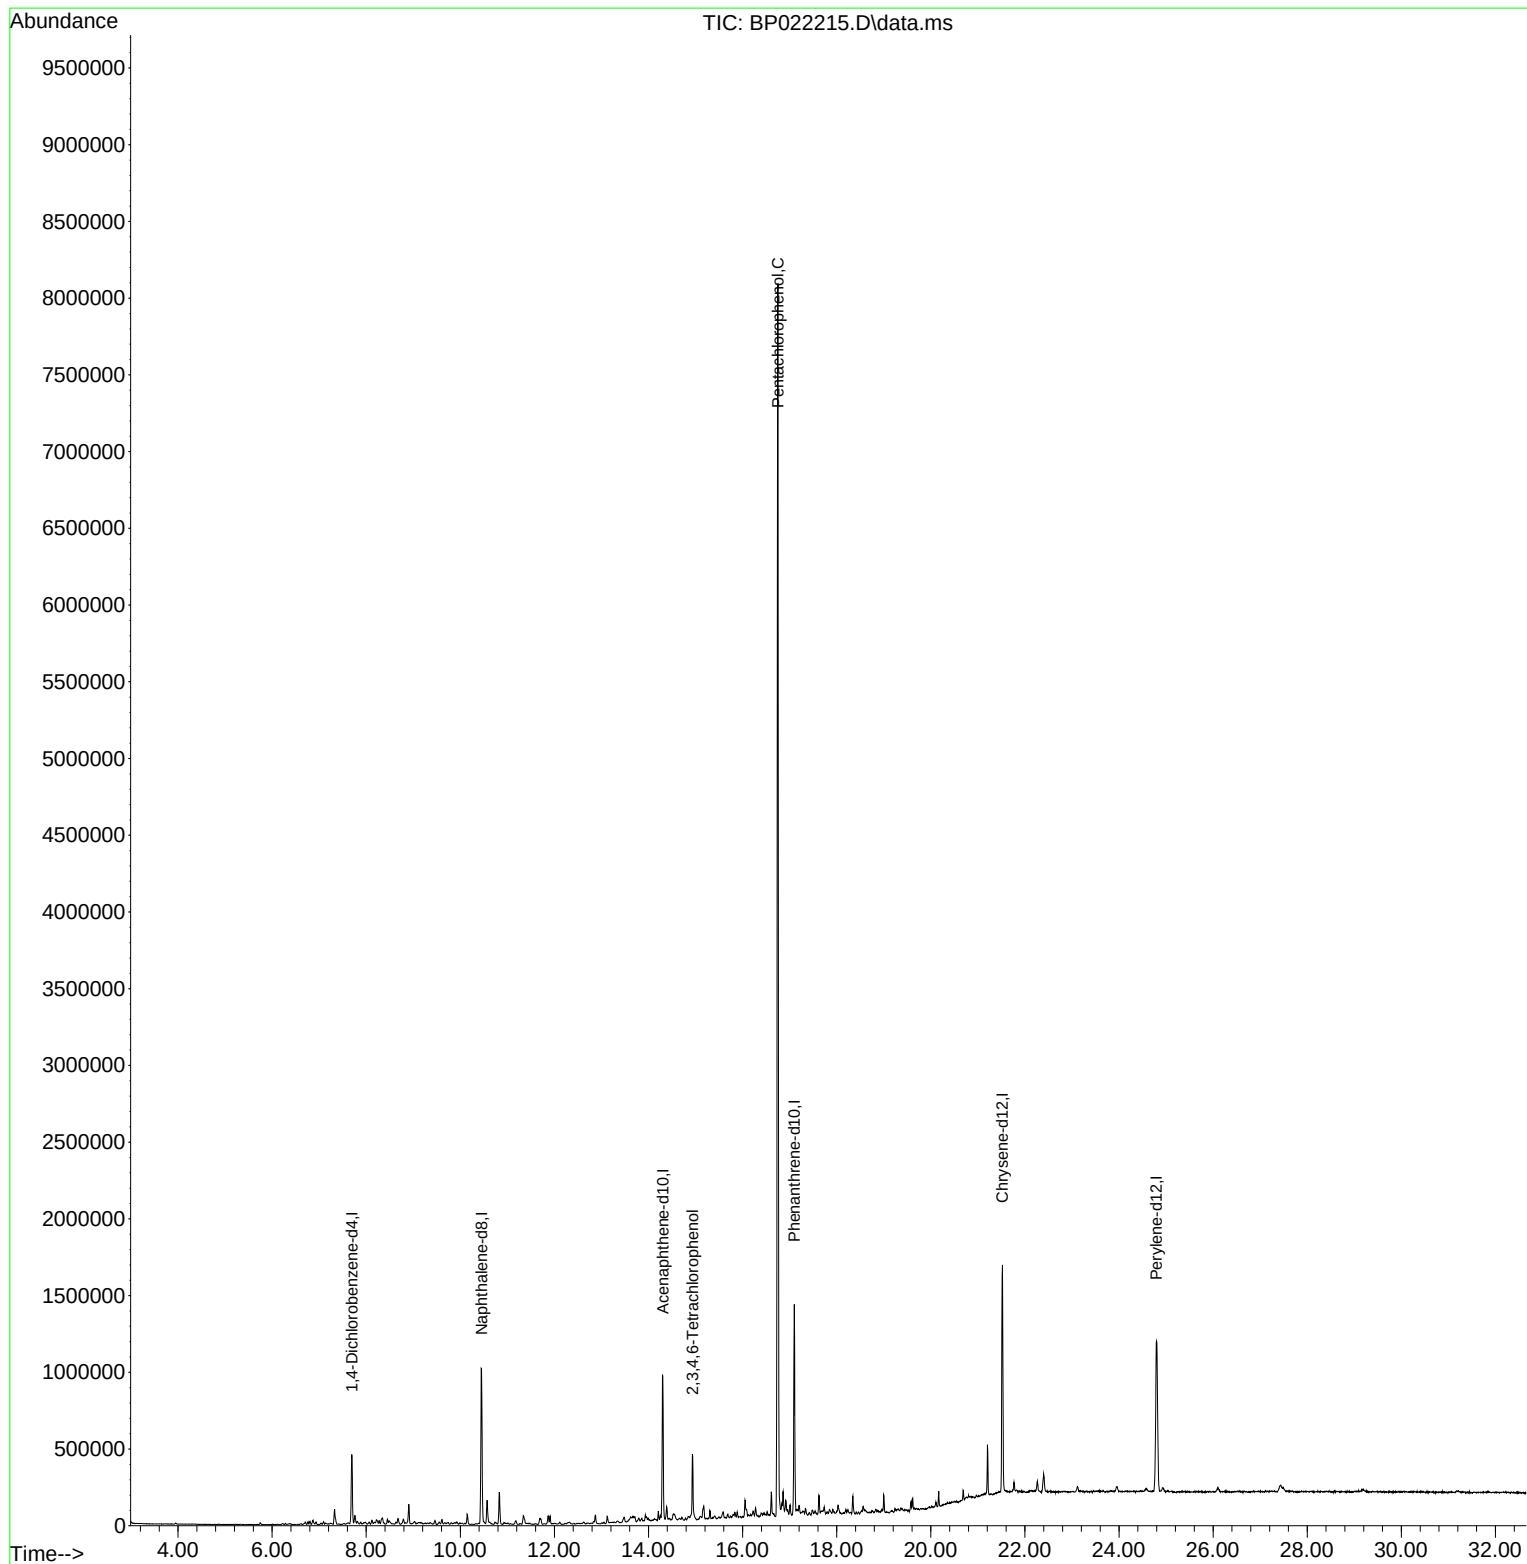


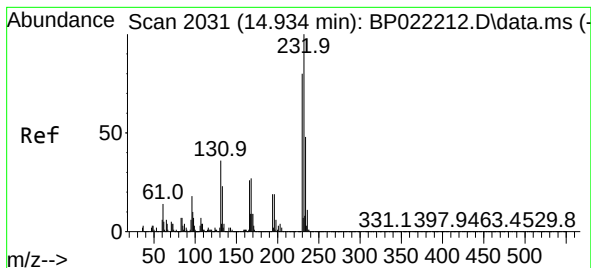

#58
2,3,4,6-Tetrachlorophenol
Concen: 10.096 ng/ul
RT: 14.939 min Scan# 2032
Delta R.T. 0.006 min
Lab File: BP022215.D
Acq: 04 Oct 2024 05:22

Instrument :
BNA_P
ClientSampleId :
DDCD3DL

Tgt Ion:232	Resp:	85219
Ion Ratio	Lower	Upper
232	100	
131	37.4	28.2 42.2
130	2.8	1.8 2.6#
166	25.5	21.8 32.6

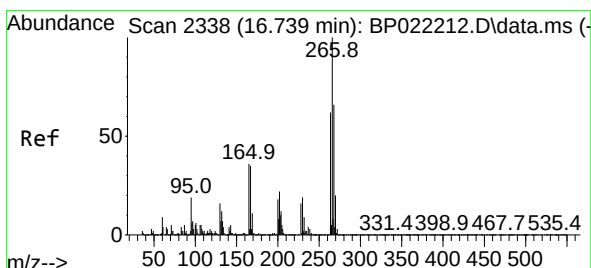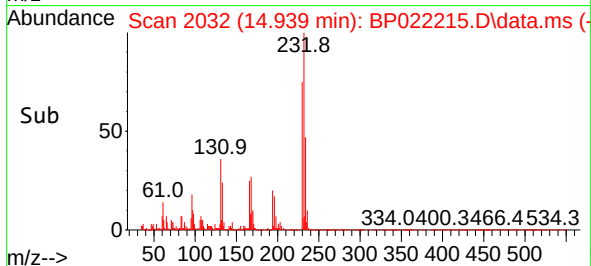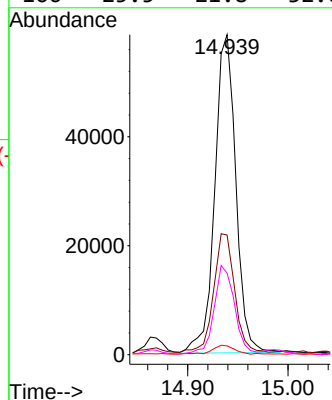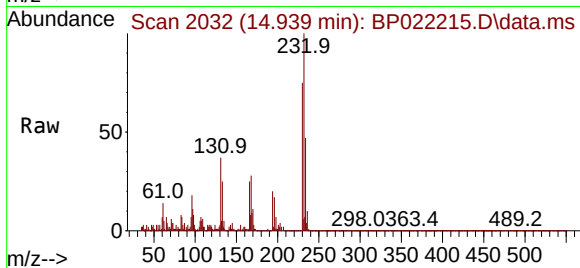

#71
Pentachlorophenol
Concen: 223.487 ng/ul
RT: 16.751 min Scan# 2340
Delta R.T. 0.011 min
Lab File: BP022215.D
Acq: 04 Oct 2024 05:22

Tgt Ion:266	Resp:	1884688
Ion Ratio	Lower	Upper
266	100	
264	61.9	50.2 75.4
268	65.0	51.4 77.0

