

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022158.D
 Acq On : 02 Oct 2024 12:04
 Operator : RC/JU
 Sample : PB163456BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK456

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	34	38	46	rBV	28390	40780	1.01%	0.110%
2	3.628	105	109	128	rBV	366864	562908	13.97%	1.517%
3	3.952	157	164	170	rBV	9316	15338	0.38%	0.041%
4	6.881	653	662	673	rBV	509158	787540	19.55%	2.122%
5	7.034	681	688	699	rBV	386533	584321	14.50%	1.575%
6	7.234	715	722	731	rBV	516332	792247	19.66%	2.135%
7	7.699	792	801	810	rVB	437394	726754	18.04%	1.959%
8	8.399	912	920	930	rBV	596773	982762	24.39%	2.649%
9	8.834	987	994	1007	rBV	458777	798454	19.82%	2.152%
10	9.552	1108	1116	1127	rBV	440972	729094	18.10%	1.965%
11	10.087	1199	1207	1220	rBV	645201	1089232	27.04%	2.936%
12	10.457	1262	1270	1280	rBV	558049	1017362	25.25%	2.742%
13	10.587	1285	1292	1303	rBV	551458	987721	24.52%	2.662%
14	11.252	1399	1405	1409	rBV8	3204	7039	0.17%	0.019%
15	12.034	1533	1538	1545	rVB2	11268	19241	0.48%	0.052%
16	12.546	1619	1625	1626	rBV6	3108	4383	0.11%	0.012%
17	12.557	1626	1627	1634	rVB7	2616	4149	0.10%	0.011%
18	13.657	1809	1814	1816	rBV5	4278	6342	0.16%	0.017%
19	13.710	1816	1823	1833	rVB	1319766	1783513	44.27%	4.807%
20	13.993	1864	1871	1881	rBV	1335914	1942246	48.21%	5.235%
21	14.140	1891	1896	1905	rVB2	11843	25241	0.63%	0.068%
22	14.304	1917	1924	1934	rVB	970801	1558617	38.69%	4.201%
23	14.522	1954	1961	1980	rBV	463314	874530	21.71%	2.357%
24	14.875	2016	2021	2030	rVB3	8220	15972	0.40%	0.043%
25	15.310	2087	2095	2103	rBV	1728249	2540209	63.05%	6.846%
26	15.434	2109	2116	2125	rBV	599717	894986	22.21%	2.412%
27	15.551	2133	2136	2141	rVB5	8754	12242	0.30%	0.033%
28	16.116	2226	2232	2240	rVB6	12829	26198	0.65%	0.071%
29	16.398	2274	2280	2286	rVB10	2600	6693	0.17%	0.018%
30	16.492	2291	2296	2301	rVB9	3181	6980	0.17%	0.019%
31	16.645	2318	2322	2325	rBV5	3476	5285	0.13%	0.014%
32	16.763	2335	2342	2346	rBV9	5929	11542	0.29%	0.031%
33	16.875	2356	2361	2368	rVB3	4581	8043	0.20%	0.022%
34	17.104	2391	2400	2409	rBV	1422347	2093408	51.96%	5.642%
35	17.198	2410	2416	2427	rVB2	2072039	2958287	73.43%	7.973%
36	18.039	2554	2559	2565	rBV3	28751	52417	1.30%	0.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022158.D
Acq On : 02 Oct 2024 12:04
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

37	19.133	2740	2745	2749	rBV	30392	41218	1.02%	0.111%
38	19.198	2753	2756	2760	rVB	23113	31052	0.77%	0.084%
39	19.381	2783	2787	2791	rBV6	19125	31108	0.77%	0.084%
40	19.581	2815	2821	2831	rVB	2660782	3683546	91.43%	9.927%
41	21.539	3148	3154	3162	rVB2	1650676	2620185	65.04%	7.062%
42	24.586	3664	3672	3685	rVB2	1748583	4028853	100.00%	10.858%
43	24.816	3702	3711	3724	rVB	1030730	2696624	66.93%	7.268%




Sum of corrected areas: 37104662

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022158.D
Acq On : 02 Oct 2024 12:04
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

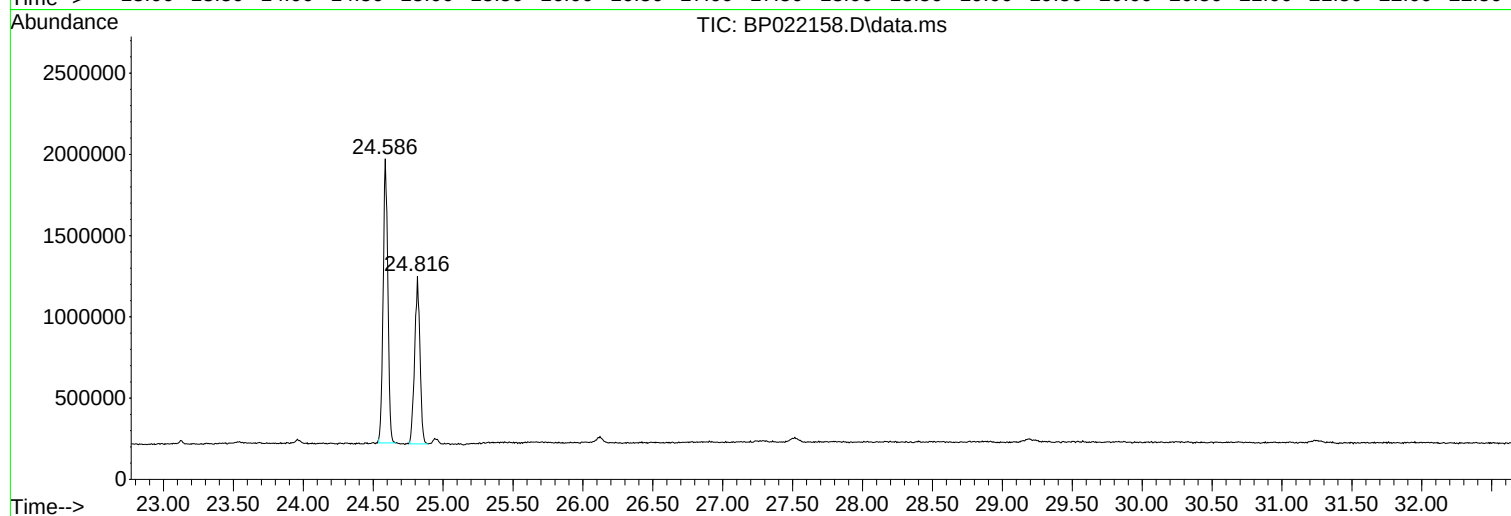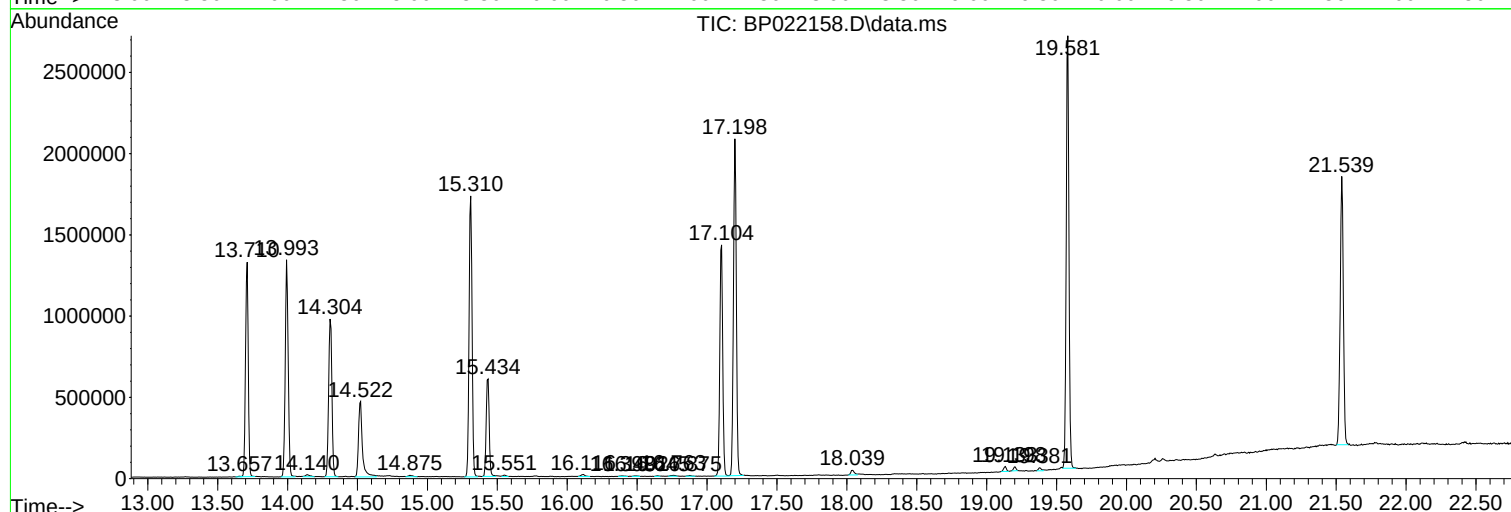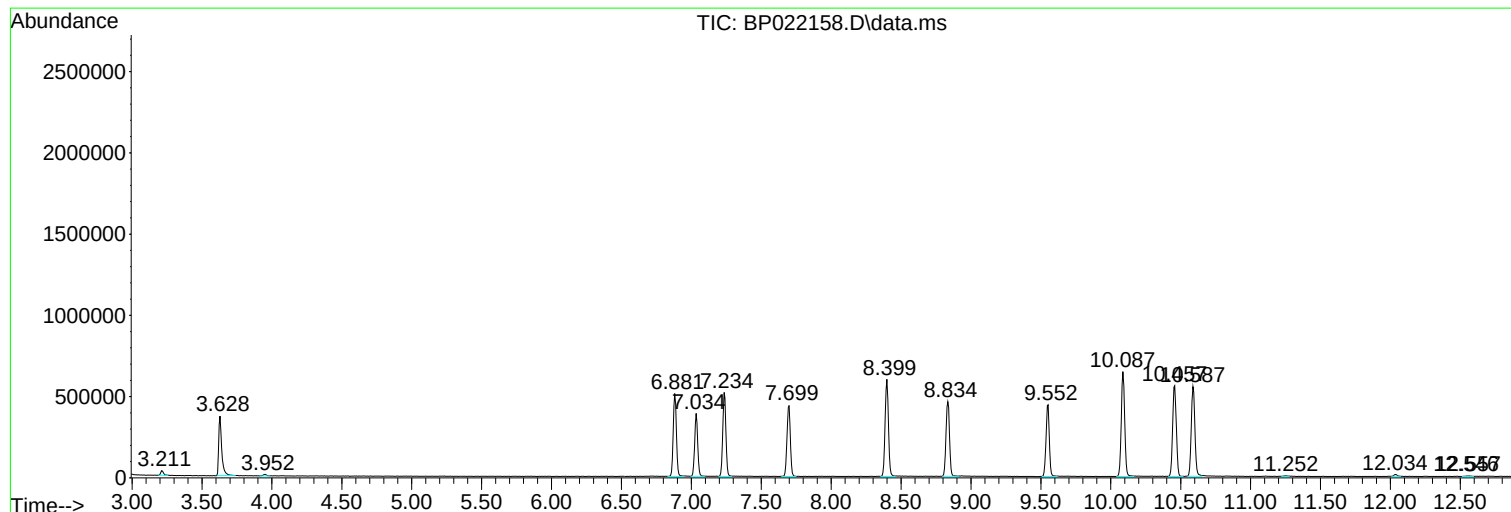

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022158.D
Acq On : 02 Oct 2024 12:04
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022158.D
Acq On : 02 Oct 2024 12:04
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------