

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022185.D
 Acq On : 03 Oct 2024 07:42
 Operator : RC/JU
 Sample : PB163456BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK456

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	49	rVB	25421	41238	1.08%	0.118%
2	3.634	106	110	128	rBV	319263	534107	14.02%	1.526%
3	3.952	160	164	171	rVB	8600	11579	0.30%	0.033%
4	6.881	654	662	675	rBV	442602	755780	19.84%	2.159%
5	7.040	680	689	697	rBV	346622	547139	14.36%	1.563%
6	7.240	715	723	735	rBV	463154	769295	20.19%	2.198%
7	7.699	791	801	810	rBV	421702	696225	18.27%	1.989%
8	8.399	913	920	933	rBV	602786	977567	25.66%	2.793%
9	8.834	982	994	1004	rBV	429951	759470	19.93%	2.170%
10	9.546	1107	1115	1129	rBV	380534	682315	17.91%	1.949%
11	10.081	1196	1206	1223	rBV	622749	1098402	28.83%	3.138%
12	10.457	1262	1270	1278	rBV	560378	984370	25.84%	2.812%
13	10.587	1283	1292	1311	rBV	582009	1002052	26.30%	2.863%
14	12.040	1533	1539	1546	rBV3	11037	18311	0.48%	0.052%
15	13.710	1815	1823	1836	rBV	1237648	1696101	44.52%	4.845%
16	13.992	1864	1871	1888	rBV2	1286394	1924275	50.50%	5.497%
17	14.157	1893	1899	1910	rVV8	5250	12652	0.33%	0.036%
18	14.304	1916	1924	1936	rVB	947246	1486133	39.00%	4.245%
19	14.522	1954	1961	1984	rBV	409346	794566	20.85%	2.270%
20	14.669	1984	1986	1990	rVV5	3645	4751	0.12%	0.014%
21	15.310	2088	2095	2109	rBV	1624891	2479415	65.07%	7.083%
22	15.439	2111	2117	2126	rBV	426884	617998	16.22%	1.765%
23	15.557	2133	2137	2149	rVB5	10144	20761	0.54%	0.059%
24	15.892	2191	2194	2200	rVB8	3292	5769	0.15%	0.016%
25	16.122	2228	2233	2237	rBV7	3928	6784	0.18%	0.019%
26	16.757	2336	2341	2343	rBV7	7651	12039	0.32%	0.034%
27	16.886	2359	2363	2366	rBV	3273	4780	0.13%	0.014%
28	17.104	2394	2400	2410	rBV	1285327	1953149	51.26%	5.579%
29	17.210	2411	2418	2429	rVV	2081904	2833929	74.38%	8.096%
30	17.804	2517	2519	2523	rVB4	3894	4578	0.12%	0.013%
31	17.957	2543	2545	2549	rBV5	2504	3870	0.10%	0.011%
32	18.033	2556	2558	2566	rVB8	8992	14599	0.38%	0.042%
33	19.128	2740	2744	2750	rVB2	26253	36599	0.96%	0.105%
34	19.204	2754	2757	2763	rVB2	21537	33632	0.88%	0.096%
35	19.586	2815	2822	2830	rBV2	2360676	3533701	92.74%	10.095%
36	21.539	3148	3154	3167	rVB	1487142	2369100	62.18%	6.768%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022185.D
Acq On : 03 Oct 2024 07:42
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

37	24.592	3663	3673	3687	rVB2	1393804	3810171	100.00%	10.884%
38	24.821	3703	3712	3722	rVB	945381	2468665	64.79%	7.052%




Sum of corrected areas: 35005867

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022185.D
Acq On : 03 Oct 2024 07:42
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

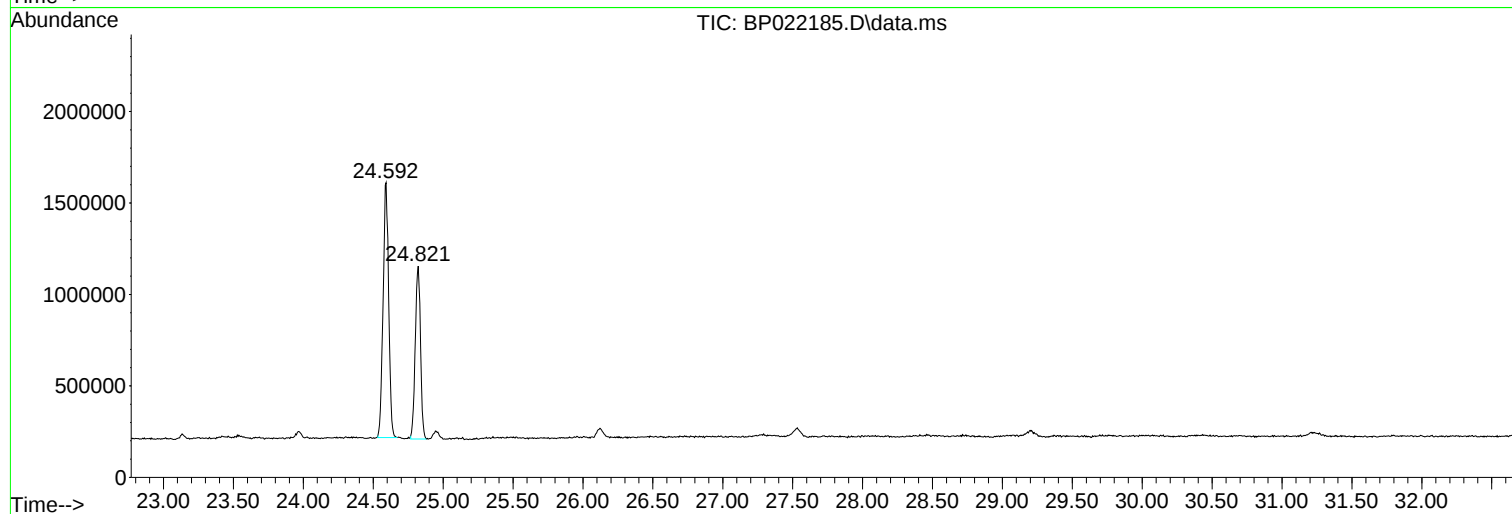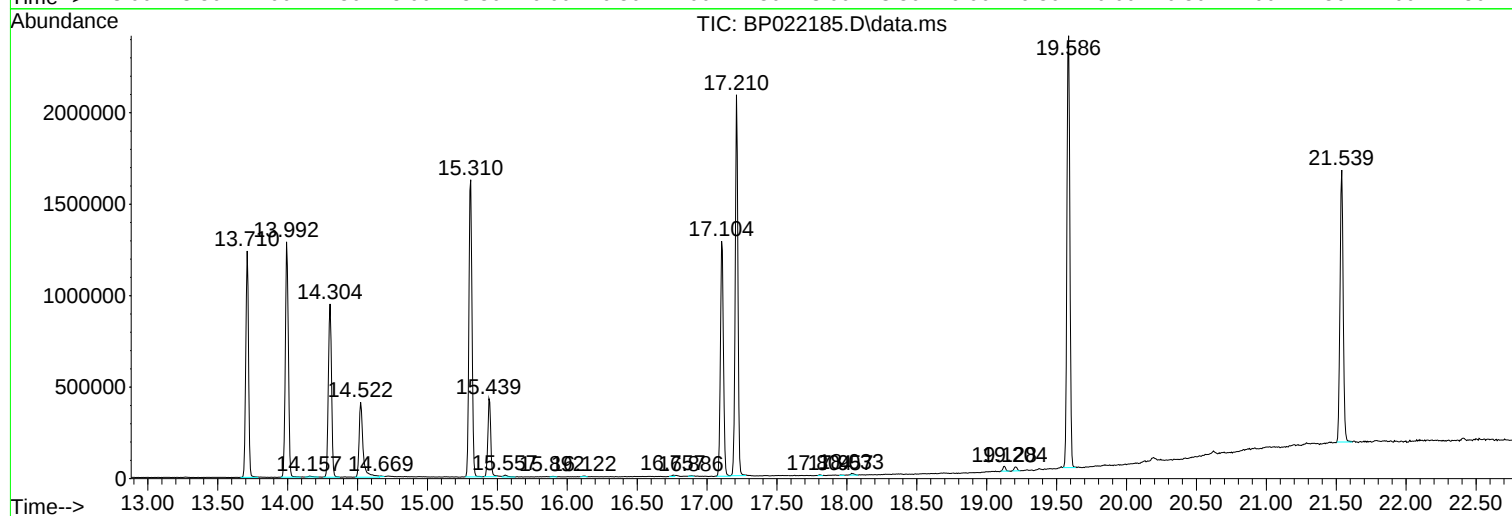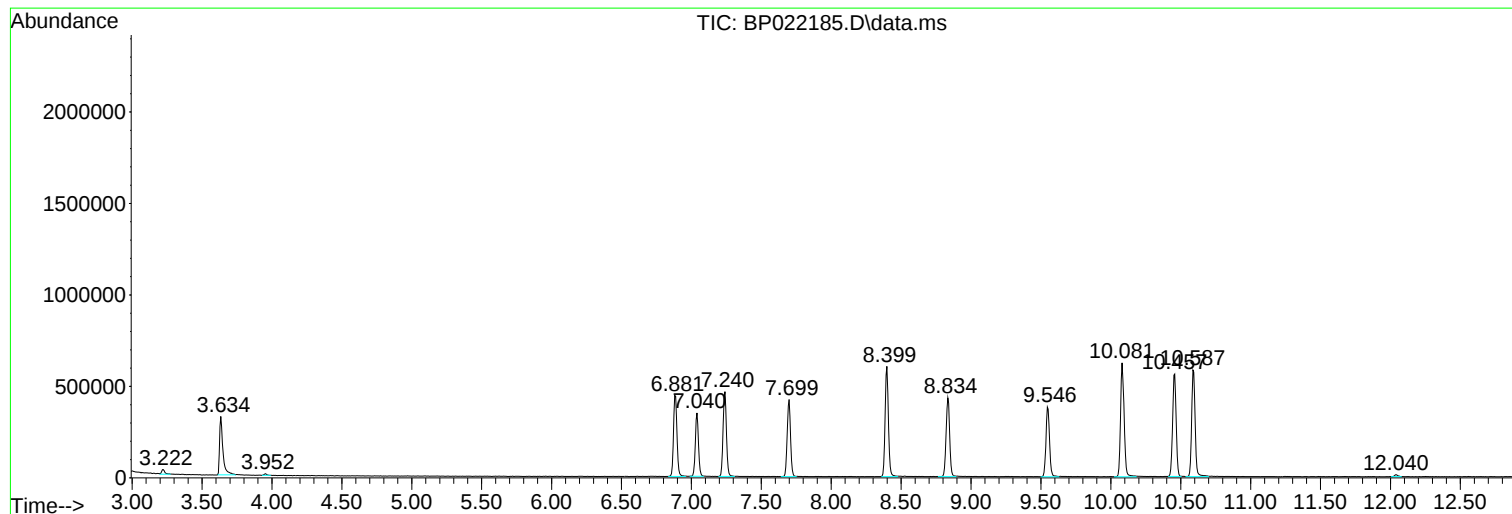

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022185.D
Acq On : 03 Oct 2024 07:42
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022185.D
Acq On : 03 Oct 2024 07:42
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------