

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022198.D
 Acq On : 03 Oct 2024 17:11
 Operator : RC/JU
 Sample : PB163456BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK456

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	35	39	48	rVB	27012	37553	1.05%	0.116%
2	3.628	105	109	130	rBV	318522	509586	14.22%	1.581%
3	3.952	159	164	170	rVB	10523	15635	0.44%	0.049%
4	4.181	198	203	207	rVB8	2635	3699	0.10%	0.011%
5	6.881	654	662	675	rBV	418725	687096	19.17%	2.131%
6	7.034	681	688	697	rVB	310650	504881	14.09%	1.566%
7	7.234	714	722	733	rBV	452232	712341	19.87%	2.210%
8	7.693	790	800	810	rBV	396547	646857	18.05%	2.007%
9	8.393	911	919	937	rBV	524037	872978	24.36%	2.708%
10	8.834	987	994	1004	rBV	416362	684060	19.09%	2.122%
11	9.552	1107	1116	1128	rBV	353322	626851	17.49%	1.945%
12	10.087	1198	1207	1217	rBV	559187	975531	27.22%	3.026%
13	10.451	1261	1269	1280	rBV	521413	883950	24.66%	2.742%
14	10.587	1284	1292	1304	rBV	519859	875156	24.42%	2.715%
15	12.040	1534	1539	1549	rVB3	8194	17692	0.49%	0.055%
16	13.704	1815	1822	1838	rBV	1123878	1562971	43.61%	4.849%
17	13.987	1863	1870	1881	rBV	1147383	1721881	48.04%	5.341%
18	14.298	1915	1923	1936	rBV	821776	1356631	37.85%	4.208%
19	14.522	1954	1961	1975	rBV	340092	703575	19.63%	2.183%
20	15.304	2087	2094	2109	rBV	1585558	2274892	63.47%	7.057%
21	15.434	2109	2116	2132	rVV	395908	624229	17.42%	1.936%
22	15.557	2132	2137	2142	rVB6	6672	11633	0.32%	0.036%
23	15.892	2189	2194	2199	rBV9	1973	5352	0.15%	0.017%
24	16.098	2225	2229	2235	rBV8	3343	5848	0.16%	0.018%
25	16.751	2335	2340	2349	rVB9	9347	21416	0.60%	0.066%
26	16.886	2360	2363	2367	rBV4	2669	3753	0.10%	0.012%
27	17.098	2392	2399	2409	rBV	1331628	1817479	50.71%	5.638%
28	17.210	2409	2418	2430	rBV	1608735	2604483	72.67%	8.079%
29	18.039	2555	2559	2563	rBV6	8204	12339	0.34%	0.038%
30	19.133	2741	2745	2749	rVB2	25054	33979	0.95%	0.105%
31	19.204	2753	2757	2761	rBV	22704	29700	0.83%	0.092%
32	19.580	2815	2821	2832	rBV	2168852	3264005	91.07%	10.125%
33	21.539	3148	3154	3165	rVB	1444551	2192858	61.18%	6.802%
34	24.586	3662	3672	3684	rVB	1377537	3584128	100.00%	11.118%
35	24.804	3700	3709	3723	rVB3	750427	2351152	65.60%	7.294%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022198.D
Acq On : 03 Oct 2024 17:11
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 32236170

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022198.D
Acq On : 03 Oct 2024 17:11
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

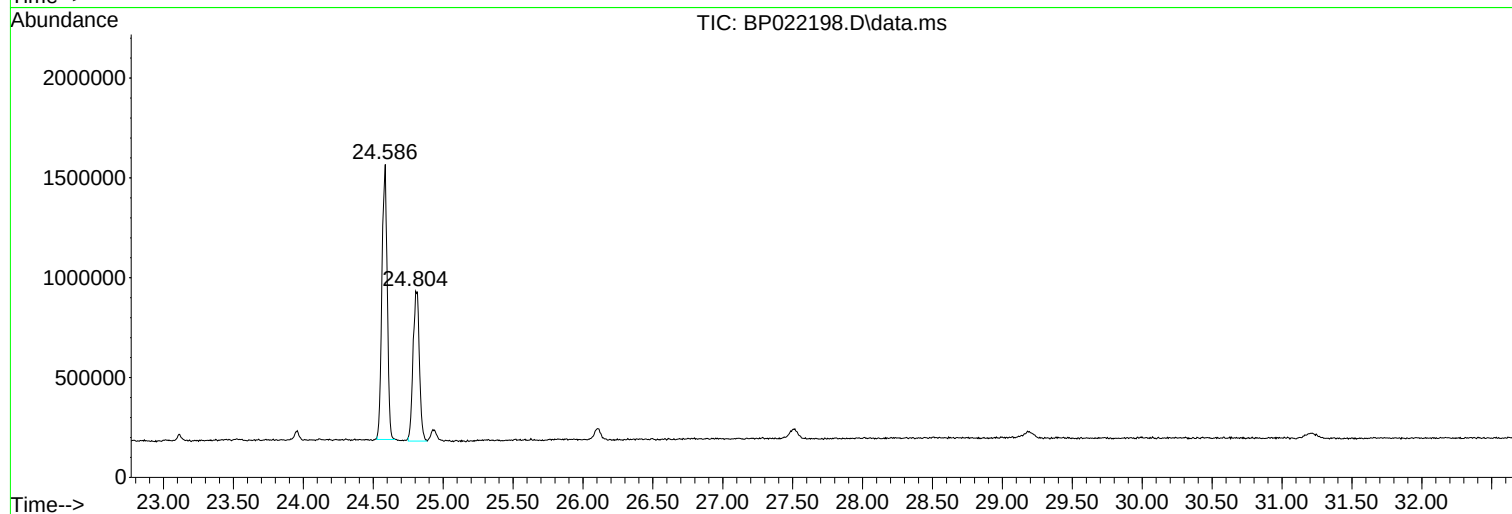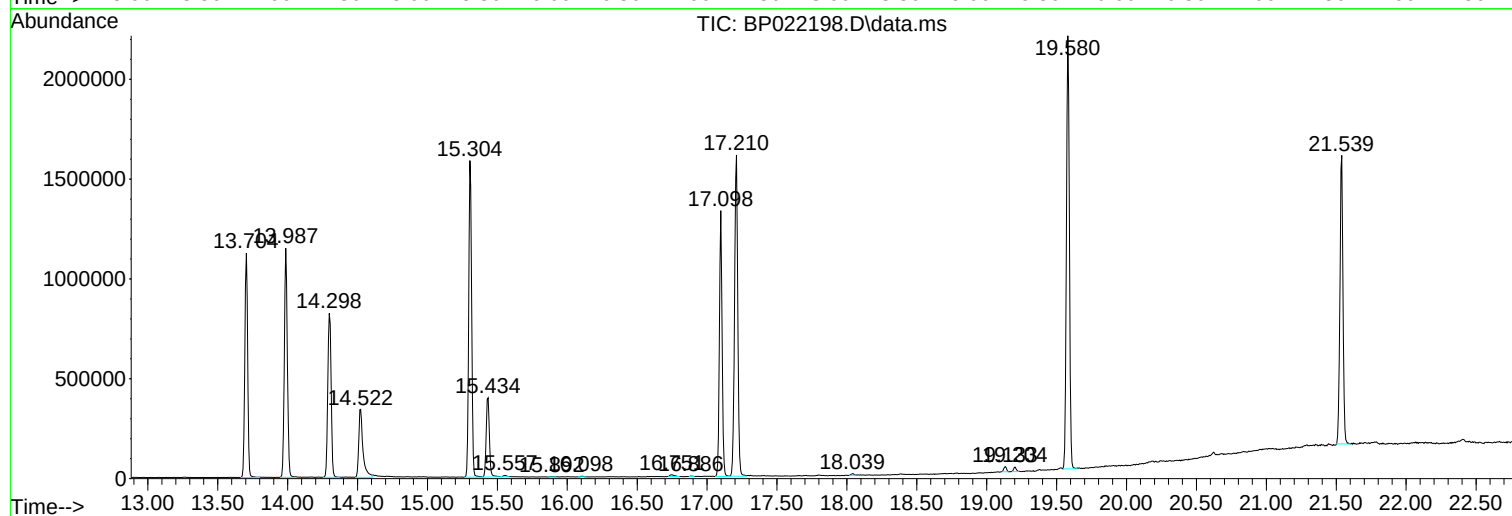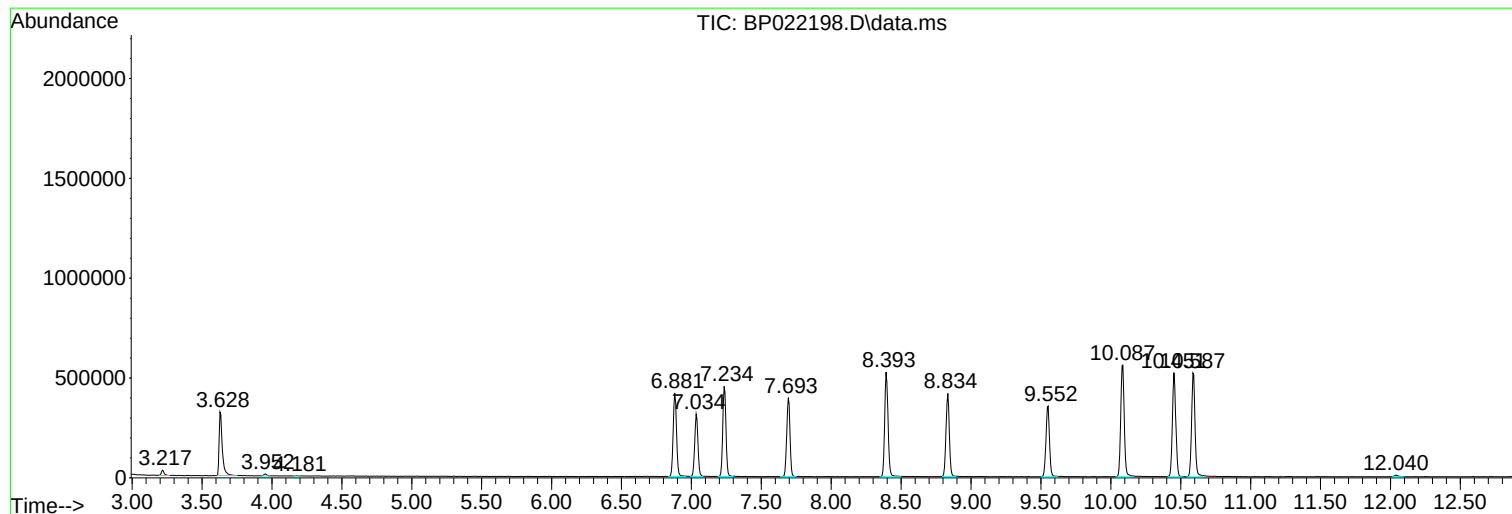

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022198.D
Acq On : 03 Oct 2024 17:11
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022198.D
Acq On : 03 Oct 2024 17:11
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------