

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022216.D
 Acq On : 04 Oct 2024 06:02
 Operator : RC/JU
 Sample : P4017-17DL2 30X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DD3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.958	161	165	167	rBV3	5240	6847	0.18%	0.048%
2	5.746	466	469	477	rVB9	4704	8192	0.22%	0.057%
3	6.763	637	642	645	rVV5	4334	7185	0.19%	0.050%
4	6.805	645	649	653	rVV	6655	9772	0.26%	0.068%
5	6.869	653	660	666	rVV6	9619	18357	0.49%	0.128%
6	6.928	668	670	677	rVB4	5310	8110	0.22%	0.056%
7	7.093	692	698	702	rBV3	5911	9151	0.25%	0.064%
8	7.328	732	738	748	rVB2	30067	55461	1.49%	0.385%
9	7.693	791	800	807	rBV	378887	612772	16.49%	4.258%
10	7.763	807	812	817	rVV3	16021	31527	0.85%	0.219%
11	7.805	817	819	827	rVB4	5352	9339	0.25%	0.065%
12	7.881	827	832	837	rVB8	3276	6106	0.16%	0.042%
13	8.063	857	863	867	rVB6	4968	8333	0.22%	0.058%
14	8.116	867	872	878	rBV3	7914	14395	0.39%	0.100%
15	8.222	886	890	896	rVV4	5761	12528	0.34%	0.087%
16	8.275	896	899	903	rVB4	5404	7074	0.19%	0.049%
17	8.340	903	910	915	rBV6	11165	26193	0.71%	0.182%
18	8.452	924	929	932	rBV2	9550	16410	0.44%	0.114%
19	8.487	932	935	939	rVB3	3538	5987	0.16%	0.042%
20	8.675	963	967	974	rVB5	11578	21082	0.57%	0.146%
21	8.787	977	986	993	rBV7	8558	22382	0.60%	0.156%
22	8.905	999	1006	1012	rVB	37239	61439	1.65%	0.427%
23	9.022	1018	1026	1027	rBV8	4325	8267	0.22%	0.057%
24	9.463	1091	1101	1110	rVB6	8411	16697	0.45%	0.116%
25	9.552	1110	1116	1120	rBV7	3824	9499	0.26%	0.066%
26	9.604	1120	1125	1129	rVB6	7707	12670	0.34%	0.088%
27	9.922	1177	1179	1184	rVB6	4370	6466	0.17%	0.045%
28	10.152	1212	1218	1227	rVB3	19832	34139	0.92%	0.237%
29	10.452	1260	1269	1282	rBV	609330	1057478	28.46%	7.348%
30	10.563	1282	1288	1296	rVV4	39086	81387	2.19%	0.565%
31	10.622	1296	1298	1305	rVB5	4574	7537	0.20%	0.052%
32	10.740	1313	1318	1321	rBV6	4191	7516	0.20%	0.052%
33	10.828	1327	1333	1346	rVB	62714	105108	2.83%	0.730%
34	11.181	1382	1393	1398	rBV7	7029	16159	0.43%	0.112%
35	11.340	1413	1420	1430	rBV7	15953	41560	1.12%	0.289%
36	11.693	1473	1480	1481	rBV4	9758	16916	0.46%	0.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022216.D
 Acq On : 04 Oct 2024 06:02
 Operator : RC/JU
 Sample : P4017-17DL2 30X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DD3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	11.869	1502	1510	1513	rBV4	17169	29647	0.80%	0.206%
38	11.904	1513	1516	1522	rVV3	13056	20793	0.56%	0.144%
39	12.110	1548	1551	1563	rVB8	4146	8399	0.23%	0.058%
40	12.328	1585	1588	1597	rVB7	3812	7000	0.19%	0.049%
41	12.487	1606	1615	1618	rBV10	2307	6191	0.17%	0.043%
42	12.834	1669	1674	1675	rVV5	4963	5945	0.16%	0.041%
43	12.869	1676	1680	1687	rVB	15791	25006	0.67%	0.174%
44	13.051	1707	1711	1716	rVB8	4181	6577	0.18%	0.046%
45	13.128	1718	1724	1731	rBV7	11267	23575	0.63%	0.164%
46	13.340	1756	1760	1766	rBV8	4482	9444	0.25%	0.066%
47	13.487	1773	1785	1791	rBV8	10856	29883	0.80%	0.208%
48	13.628	1797	1809	1812	rBV10	9010	25359	0.68%	0.176%
49	13.681	1814	1818	1820	rVV5	9041	17077	0.46%	0.119%
50	13.704	1820	1822	1828	rVB	10216	18128	0.49%	0.126%
51	13.793	1830	1837	1842	rBV10	7382	15672	0.42%	0.109%
52	13.857	1842	1848	1852	rVB9	4422	8154	0.22%	0.057%
53	13.934	1857	1861	1863	rBV4	8753	10515	0.28%	0.073%
54	13.957	1863	1865	1869	rVV5	7196	8153	0.22%	0.057%
55	14.210	1904	1908	1911	rBV	15183	19085	0.51%	0.133%
56	14.251	1911	1915	1917	rVV5	7070	9986	0.27%	0.069%
57	14.304	1917	1924	1934	rVV	829755	1235240	33.25%	8.583%
58	14.392	1934	1939	1944	rVV3	24587	42871	1.15%	0.298%
59	14.522	1956	1961	1962	rBV5	8889	12955	0.35%	0.090%
60	14.716	1990	1994	1998	rBV6	7679	10277	0.28%	0.071%
61	14.834	2010	2014	2015	rBV4	5168	6975	0.19%	0.048%
62	14.892	2021	2024	2026	rBV4	4517	6602	0.18%	0.046%
63	14.945	2027	2033	2048	rVB2	91098	180355	4.85%	1.253%
64	15.110	2056	2061	2065	rBV7	5169	14051	0.38%	0.098%
65	15.151	2065	2068	2069	rVV3	18853	19524	0.53%	0.136%
66	15.169	2069	2071	2077	rVB2	26765	33002	0.89%	0.229%
67	15.310	2091	2095	2099	rBV2	15033	21502	0.58%	0.149%
68	15.381	2099	2107	2110	rBV10	3732	11436	0.31%	0.079%
69	15.410	2110	2112	2118	rVB6	6198	10917	0.29%	0.076%
70	15.587	2136	2142	2148	rVB4	10801	23029	0.62%	0.160%
71	15.687	2156	2159	2164	rBV6	6701	10586	0.28%	0.074%
72	15.745	2167	2169	2174	rVV5	5673	9203	0.25%	0.064%
73	15.798	2174	2178	2179	rVV4	9433	11610	0.31%	0.081%
74	15.834	2182	2184	2189	rVV6	11728	18751	0.50%	0.130%
75	15.887	2189	2193	2197	rVB3	12419	17774	0.48%	0.123%
76	16.063	2218	2223	2225	rBV2	32761	45548	1.23%	0.316%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
 Data File : BP022216.D
 Acq On : 04 Oct 2024 06:02
 Operator : RC/JU
 Sample : P4017-17DL2 30X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DD CD3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

77	16.216	2247	2249	2255	rVB7	9297	15081	0.41%	0.105%
78	16.281	2256	2260	2265	rVB7	13855	21604	0.58%	0.150%
79	16.410	2278	2282	2285	rBV5	6360	9885	0.27%	0.069%
80	16.610	2312	2316	2321	rBV2	37664	55167	1.48%	0.383%
81	16.757	2332	2341	2351	rBV	2266403	3715231	100.00%	25.814%
82	16.863	2357	2359	2366	rVB2	34230	43125	1.16%	0.300%
83	16.922	2366	2369	2374	rVB2	19742	24840	0.67%	0.173%
84	17.016	2380	2385	2390	rVB2	21208	33873	0.91%	0.235%
85	17.104	2392	2400	2410	rBV	889718	1613065	43.42%	11.208%
86	17.204	2415	2417	2425	rVB	19481	30354	0.82%	0.211%
87	17.339	2438	2440	2448	rVB9	10711	22273	0.60%	0.155%
88	17.428	2451	2455	2460	rVB8	4601	7465	0.20%	0.052%
89	17.492	2462	2466	2471	rVV8	8485	13459	0.36%	0.094%
90	17.628	2485	2489	2493	rBV	31218	40583	1.09%	0.282%
91	17.745	2505	2509	2513	rVB7	11874	17364	0.47%	0.121%
92	17.857	2524	2528	2529	rBV4	8027	9994	0.27%	0.069%
93	18.033	2555	2558	2565	rVB8	12891	25199	0.68%	0.175%
94	18.345	2607	2611	2619	rVB	33288	47135	1.27%	0.328%
95	19.004	2719	2723	2729	rVB3	27427	39841	1.07%	0.277%
96	19.616	2824	2827	2830	rVB3	20103	20539	0.55%	0.143%
97	20.169	2919	2921	2925	rVB4	23397	23183	0.62%	0.161%
98	21.210	3095	3098	3106	rVB4	65751	90613	2.44%	0.630%
99	21.527	3147	3152	3161	rBV2	1119724	1932876	52.03%	13.430%
100	24.815	3703	3711	3724	rVB	801633	2092594	56.32%	14.540%




Sum of corrected areas: 14392181

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022216.D
Acq On : 04 Oct 2024 06:02
Operator : RC/JU
Sample : P4017-17DL2 30X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCD3DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

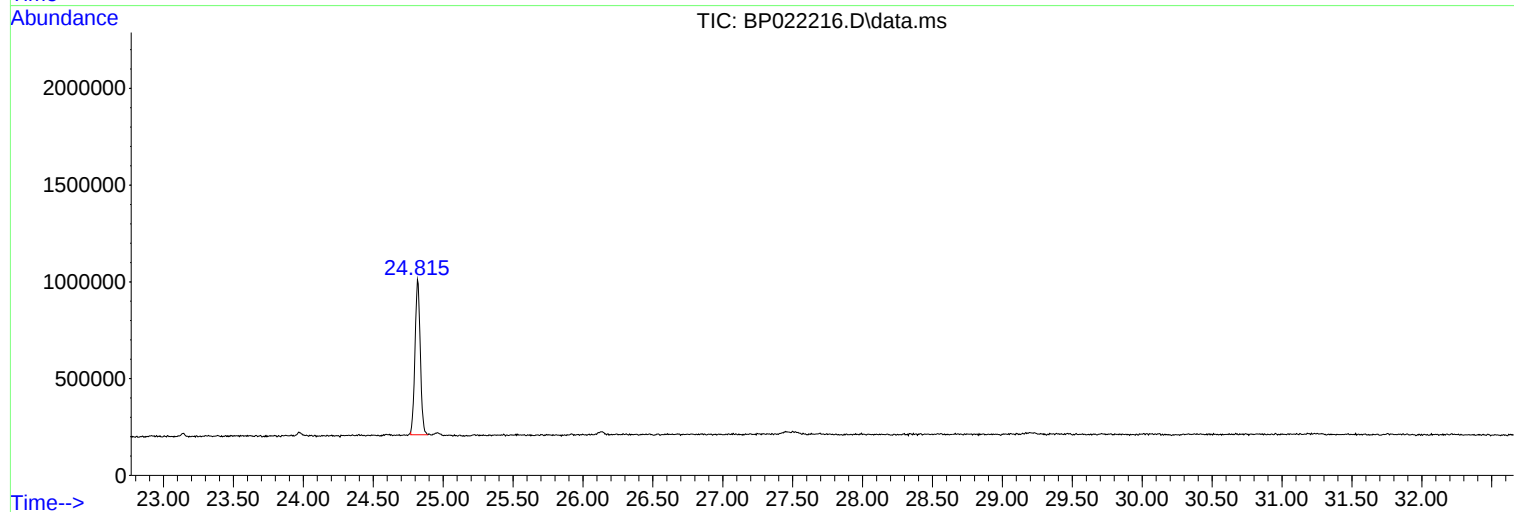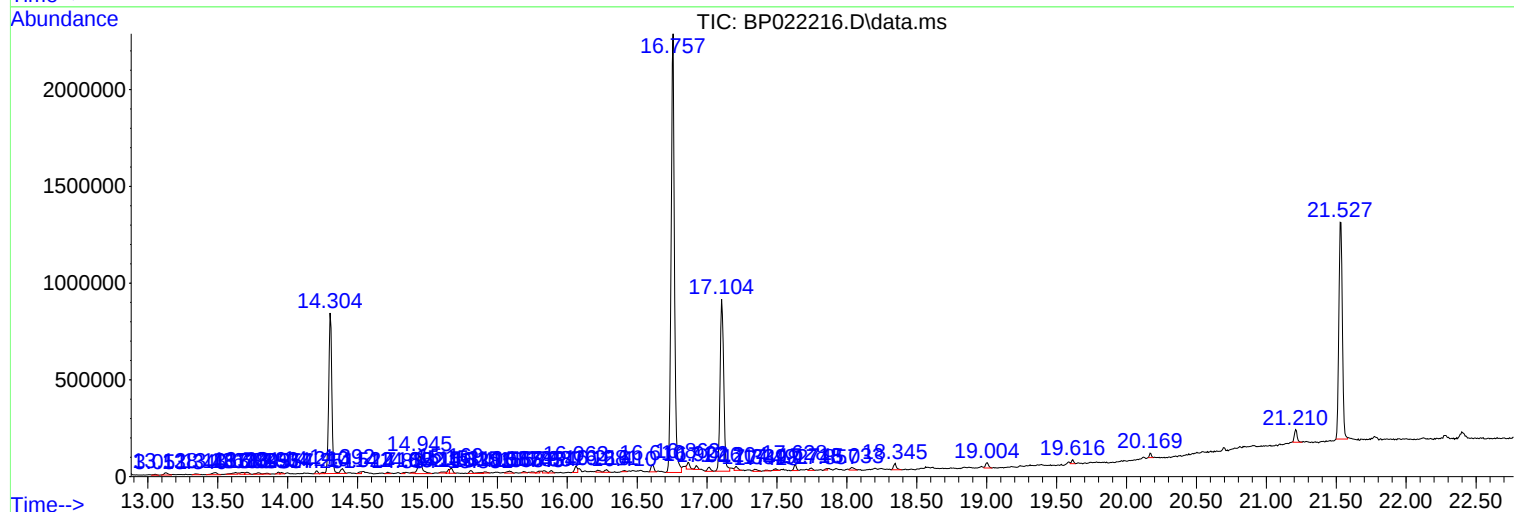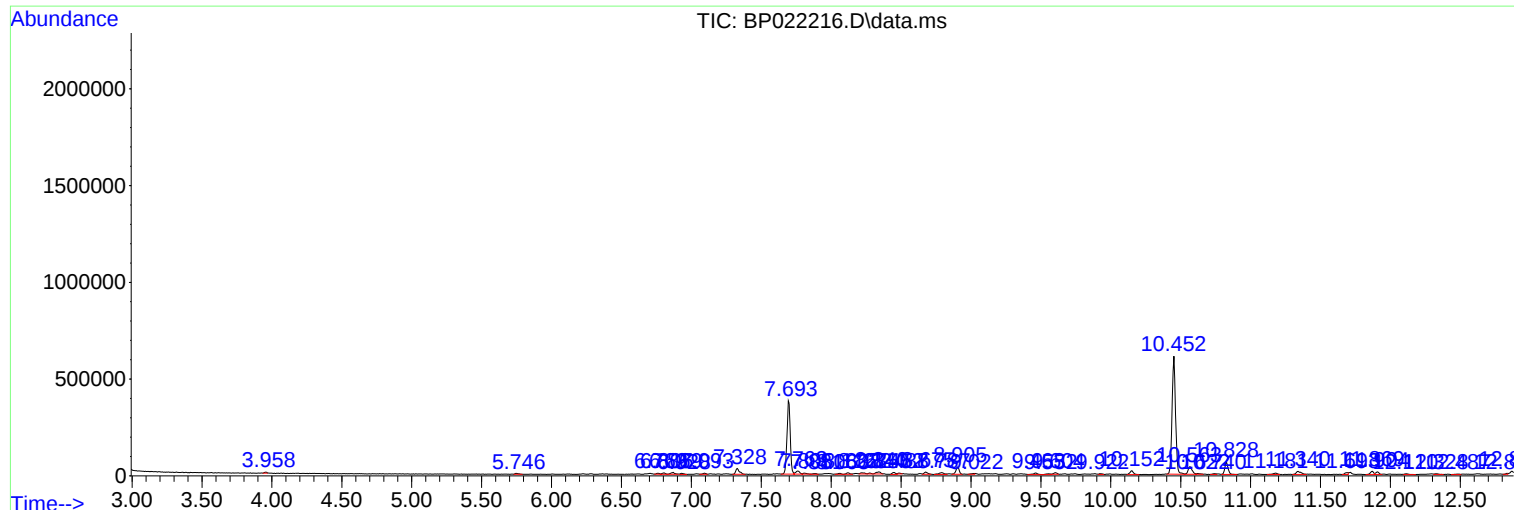

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022216.D
Acq On : 04 Oct 2024 06:02
Operator : RC/JU
Sample : P4017-17DL2 30X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCD3DL2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.905	2.01 ng/ul	61439	1,4-Dichlorobenzene-d4	7.699

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetradecane	198	C14H30	000629-59-4	87
2			Hexadecane	226	C16H34	000544-76-3	80
3			Undecane	156	C11H24	001120-21-4	80
4			Tetradecane	198	C14H30	000629-59-4	72
5			Nonane, 3,7-dimethyl-	156	C11H24	017302-32-8	72

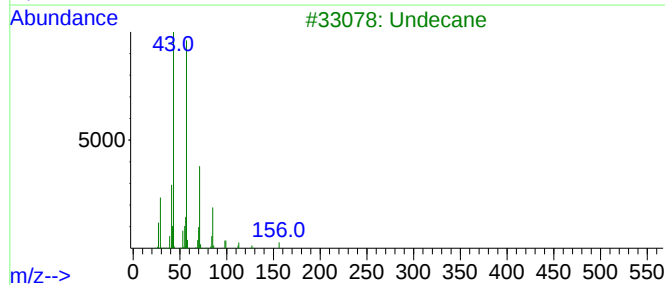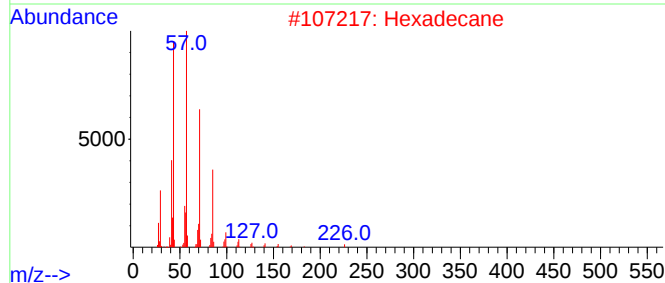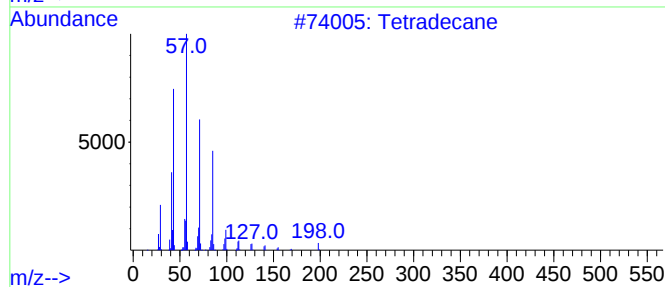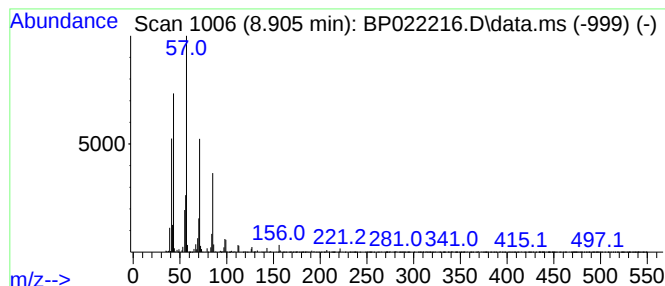

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100224\
Data File : BP022216.D
Acq On : 04 Oct 2024 06:02
Operator : RC/JU
Sample : P4017-17DL2 30X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCD3DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	8.905	2.0	ng/u1	61439	1	7.699	612772	20.0