
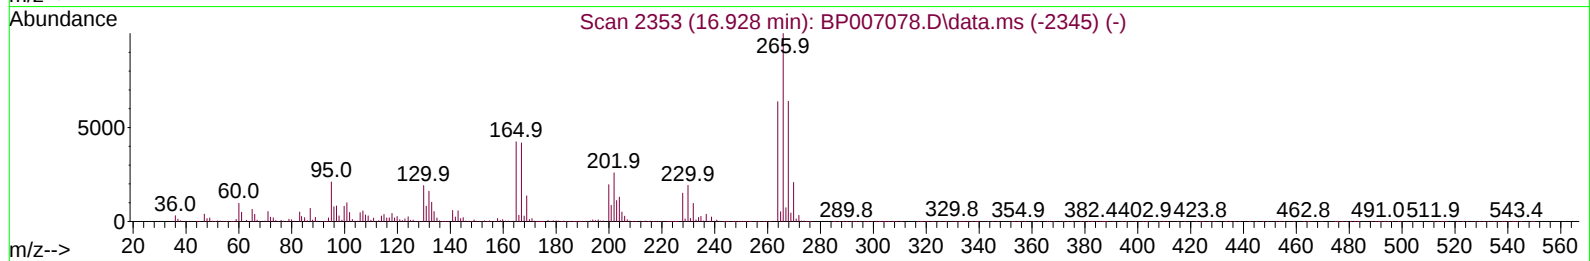
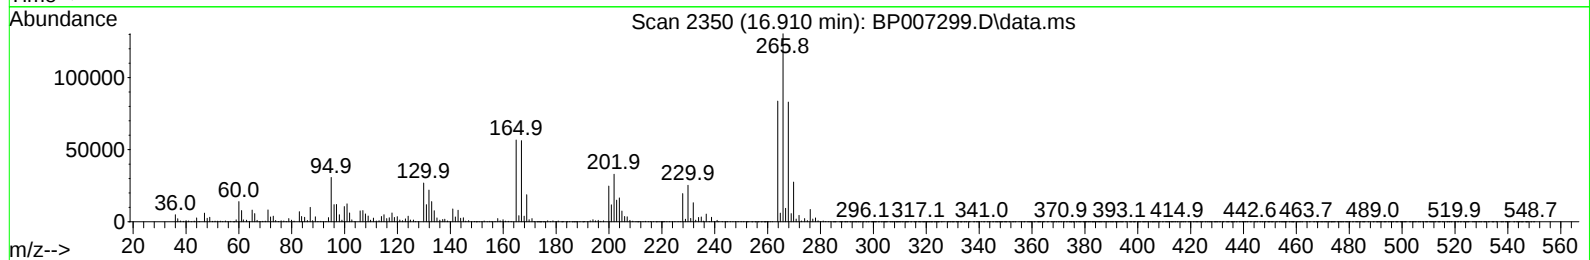


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
Data File : BP007299.D
Acq On : 04 Oct 2021 10:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 13:24:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 12:49:05 2021
Response via : Initial Calibration

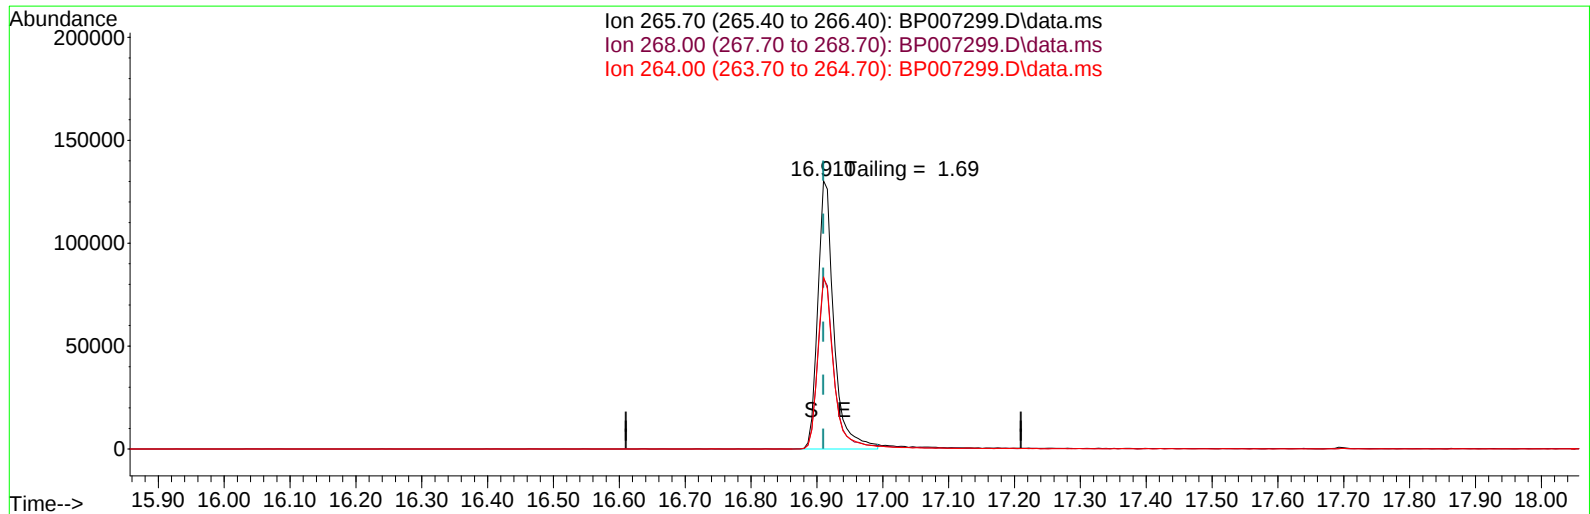

TIC: BP007299.D\data.ms

(70) Pentachlorophenol (C)




16.910min (+ 0.000) 342705.19 ng

response 226859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.63
264.00	62.90	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
 Data File : BP007299.D
 Acq On : 04 Oct 2021 10:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 13:24:06 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 01 12:49:05 2021
 Response via : Initial Calibration

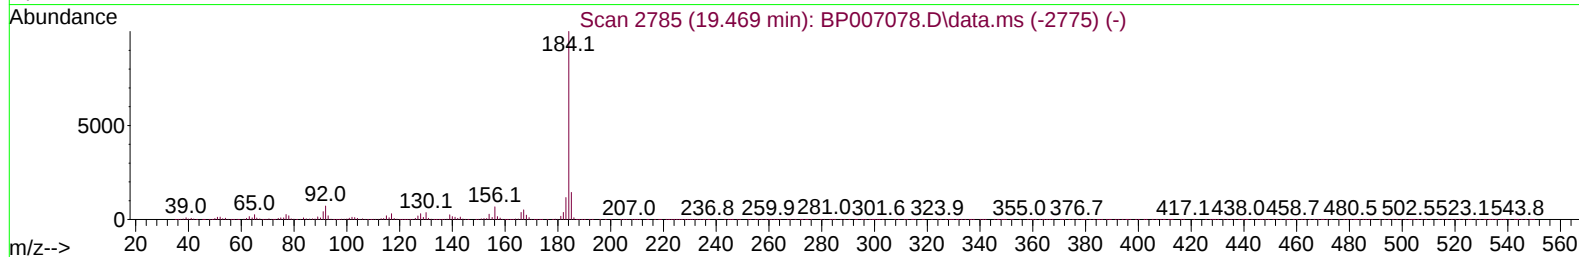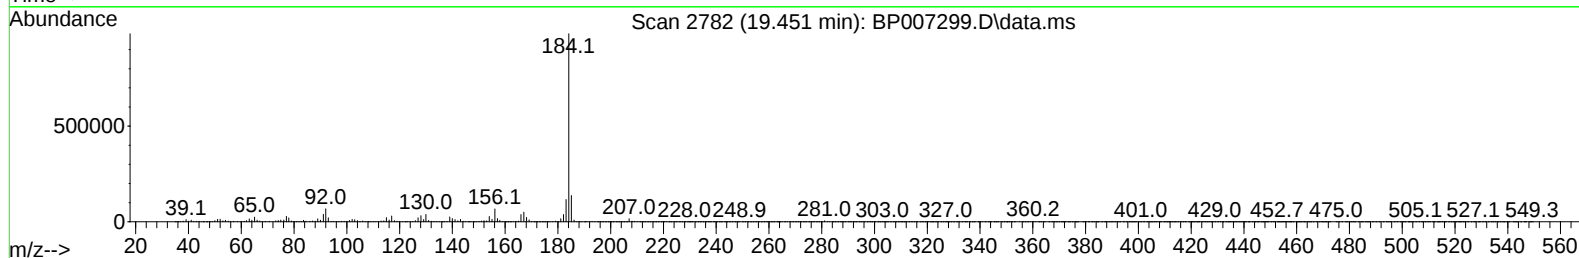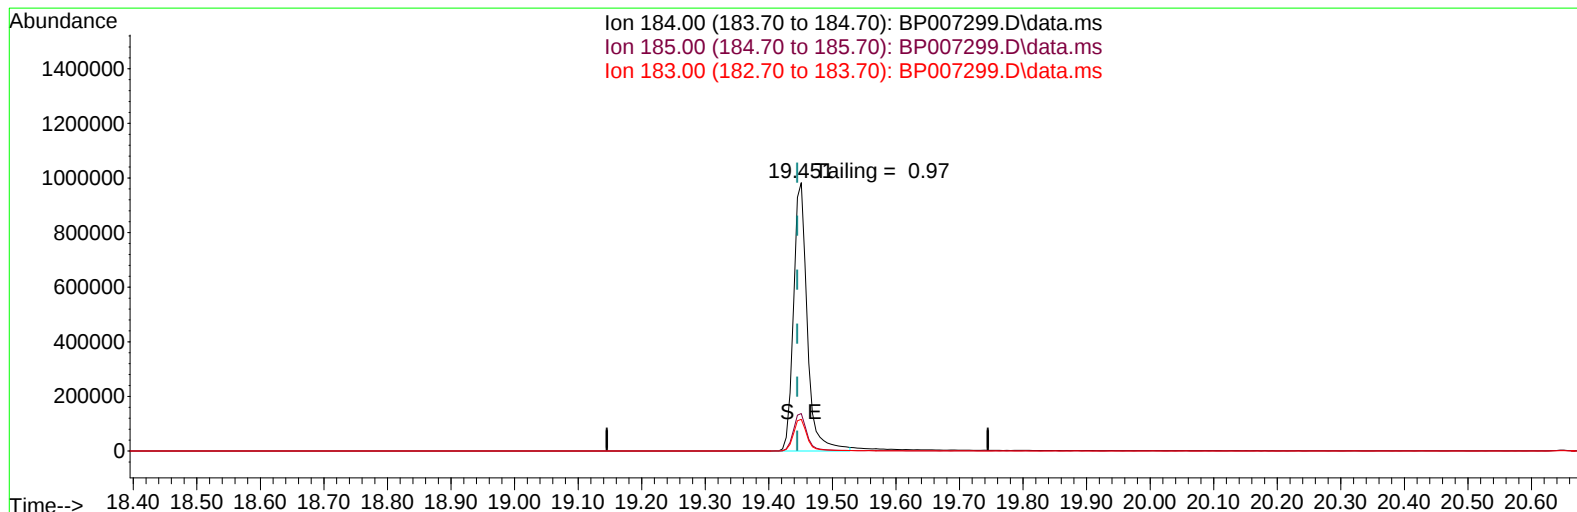

TIC: BP007299.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 321001.68 ng

response 1529057

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.97
183.00	11.90	11.80
0.00	0.00	0.00