

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
 Data File : BP007301.D
 Acq On : 04 Oct 2021 12:09
 Operator : CG/JU
 Sample : PB139537BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139537BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	394	401	423	rBV	2908192	4353496	42.23%	9.983%
2	7.046	665	673	696	rBV	2532271	4227493	41.00%	9.694%
3	7.863	805	812	820	rBV	596459	948884	9.20%	2.176%
4	9.028	1002	1010	1031	rBV	1524164	2694758	26.14%	6.179%
5	10.663	1279	1288	1308	rBV	705139	1268604	12.30%	2.909%
6	13.122	1699	1706	1728	rBV	4058647	6422771	62.30%	14.728%
7	14.498	1933	1940	1955	rBV	1042308	1668459	16.18%	3.826%
8	15.998	2187	2195	2227	rBV	3072900	4935057	47.87%	11.317%
9	17.257	2402	2409	2419	rBV	1326033	2030272	19.69%	4.656%
10	19.816	2838	2844	2857	rBV	8366561	10310009	100.00%	23.642%
11	21.339	3099	3103	3115	rBV	1726521	2339199	22.69%	5.364%
12	23.751	3506	3513	3523	rVB2	1106966	2410180	23.38%	5.527%




Sum of corrected areas: 43609182

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
Data File : BP007301.D
Acq On : 04 Oct 2021 12:09
Operator : CG/JU
Sample : PB139537BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139537BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

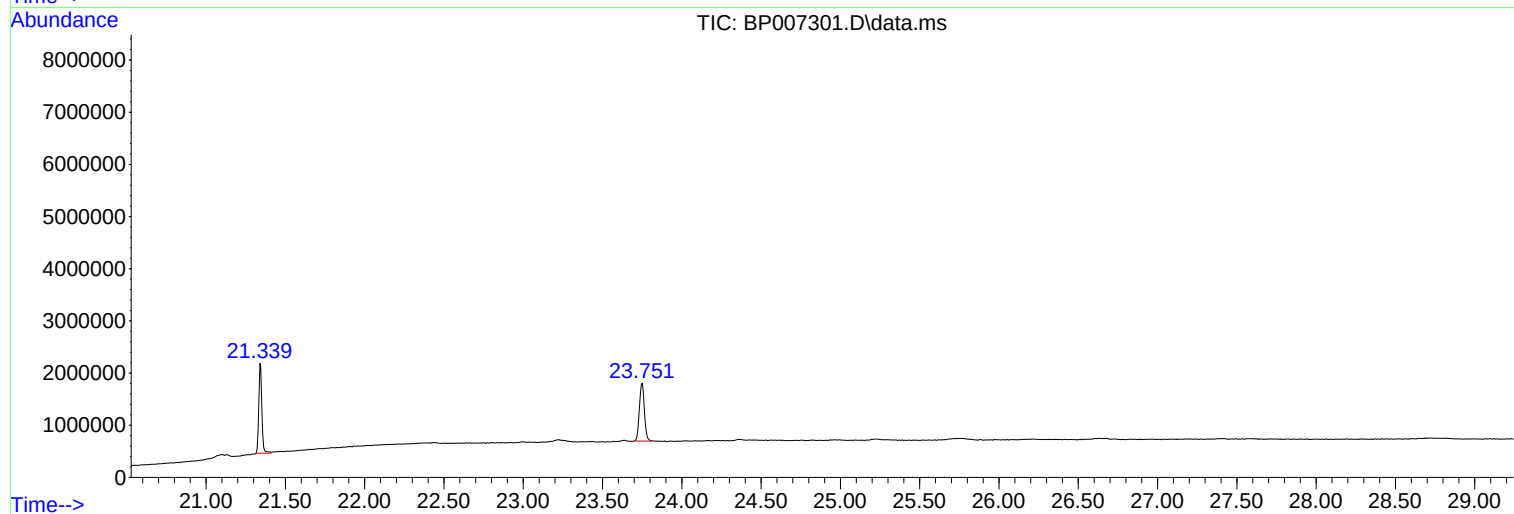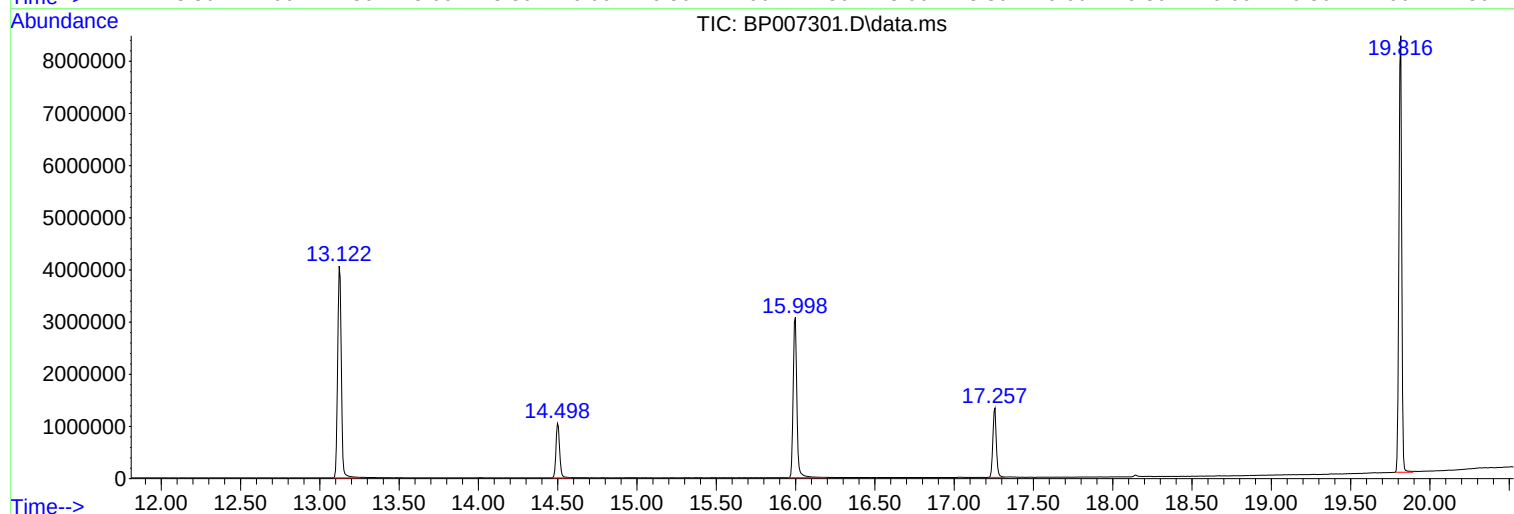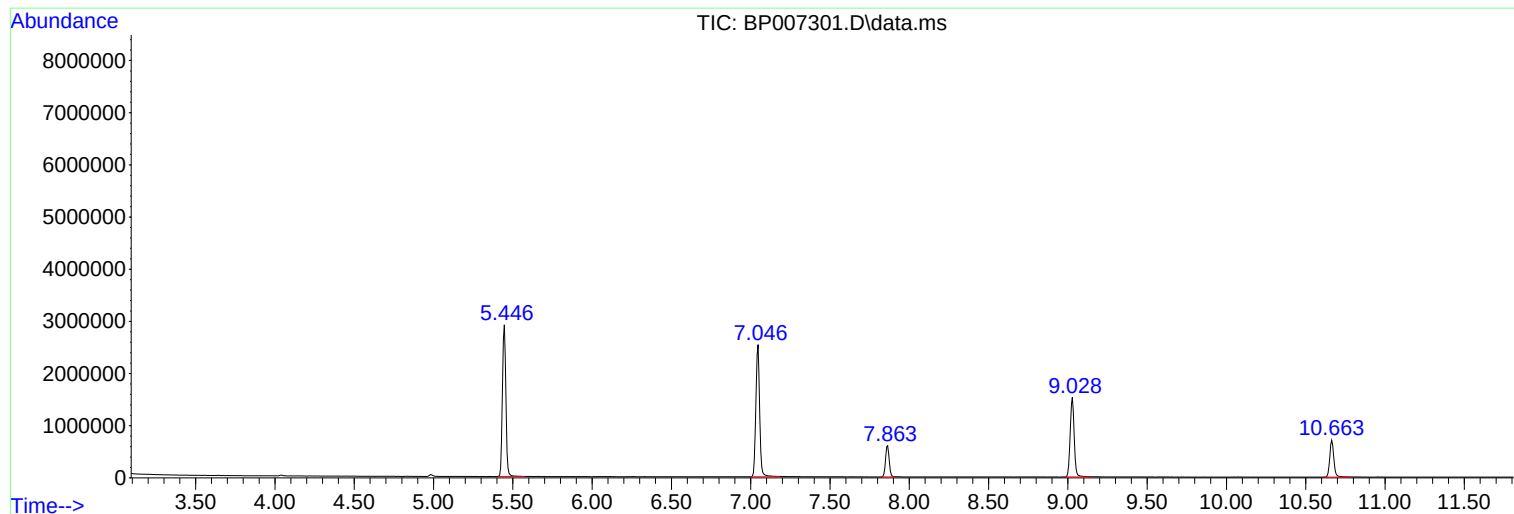

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
Data File : BP007301.D
Acq On : 04 Oct 2021 12:09
Operator : CG/JU
Sample : PB139537BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139537BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
Data File : BP007301.D
Acq On : 04 Oct 2021 12:09
Operator : CG/JU
Sample : PB139537BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139537BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------