

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
 Data File : BP007307.D
 Acq On : 04 Oct 2021 16:21
 Operator : CG/JU
 Sample : M4040-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P287-DITCH

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	395	401	416	rBV	1203156	1762393	19.82%	4.228%
2	7.046	665	673	688	rBV	567023	985021	11.08%	2.363%
3	7.863	804	812	820	rBV	585334	923442	10.38%	2.215%
4	9.028	996	1010	1029	rBV	1656106	2841908	31.96%	6.818%
5	10.446	1243	1251	1271	rBV	478345	961713	10.82%	2.307%
6	10.663	1280	1288	1300	rBV	686445	1186062	13.34%	2.845%
7	12.293	1558	1565	1578	rBV2	49361	136458	1.53%	0.327%
8	13.122	1698	1706	1728	rBV	4303235	6544400	73.60%	15.700%
9	14.363	1908	1917	1932	rBV4	28145	98834	1.11%	0.237%
10	14.498	1933	1940	1958	rVB	1020000	1537198	17.29%	3.688%
11	15.992	2187	2194	2211	rBV	3188654	4689670	52.74%	11.250%
12	17.251	2400	2408	2412	rBV	1196798	1790310	20.13%	4.295%
13	17.292	2412	2415	2419	rVV	636860	765188	8.61%	1.836%
14	17.333	2419	2422	2431	rVB2	60050	97748	1.10%	0.234%
15	17.469	2441	2445	2454	rVB2	85523	121700	1.37%	0.292%
16	17.616	2465	2470	2478	rBV	195945	257564	2.90%	0.618%
17	17.922	2517	2522	2526	rBV	104063	129889	1.46%	0.312%
18	18.139	2554	2559	2566	rBV	168190	263017	2.96%	0.631%
19	18.775	2663	2667	2670	rBV	123489	140840	1.58%	0.338%
20	19.051	2710	2714	2718	rBV	111773	125734	1.41%	0.302%
21	19.810	2837	2843	2851	rBV	7517282	8892227	100.00%	21.332%
22	21.039	3049	3052	3059	rBV2	476457	602156	6.77%	1.445%
23	21.333	3098	3102	3109	rBV	1600447	2035445	22.89%	4.883%
24	22.574	3310	3313	3318	rVB	230386	315435	3.55%	0.757%
25	23.739	3505	3511	3521	rVB2	1177320	2422398	27.24%	5.811%
26	26.468	3970	3975	3988	rVB3	704716	2058400	23.15%	4.938%




Sum of corrected areas: 41685150

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
Data File : BP007307.D
Acq On : 04 Oct 2021 16:21
Operator : CG/JU
Sample : M4040-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P287-DITCH

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

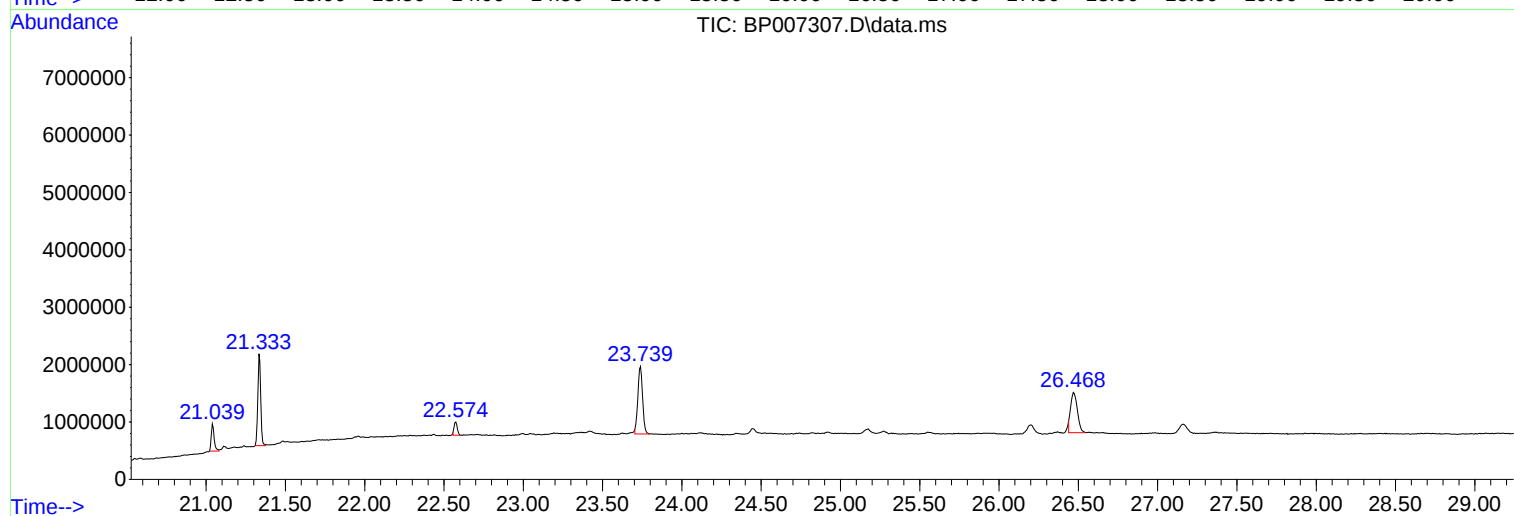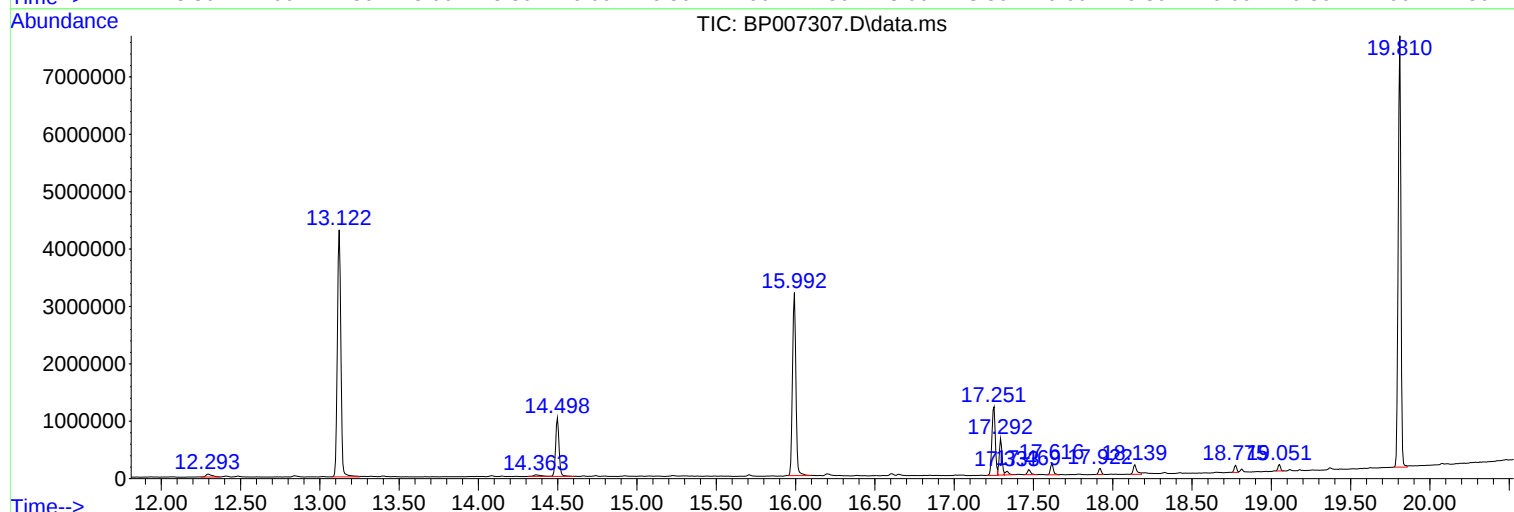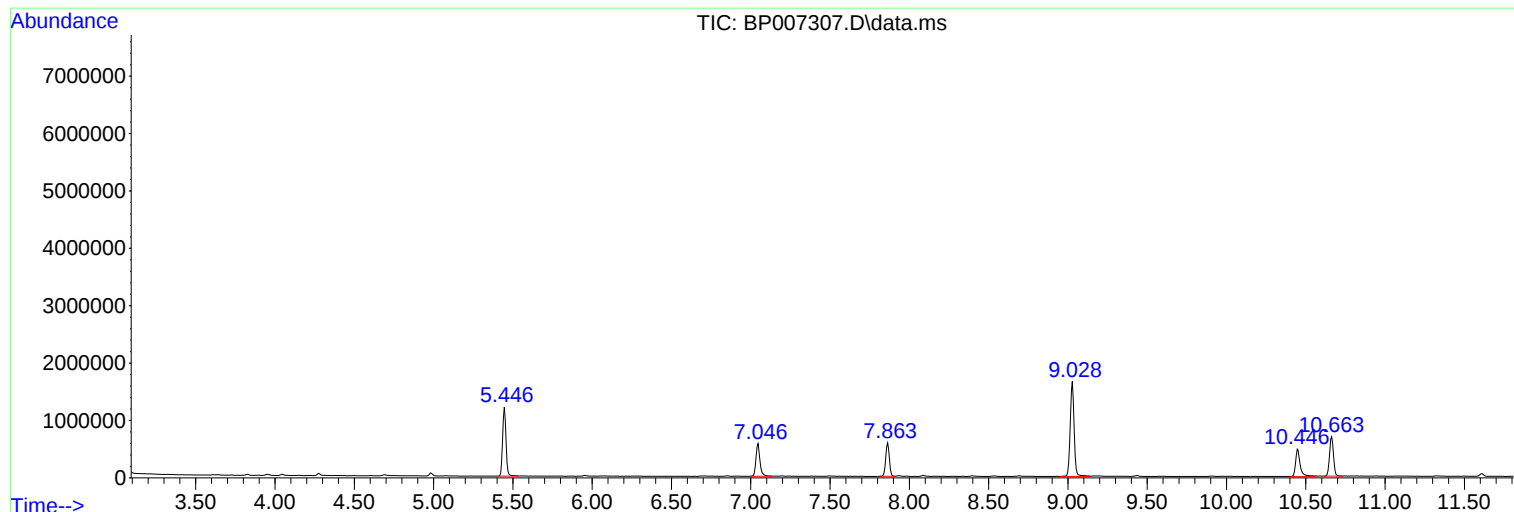

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
Data File : BP007307.D
Acq On : 04 Oct 2021 16:21
Operator : CG/JU
Sample : M4040-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P287-DITCH

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
Data File : BP007307.D
Acq On : 04 Oct 2021 16:21
Operator : CG/JU
Sample : M4040-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P287-DITCH

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
