


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
 Data File : BP007299.D
 Acq On : 04 Oct 2021 10:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 12:49:05 2021

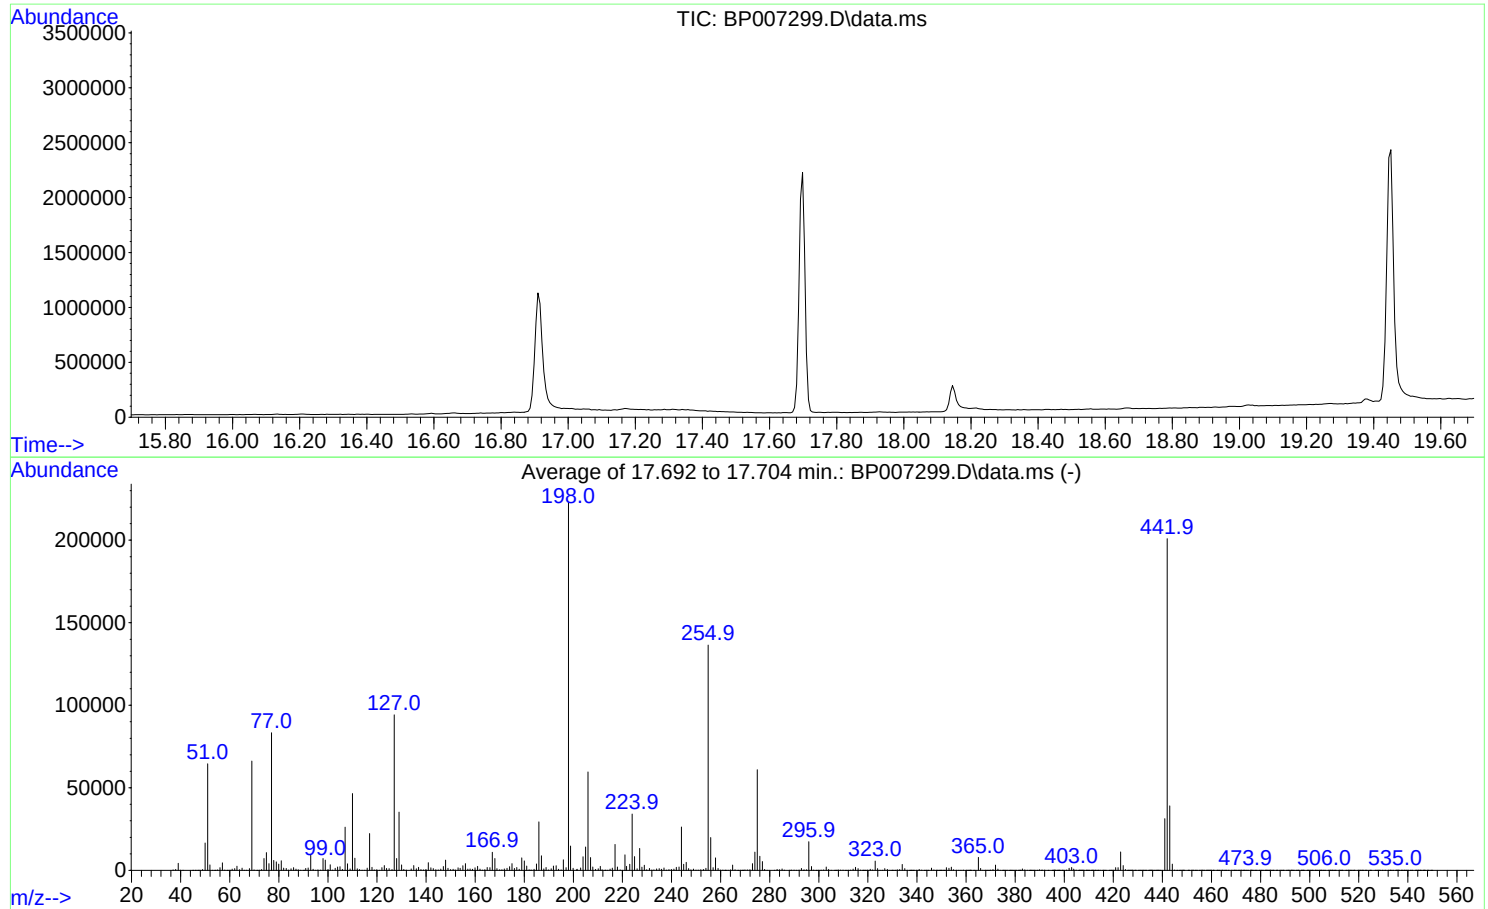




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	64541	PASS
68	69	0.00	2	1.6	1042	PASS
69	198	0.00	100	29.7	66158	PASS
70	69	0.00	2	0.5	334	PASS
127	198	10	80	42.3	94226	PASS
197	198	0.00	2	0.7	1627	PASS
198	198	100	100	100.0	222821	PASS
199	198	5	9	6.6	14777	PASS
275	198	10	60	27.3	60935	PASS
365	198	1	100	3.5	7828	PASS
441	198	0.01	100	14.0	31301	PASS
442	442	100	100	100.0	200885	PASS
443	442	15	24	19.4	39043	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
Data File : BP007299.D
Acq On : 04 Oct 2021 10:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Oct 04 13:24:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 12:49:05 2021
Response via : Initial Calibration

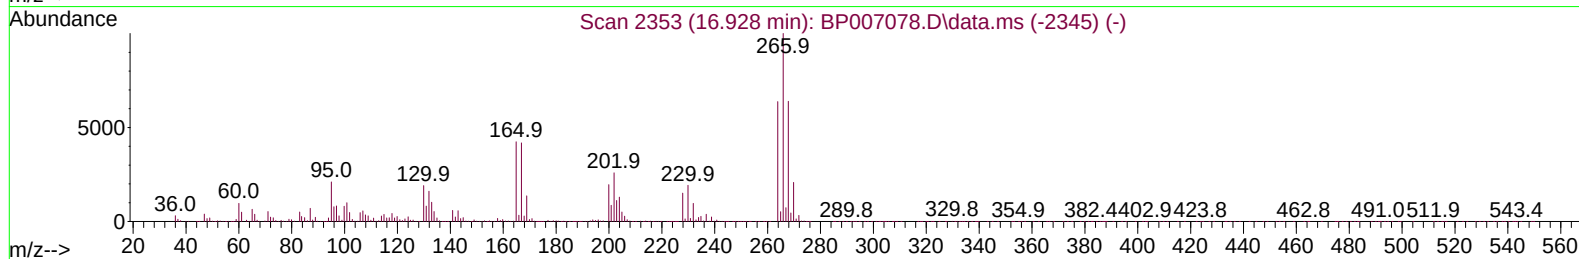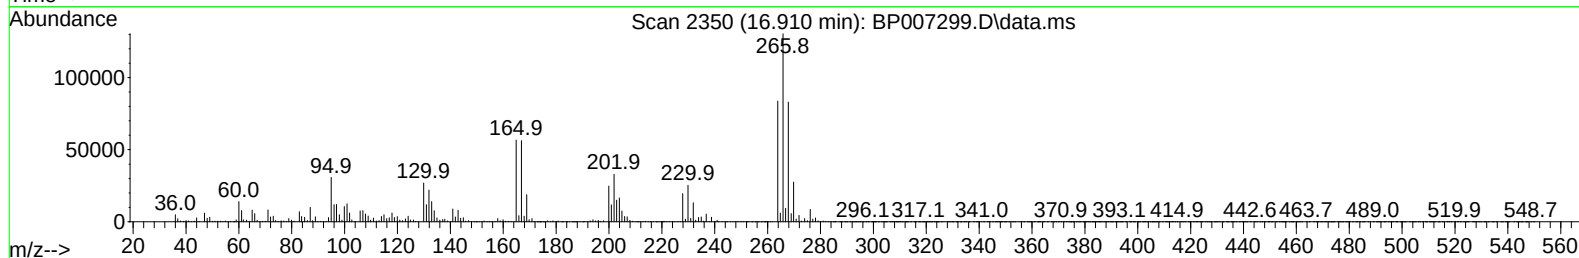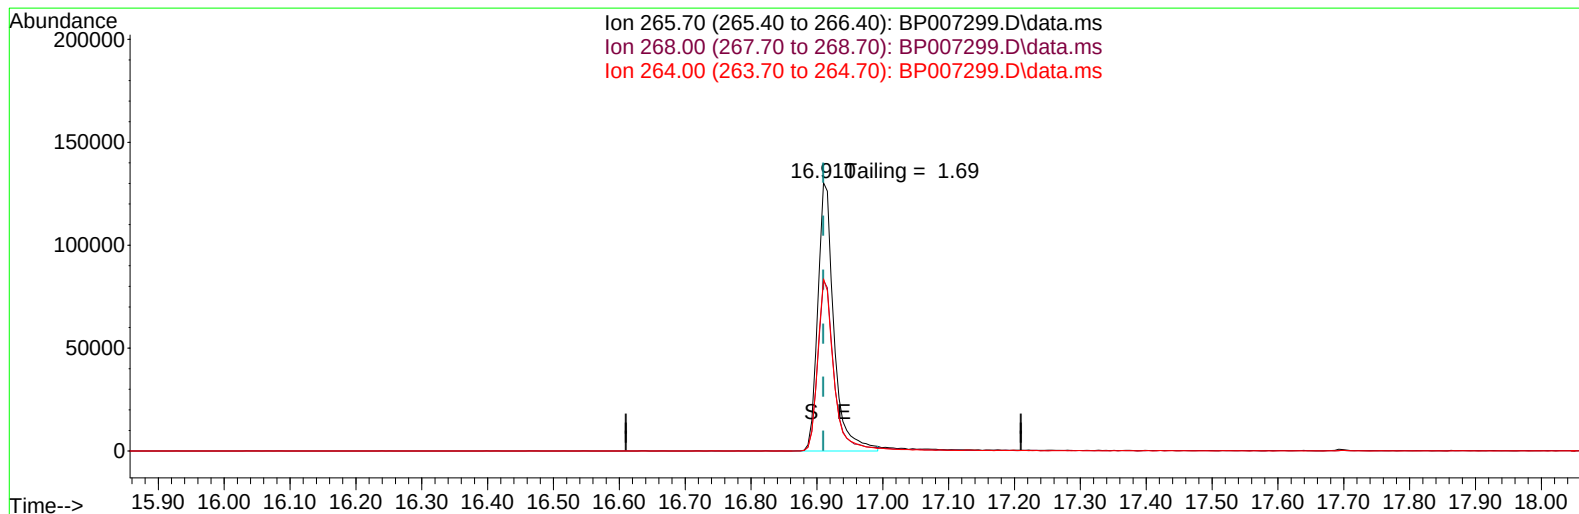

TIC: BP007299.D\data.ms

(70) Pentachlorophenol (C)

16.910min (+ 0.000) 342705.19 ng




response 226859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.63
264.00	62.90	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100421\
 Data File : BP007299.D
 Acq On : 04 Oct 2021 10:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Oct 04 13:24:06 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 01 12:49:05 2021
 Response via : Initial Calibration

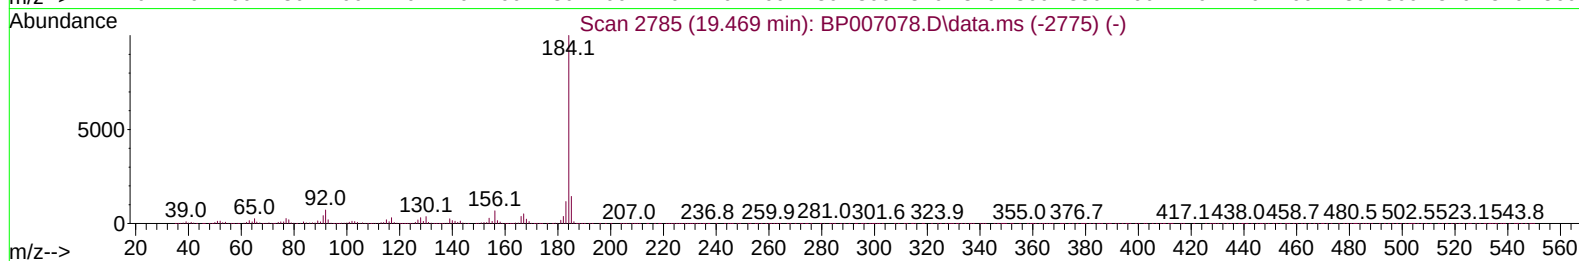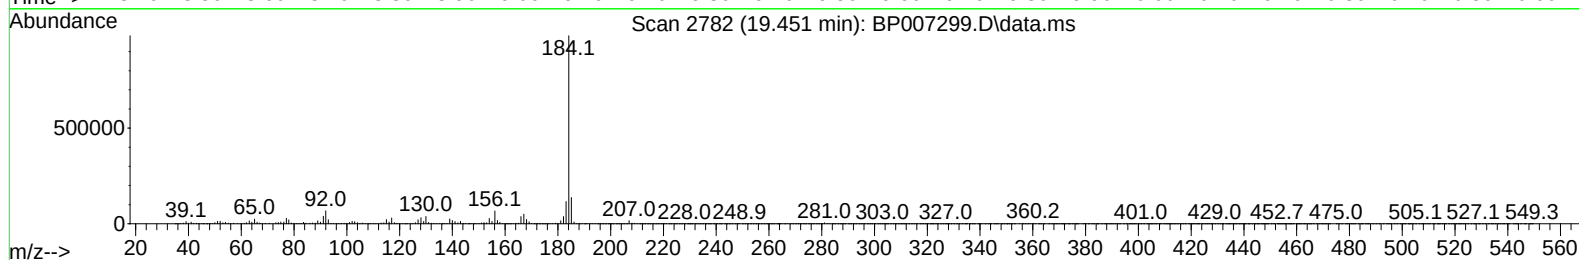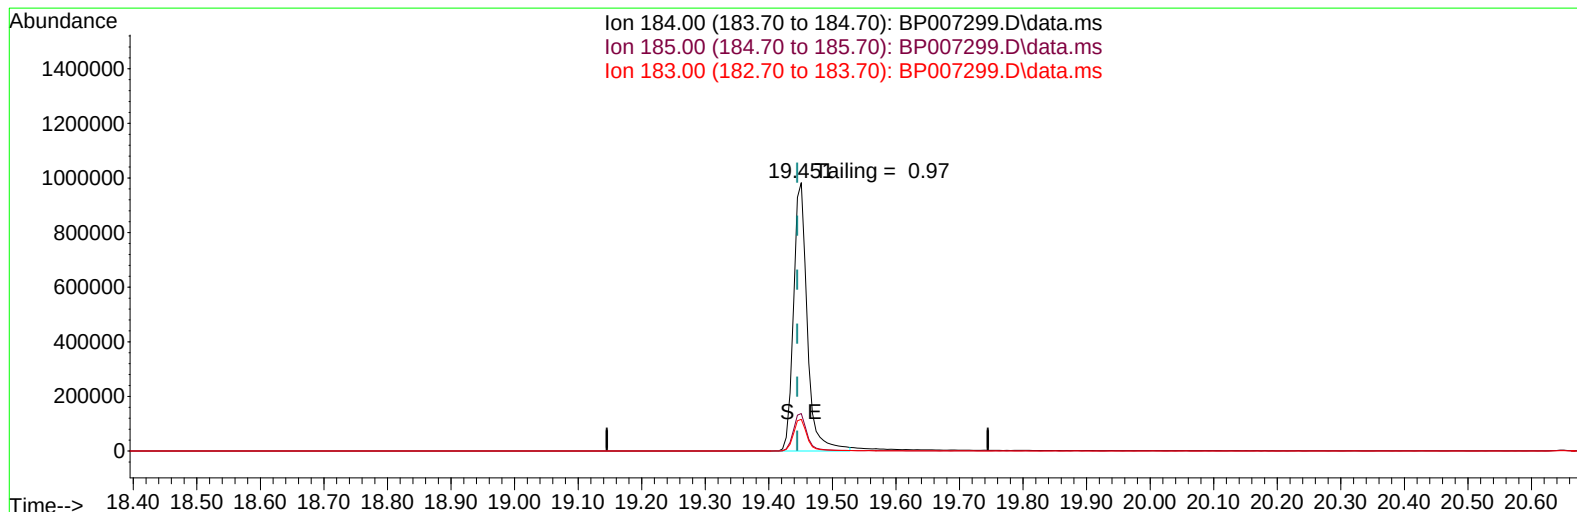

TIC: BP007299.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 321001.68 ng

response 1529057

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.97
183.00	11.90	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/4/2021	BNA_P	<u>BP007299.D</u>
Compound Name	Response	Retention Time
DDT	788662	20.65
DDD	9018	20.22
DDE	1240	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10258	798920	1.28

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP