




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022246.D
Acq On : 05 Oct 2024 03:20
Operator : RC/JU
Sample : P4264-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCYO2

Manual IntegrationsAPPROVED

Quant Time: Oct 05 05:00:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 05:25:28 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/06/2024
Supervised By :mohammad ahmed 10/06/2024

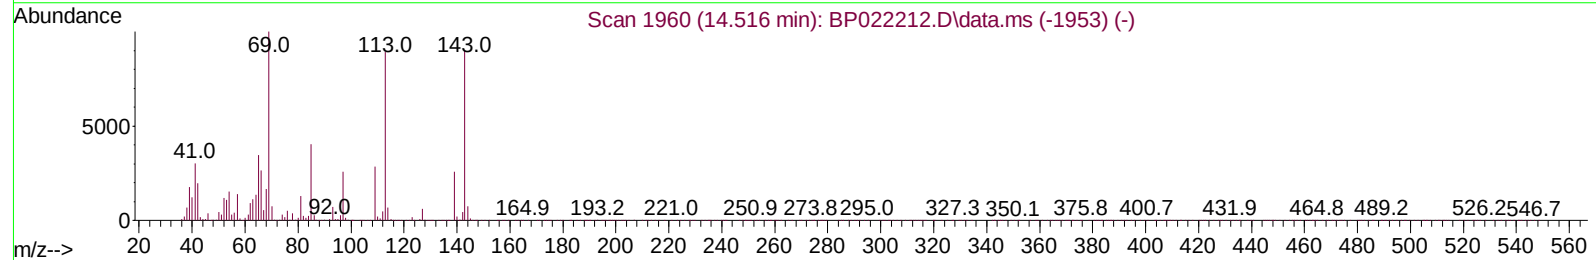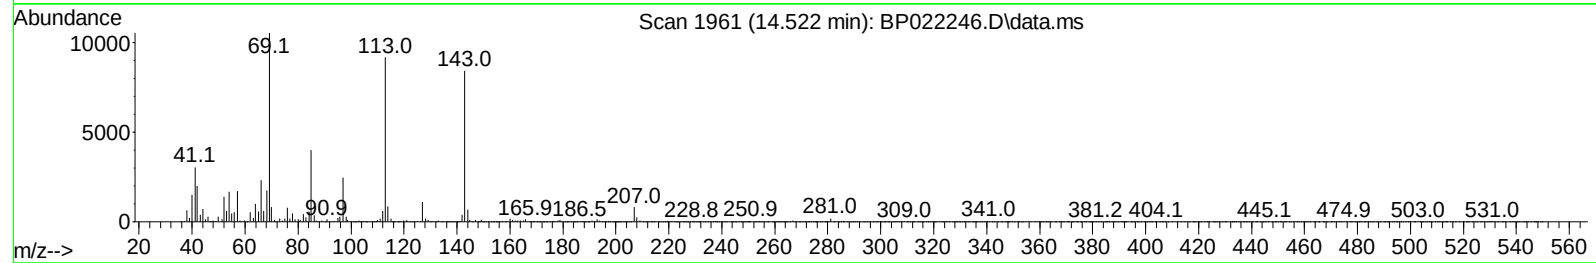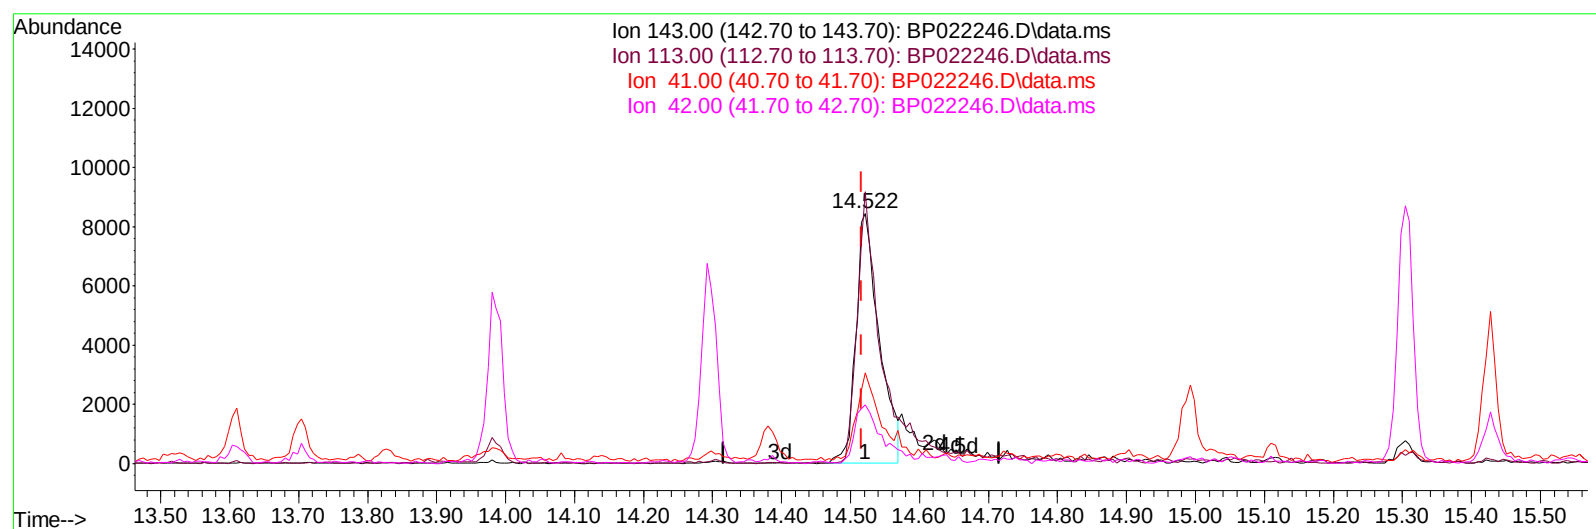

TIC: BP022246.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (+ 0.006) 4.41 ng/ul

response 19868

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.70	108.61
41.00	35.80	36.17
42.00	26.20	23.52




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022246.D
 Acq On : 05 Oct 2024 03:20
 Operator : RC/JU
 Sample : P4264-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCYO2

Manual IntegrationsAPPROVED

Quant Time: Oct 05 05:00:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 05:25:28 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/06/2024
 Supervised By :mohammad ahmed 10/06/2024

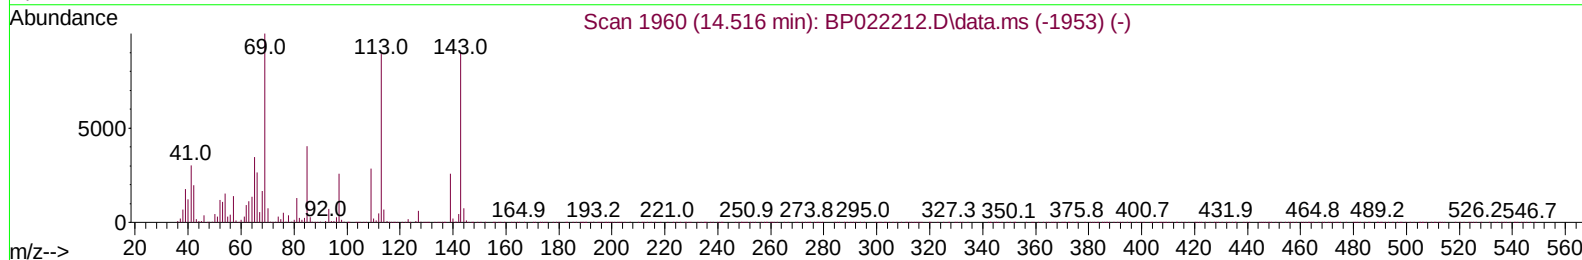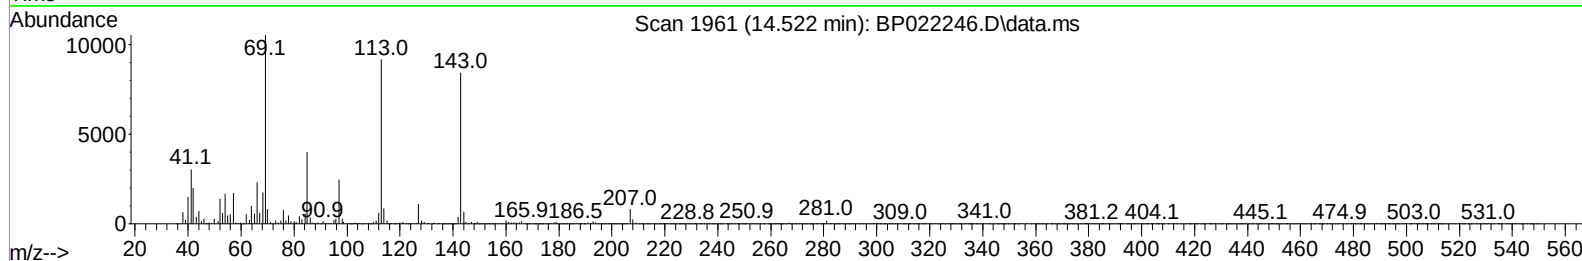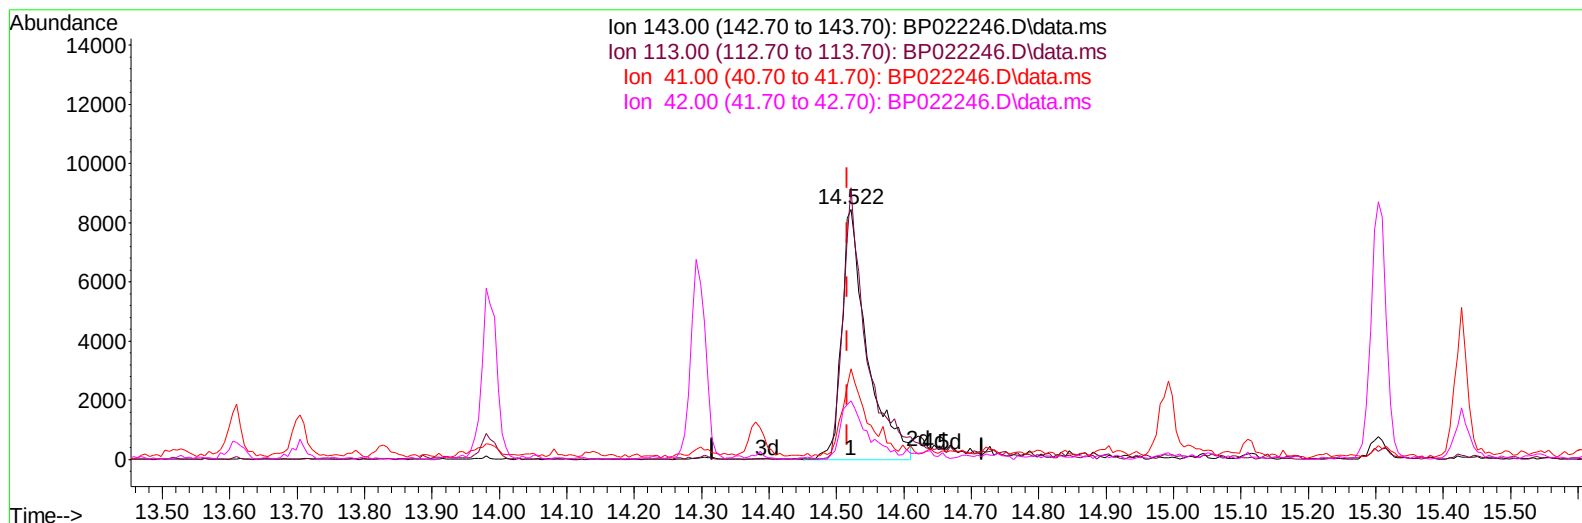

TIC: BP022246.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (+ 0.006) 4.96 ng/ul m

response 22313

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.70	108.61
41.00	35.80	36.17
42.00	26.20	23.52

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022246.D
 Acq On : 05 Oct 2024 03:20
 Operator : RC/JU
 Sample : P4264-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCYO2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/06/2024
 Supervised By :mohammad ahmed 10/06/2024

Quant Time: Oct 05 05:01:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 05:25:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	115595	20.000	ng/ul	0.00
20) Naphthalene-d8	10.451	136	435138	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.298	164	340353	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.092	188	795934	20.000	ng/ul	0.00
79) Chrysene-d12	21.521	240	861955	20.000	ng/ul	-0.01
88) Perylene-d12	24.803	264	986260	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.216	96	9847	3.337	ng/uL	0.00
4) Pyridine-d5	3.634	84	36443	4.320	ng/ul	0.00
7) Phenol-d5	6.875	99	59043	6.244	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	136773	23.490	ng/ul	0.00
11) 2-Chlorophenol-d4	7.234	132	158293	23.137	ng/ul	0.00
15) 4-Methylphenol-d8	8.392	113	115855	15.462	ng/ul	0.00
21) Nitrobenzene-d5	8.834	128	88191	27.079	ng/ul	0.00
24) 2-Nitrophenol-d4	9.545	143	102815	27.842	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.081	165	202937	25.306	ng/ul	0.00
31) 4-Chloroaniline-d4	10.586	131	164282	17.169	ng/ul	0.00
46) Dimethylphthalate-d6	13.704	166	732655	27.847	ng/ul	0.00
49) Acenaphthylene-d8	13.986	160	729967	26.206	ng/ul	0.00
54) 4-Nitrophenol-d4	14.522	143	22313m	4.958	ng/ul	0.00
60) Fluorene-d10	15.304	176	627394	26.959	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.427	200	108925	22.043	ng/ul	0.00
73) Anthracene-d10	17.192	188	1162890	31.296	ng/ul	-0.01
81) Pyrene-d10	19.568	212	1469162	32.899	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.592	264	1619104	31.212	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022246.D
Acq On : 05 Oct 2024 03:20
Operator : RC/JU
Sample : P4264-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCYO2

Manual IntegrationsAPPROVED

Quant Time: Oct 05 05:01:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 05:25:28 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/06/2024
Supervised By :mohammad ahmed 10/06/2024

