

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022232.D
 Acq On : 04 Oct 2024 17:05
 Operator : RC/JU
 Sample : P4019-09MEDL 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDCE5MEDL

Quant Time: Oct 05 00:30:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 04 05:25:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	134450	20.000	ng/ul	0.00
20) Naphthalene-d8	10.457	136	508402	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164	395374	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.092	188	955834	20.000	ng/ul	0.00
79) Chrysene-d12	21.521	240	1049156	20.000	ng/ul	-0.01
88) Perylene-d12	24.810	264	1225638	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	1914	0.558	ng/uL	0.00
4) Pyridine-d5	3.640	84	19627	2.000	ng/ul	0.01
7) Phenol-d5	6.875	99	31333	2.849	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	20069	2.963	ng/ul	0.00
11) 2-Chlorophenol-d4	7.234	132	24996	3.141	ng/ul	0.00
15) 4-Methylphenol-d8	8.399	113	24304	2.789	ng/ul	0.00
21) Nitrobenzene-d5	8.834	128	11363	2.986	ng/ul	0.00
24) 2-Nitrophenol-d4	9.552	143	12223	2.833	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.087	165	27053	2.887	ng/ul	0.00
31) 4-Chloroaniline-d4	10.593	131	31379	2.807	ng/ul	0.00
46) Dimethylphthalate-d6	13.710	166	109226	3.574	ng/ul	0.00
49) Acenaphthylene-d8	13.992	160	109774	3.392	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.310	176	95295	3.525	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.198	188	164767	3.693	ng/ul	0.00
81) Pyrene-d10	19.575	212	203878	3.751	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.580	264	224302	3.479	ng/ul	0.00
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	14.945	232	37609	4.117	ng/ul#	99
71) Pentachlorophenol	16.739	266	449642	48.354	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022232.D
Acq On : 04 Oct 2024 17:05
Operator : RC/JU
Sample : P4019-09MEDL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDCE5MEDL

Quant Time: Oct 05 00:30:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 04 05:25:28 2024
Response via : Initial Calibration

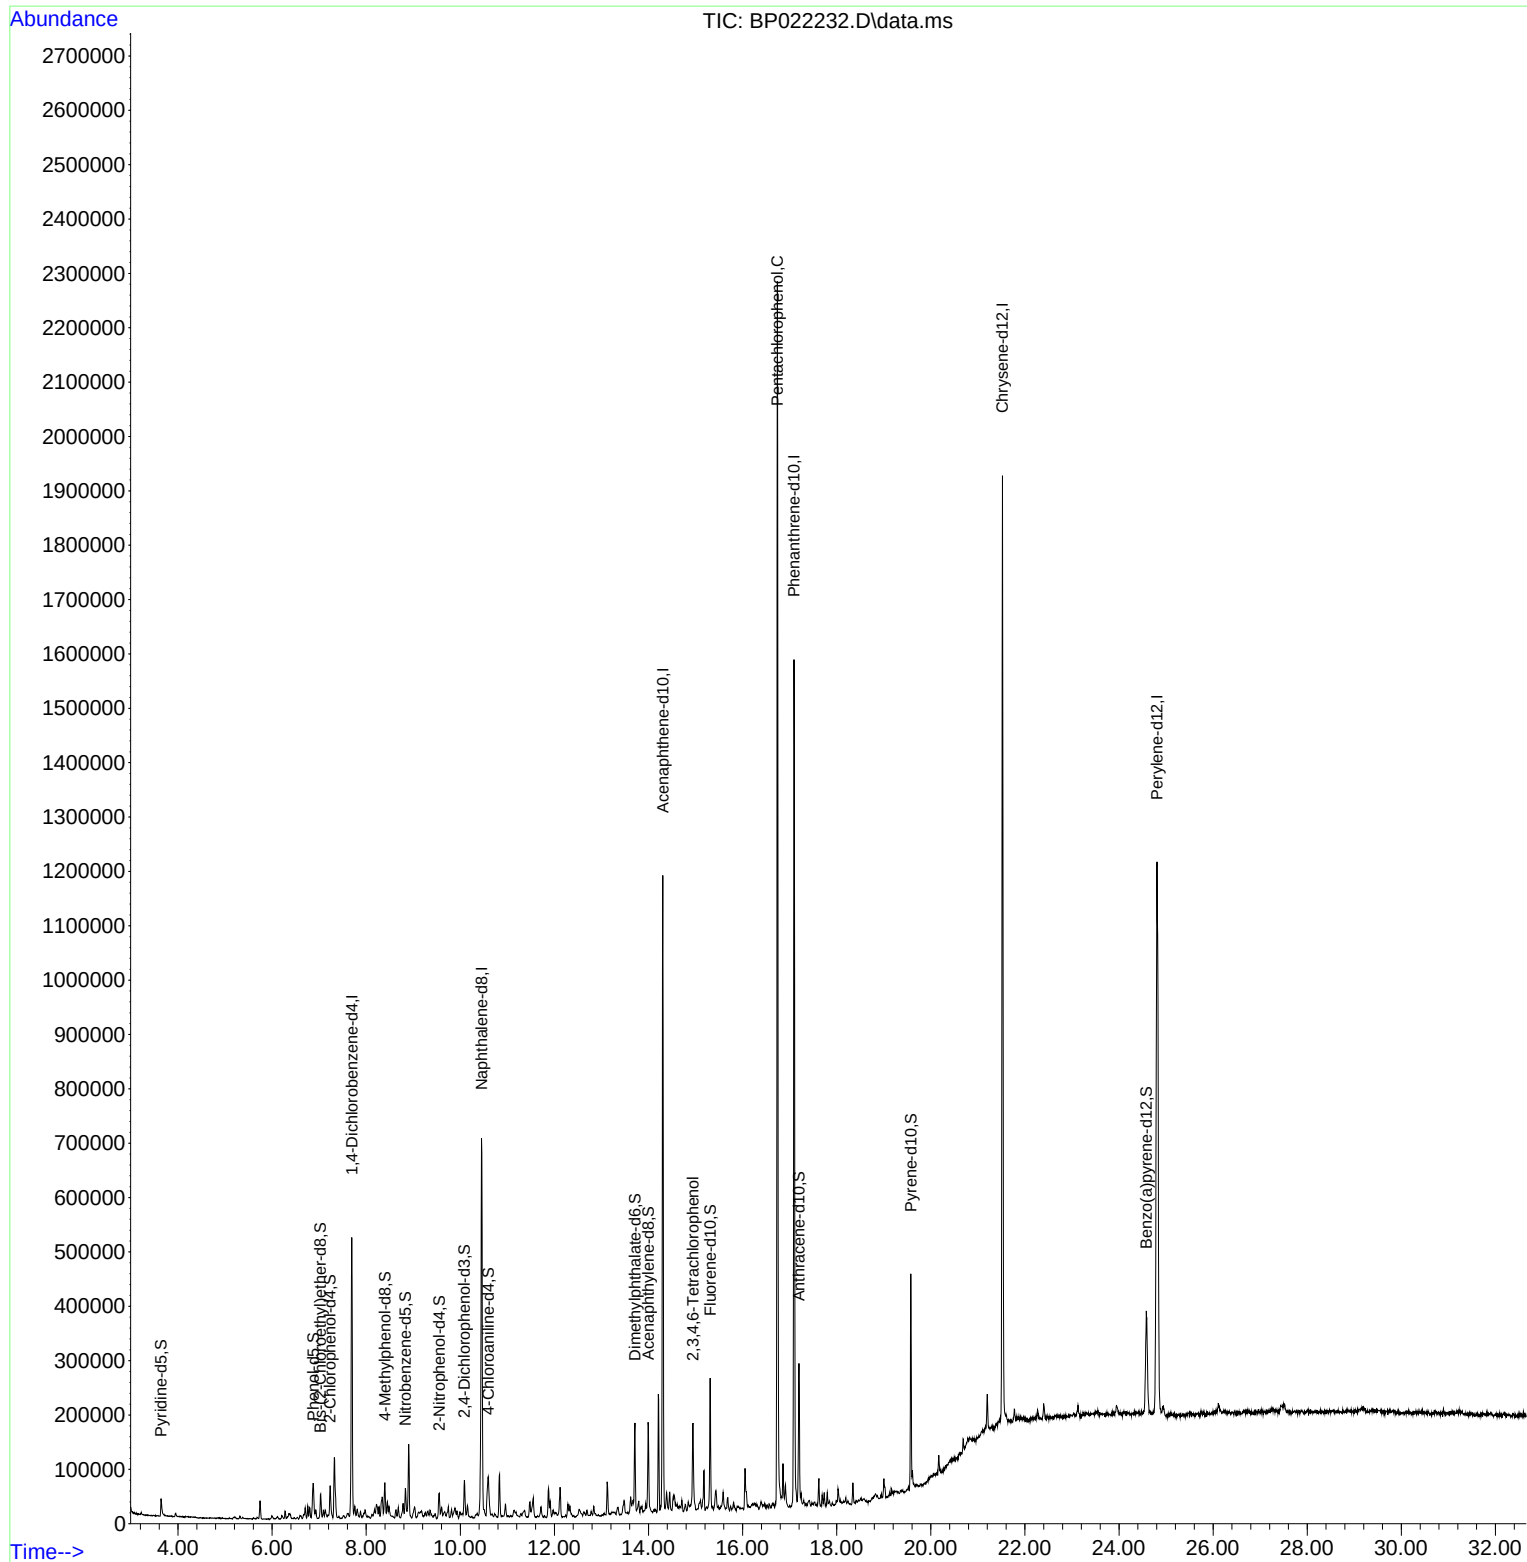




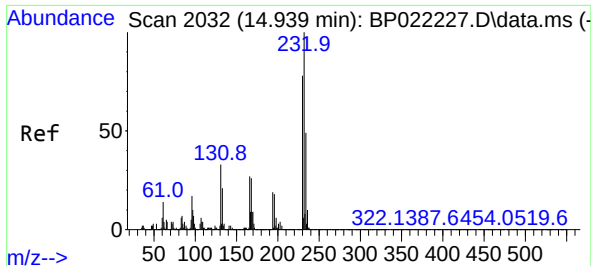


#58
2,3,4,6-Tetrachlorophenol
Concen: 4.117 ng/ul
RT: 14.945 min Scan# 2032
Delta R.T. 0.012 min
Lab File: BP022232.D
Acq: 04 Oct 2024 17:05

Instrument :
BNA_P
ClientSampleId :
DDCE5MEDL

Tgt Ion:232 Resp: 37609

Ion	Ratio	Lower	Upper
232	100		
131	34.6	28.2	42.2
130	2.8	1.8	2.6#
166	27.2	21.8	32.6

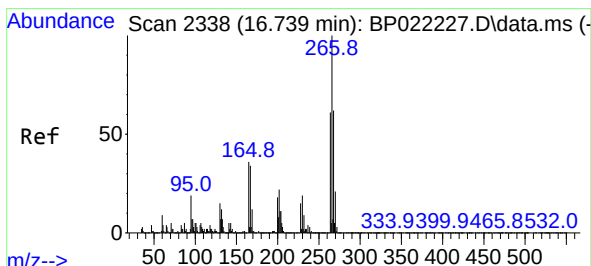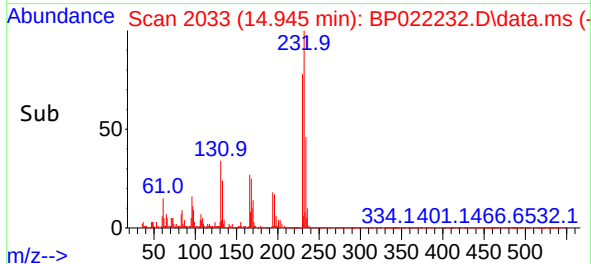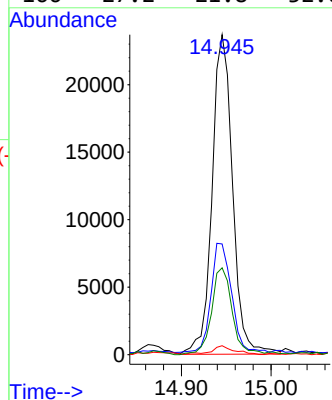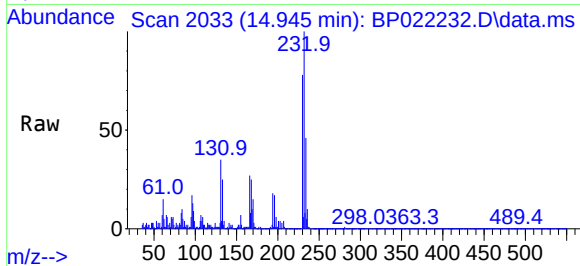

#71
Pentachlorophenol
Concen: 48.354 ng/ul
RT: 16.739 min Scan# 2338
Delta R.T. -0.000 min
Lab File: BP022232.D
Acq: 04 Oct 2024 17:05

Tgt Ion:266 Resp: 449642

Ion	Ratio	Lower	Upper
266	100		
264	63.2	50.2	75.4
268	63.8	51.4	77.0

