

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022228.D
 Acq On : 04 Oct 2024 14:21
 Operator : RC/JU
 Sample : PB163610BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022228.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	35	39	46	rVB	31576	40883	1.24%	0.117%
2	3.628	105	109	127	rBV	386927	623423	18.96%	1.781%
3	3.952	159	164	169	rVB2	7109	11248	0.34%	0.032%
4	6.875	654	661	673	rBV	455697	757984	23.05%	2.165%
5	7.034	681	688	696	rBV	357624	553015	16.82%	1.580%
6	7.234	715	722	734	rBV	475065	781386	23.77%	2.232%
7	7.693	792	800	809	rBV	531935	836784	25.45%	2.390%
8	8.393	911	919	932	rBV	618197	968834	29.47%	2.768%
9	8.834	986	994	1003	rBV	463809	755849	22.99%	2.159%
10	9.546	1106	1115	1126	rBV	394681	645582	19.64%	1.844%
11	10.081	1196	1206	1221	rBV	611521	1083442	32.95%	3.095%
12	10.451	1260	1269	1280	rBV	732015	1177187	35.80%	3.363%
13	10.587	1283	1292	1308	rBV	516627	998423	30.37%	2.852%
14	12.040	1532	1539	1544	rBV3	9863	17134	0.52%	0.049%
15	13.710	1816	1823	1835	rBV	1204310	1642783	49.97%	4.693%
16	13.992	1863	1871	1883	rBV	1277777	1911814	58.15%	5.461%
17	14.298	1916	1923	1933	rBV	1195771	1748550	53.18%	4.995%
18	14.522	1954	1961	1979	rBV	309347	645940	19.65%	1.845%
19	14.969	2034	2037	2043	rVB8	1991	3306	0.10%	0.009%
20	15.310	2086	2095	2105	rBV	1873182	2476200	75.31%	7.074%
21	15.434	2110	2116	2126	rVV	308830	464628	14.13%	1.327%
22	15.563	2133	2138	2144	rVB4	7729	13182	0.40%	0.038%
23	16.745	2334	2339	2348	rBV4	4054	11198	0.34%	0.032%
24	16.886	2360	2363	2367	rBV5	3673	6118	0.19%	0.017%
25	16.981	2371	2379	2380	rBV7	2225	4217	0.13%	0.012%
26	17.098	2392	2399	2408	rBV	1593295	2259767	68.73%	6.455%
27	17.204	2410	2417	2432	rVV	1735209	2702783	82.21%	7.721%
28	19.128	2740	2744	2750	rBV3	26046	38438	1.17%	0.110%
29	19.198	2752	2756	2761	rBV	22238	33777	1.03%	0.096%
30	19.580	2814	2821	2832	rBV	2330329	3240514	98.56%	9.257%
31	21.539	3148	3154	3163	rVB	1720029	2618895	79.65%	7.481%
32	24.574	3662	3670	3685	rVB	1291264	3287807	100.00%	9.392%
33	24.821	3702	3712	3727	rVB	952481	2644420	80.43%	7.554%


Sum of corrected areas: 35005511

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022228.D
Acq On : 04 Oct 2024 14:21
Operator : RC/JU
Sample : PB163610BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK610

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

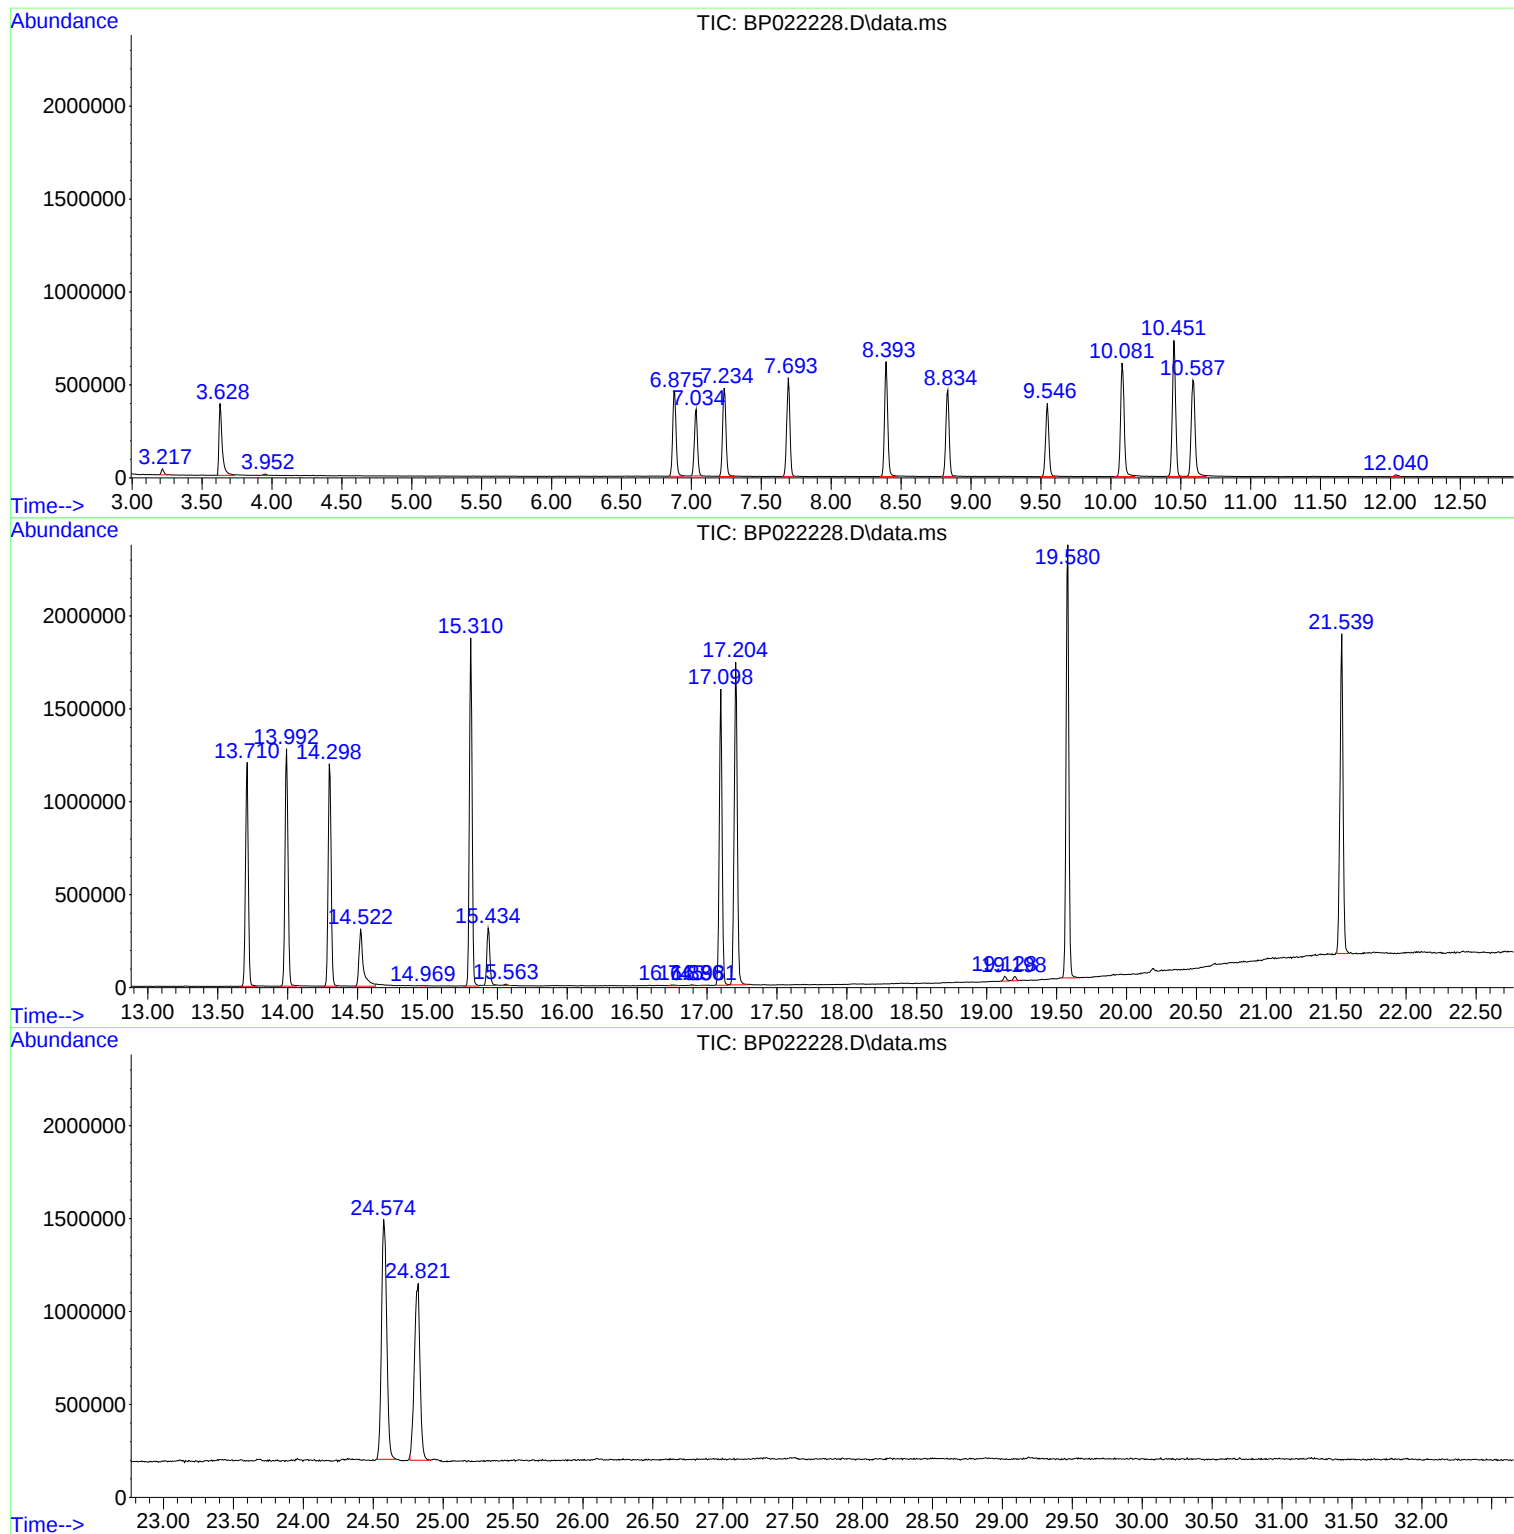

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022228.D
Acq On : 04 Oct 2024 14:21
Operator : RC/JU
Sample : PB163610BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK610

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022228.D
Acq On : 04 Oct 2024 14:21
Operator : RC/JU
Sample : PB163610BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK610

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc