

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022230.D
 Acq On : 04 Oct 2024 15:43
 Operator : RC/JU
 Sample : P3927-08MEDL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDC93MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.634	106	110	123	rBV	47616	80373	2.48%	0.349%
2	6.875	652	661	674	rVB	67431	130771	4.04%	0.569%
3	7.028	680	687	696	rBV	53770	91356	2.82%	0.397%
4	7.128	700	704	714	rVB6	8783	14994	0.46%	0.065%
5	7.234	714	722	731	rBV2	69489	125292	3.87%	0.545%
6	7.322	732	737	745	rVB3	15975	28189	0.87%	0.123%
7	7.687	791	799	808	rBV	415968	714910	22.10%	3.108%
8	8.116	865	872	876	rBV2	20299	32604	1.01%	0.142%
9	8.163	876	880	885	rVV4	7280	14409	0.45%	0.063%
10	8.216	885	889	895	rVV6	5637	11712	0.36%	0.051%
11	8.340	902	910	913	rBV7	9158	21116	0.65%	0.092%
12	8.393	913	919	926	rVV	97428	162440	5.02%	0.706%
13	8.446	926	928	932	rVV3	8504	11901	0.37%	0.052%
14	8.675	962	967	975	rVB7	9088	17567	0.54%	0.076%
15	8.787	980	986	988	rBV5	6877	12847	0.40%	0.056%
16	8.834	988	994	1000	rVV	71618	123798	3.83%	0.538%
17	8.899	1000	1005	1011	rVV	42996	66387	2.05%	0.289%
18	9.028	1020	1027	1032	rVB10	6276	13910	0.43%	0.060%
19	9.104	1035	1040	1047	rBV8	6695	14950	0.46%	0.065%
20	9.457	1095	1100	1106	rVB4	7902	14040	0.43%	0.061%
21	9.546	1106	1115	1121	rBV2	61480	117818	3.64%	0.512%
22	9.740	1146	1148	1153	rVB5	8569	10898	0.34%	0.047%
23	9.804	1153	1159	1164	rBV8	6704	12056	0.37%	0.052%
24	10.087	1201	1207	1213	rBV	96062	163273	5.05%	0.710%
25	10.145	1213	1217	1223	rVB4	10533	18545	0.57%	0.081%
26	10.451	1257	1269	1276	rBV	685744	1219142	37.68%	5.301%
27	10.593	1283	1293	1304	rBV2	93300	256259	7.92%	1.114%
28	10.734	1311	1317	1328	rVB2	4787	12765	0.39%	0.055%
29	10.828	1328	1333	1342	rVB	46825	76680	2.37%	0.333%
30	10.957	1346	1355	1362	rBV3	16801	39277	1.21%	0.171%
31	11.340	1415	1420	1423	rBV5	8522	15449	0.48%	0.067%
32	11.481	1438	1444	1448	rBV2	21764	39148	1.21%	0.170%
33	11.551	1448	1456	1463	rVB	46906	83674	2.59%	0.364%
34	11.710	1475	1483	1490	rBV5	33321	67507	2.09%	0.294%
35	11.875	1502	1511	1514	rBV2	43827	73017	2.26%	0.317%
36	11.910	1514	1517	1523	rVV2	34573	50493	1.56%	0.220%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022230.D
 Acq On : 04 Oct 2024 15:43
 Operator : RC/JU
 Sample : P3927-08MEDL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDC93MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	11.969	1523	1527	1530	rVV6	9107	17223	0.53%	0.075%
38	12.010	1530	1534	1537	rVV3	11861	23311	0.72%	0.101%
39	12.040	1537	1539	1546	rVV5	11115	22908	0.71%	0.100%
40	12.122	1546	1553	1559	rVB2	59607	104713	3.24%	0.455%

41	12.287	1575	1581	1585	rVV5	23158	44962	1.39%	0.195%
42	12.328	1585	1588	1595	rVV	18314	31502	0.97%	0.137%
43	12.522	1609	1621	1632	rBV9	12311	49998	1.55%	0.217%
44	12.692	1645	1650	1657	rBV8	9574	19715	0.61%	0.086%
45	12.828	1669	1673	1676	rVV4	12558	18315	0.57%	0.080%

46	12.869	1677	1680	1688	rVB4	10684	19188	0.59%	0.083%
47	13.051	1707	1711	1715	rVV5	11768	17076	0.53%	0.074%
48	13.122	1718	1723	1730	rVV	53393	80818	2.50%	0.351%
49	13.351	1755	1762	1768	rVB7	16788	36193	1.12%	0.157%
50	13.475	1775	1783	1788	rBV6	22302	56215	1.74%	0.244%

51	13.563	1793	1798	1804	rBV4	11846	19738	0.61%	0.086%
52	13.628	1804	1809	1812	rBV3	22111	43682	1.35%	0.190%
53	13.722	1820	1825	1829	rVB	255302	335672	10.38%	1.459%
54	13.786	1833	1836	1840	rVB4	18493	22989	0.71%	0.100%
55	13.845	1840	1846	1847	rBV6	8594	14860	0.46%	0.065%

56	13.939	1855	1862	1866	rBV4	30986	53531	1.65%	0.233%
57	13.998	1866	1872	1877	rVV	236960	343509	10.62%	1.494%
58	14.210	1902	1908	1913	rVB	214958	317081	9.80%	1.379%
59	14.304	1913	1924	1931	rBV	978121	1547753	47.84%	6.729%
60	14.392	1935	1939	1944	rVB4	17133	27296	0.84%	0.119%

61	14.451	1944	1949	1954	rVB	102027	137036	4.24%	0.596%
62	14.528	1956	1962	1971	rBV8	42895	116200	3.59%	0.505%
63	14.716	1991	1994	1999	rVB4	17086	30383	0.94%	0.132%
64	14.786	2004	2006	2012	rVB2	11410	14512	0.45%	0.063%
65	14.839	2012	2015	2018	rBV5	11855	17189	0.53%	0.075%

66	14.945	2027	2033	2042	rVB	140543	243232	7.52%	1.058%
67	15.016	2042	2045	2050	rVB	27159	34648	1.07%	0.151%
68	15.086	2051	2057	2065	rBV	96468	156591	4.84%	0.681%
69	15.175	2065	2072	2077	rVB3	61128	116395	3.60%	0.506%
70	15.233	2077	2082	2087	rBV8	9511	17772	0.55%	0.077%

71	15.310	2087	2095	2103	rBV	329807	538753	16.65%	2.342%
72	15.439	2109	2117	2124	rBV3	66085	135362	4.18%	0.589%
73	15.586	2138	2142	2150	rVB6	20615	43313	1.34%	0.188%
74	15.692	2155	2160	2166	rVB	55417	89224	2.76%	0.388%
75	15.892	2190	2194	2199	rBV8	9423	19014	0.59%	0.083%

76	15.963	2201	2206	2212	rVB	37609	54975	1.70%	0.239%
----	--------	------	------	------	-----	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022230.D
 Acq On : 04 Oct 2024 15:43
 Operator : RC/JU
 Sample : P3927-08MEDL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DDC93MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

77	16.051	2217	2221	2230	rBV	63345	126080	3.90%	0.548%
78	16.263	2255	2257	2261	rVB4	10621	12845	0.40%	0.056%
79	16.410	2276	2282	2287	rBV7	19703	41241	1.27%	0.179%
80	16.745	2332	2339	2353	rBV	1928630	3235279	100.00%	14.066%
81	16.869	2357	2360	2365	rVV	73699	102552	3.17%	0.446%
82	16.922	2365	2369	2378	rVB3	34804	65145	2.01%	0.283%
83	17.098	2393	2399	2406	rBV	1344743	2080553	64.31%	9.046%
84	17.198	2411	2416	2422	rVV2	394005	617381	19.08%	2.684%
85	17.245	2422	2424	2430	rVB5	25148	32934	1.02%	0.143%
86	17.404	2447	2451	2459	rVB6	21732	49481	1.53%	0.215%
87	17.622	2484	2488	2493	rVB	52161	65939	2.04%	0.287%
88	17.692	2497	2500	2503	rVV	12708	16604	0.51%	0.072%
89	17.739	2503	2508	2515	rVB7	32056	56162	1.74%	0.244%
90	17.810	2516	2520	2524	rBV	51212	66084	2.04%	0.287%
91	18.033	2554	2558	2566	rVB6	30682	62127	1.92%	0.270%
92	18.339	2606	2610	2617	rBV2	41109	60543	1.87%	0.263%
93	19.021	2719	2726	2730	rBV4	44592	89292	2.76%	0.388%
94	19.169	2748	2751	2754	rVB5	17139	18569	0.57%	0.081%
95	19.574	2814	2820	2832	rBV2	452100	791934	24.48%	3.443%
96	20.180	2919	2923	2927	rBV6	39363	61238	1.89%	0.266%
97	21.210	3094	3098	3104	rVB2	78804	112981	3.49%	0.491%
98	21.533	3147	3153	3162	rVB2	1636003	2609696	80.66%	11.346%
99	24.580	3664	3671	3682	rVB2	301680	793135	24.52%	3.448%
100	24.809	3701	3710	3724	rVB	1019339	2839807	87.78%	12.347%


Sum of corrected areas: 23000016

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022230.D
Acq On : 04 Oct 2024 15:43
Operator : RC/JU
Sample : P3927-08MEDL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDC93MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

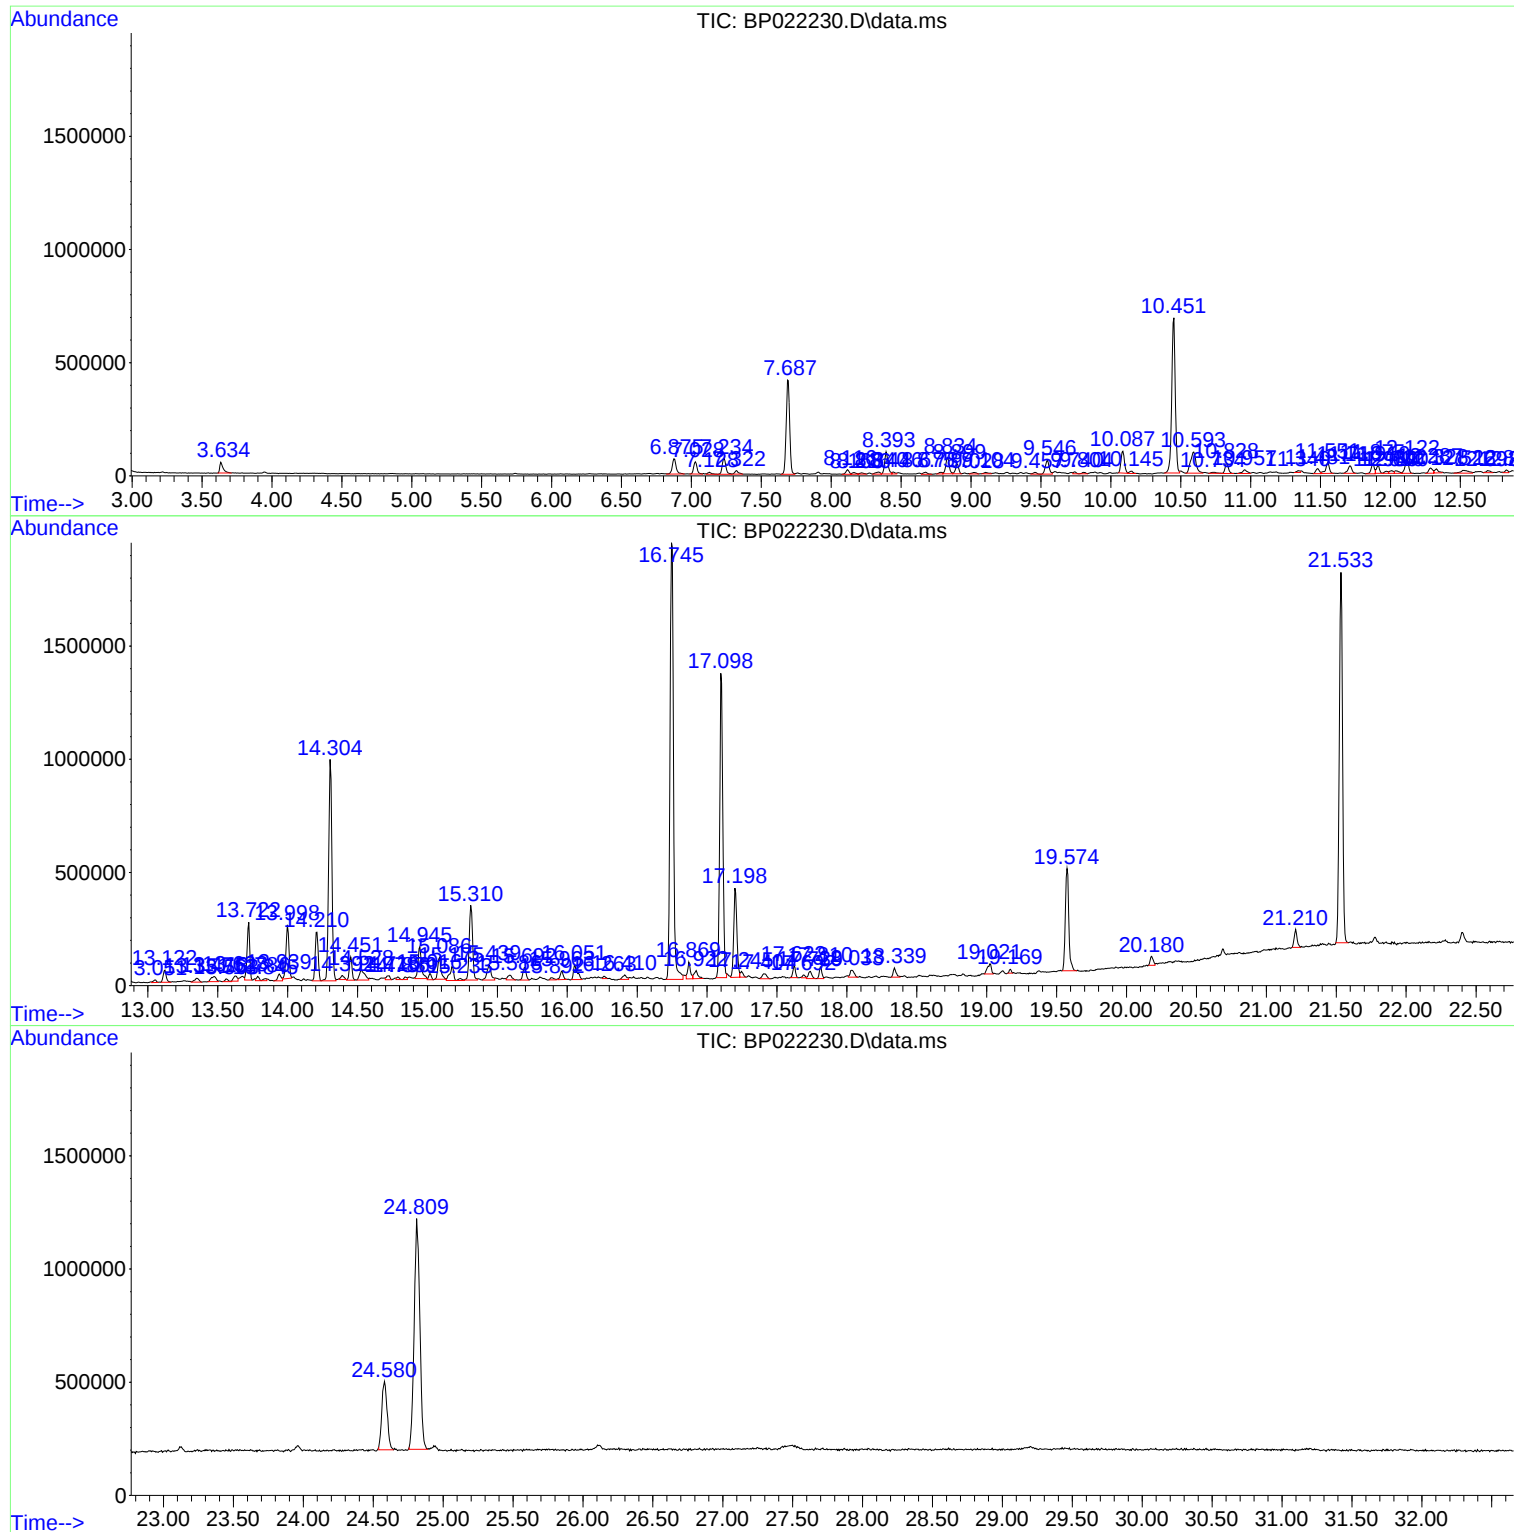

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022230.D
Acq On : 04 Oct 2024 15:43
Operator : RC/JU
Sample : P3927-08MEDL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
DDC93MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
14.210	4.10 ng/ul	317081	Acenaphthene-d10	14.304	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Decane, 5,6-dipropyl-	226	C16H34	119209-20-0	86
2	Nonane, 2,3-dimethyl-	156	C11H24	002884-06-2	80
3	Sulfurous acid, butyl octyl ester	250	C12H26O3S	1000309-17-5	72
4	Dodecane, 2,6,11-trimethyl-	212	C15H32	031295-56-4	72
5	Heneicosane	296	C21H44	000629-94-7	59

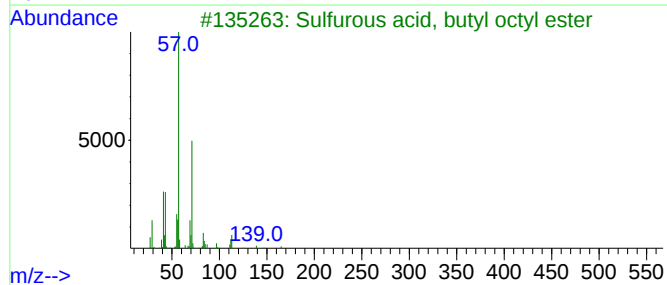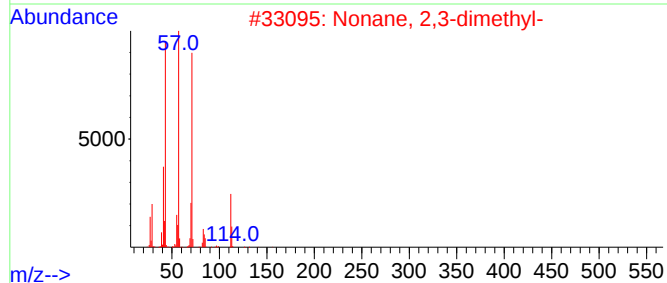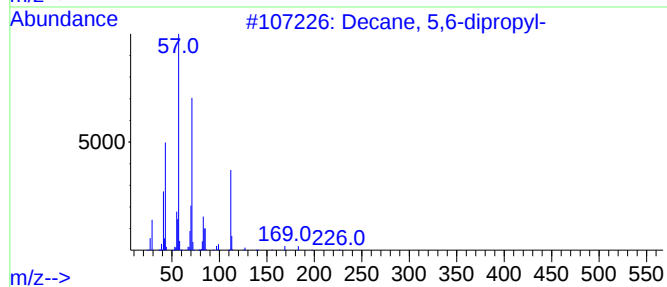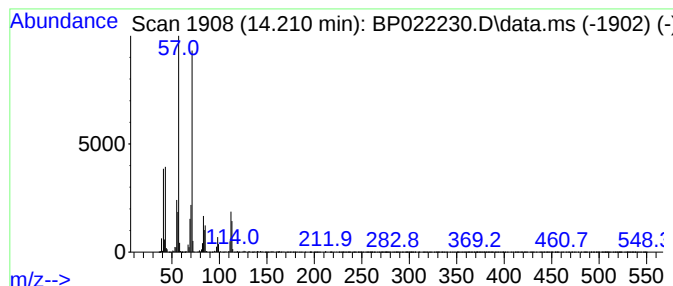

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022230.D
Acq On : 04 Oct 2024 15:43
Operator : RC/JU
Sample : P3927-08MEDL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDC93MEDL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 4,6,8-Trimethylazulene Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.086	2.02 ng/ul	156591	Acenaphthene-d10	14.304

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			4,6,8-Trimethylazulene	170	C13H14	000941-81-1	55
2			Naphthalene, 1,6,7-trimethyl-	170	C13H14	002245-38-7	50
3			Methyl 2-diethylamino-3-methyl-b...	185	C10H19NO2	075122-81-5	50
4			4,6,8-Trimethylazulene	170	C13H14	000941-81-1	46
5			Naphthalene, 1,4,6-trimethyl-	170	C13H14	002131-42-2	45

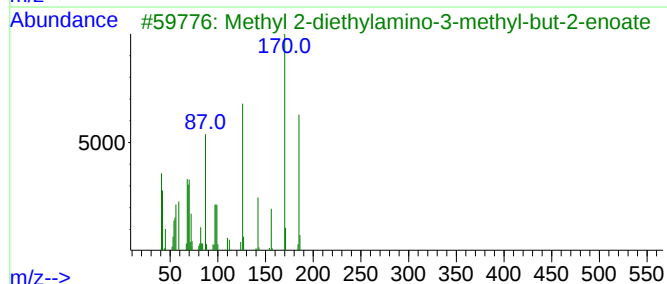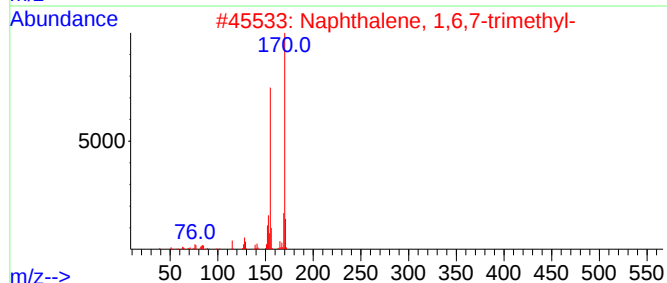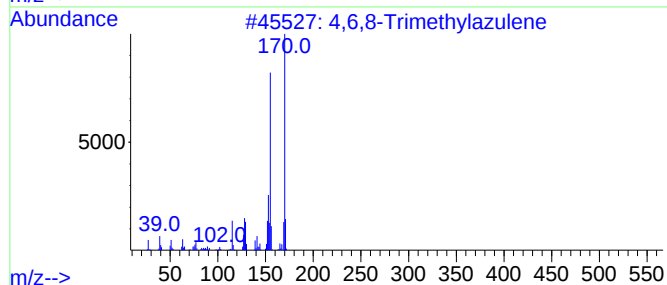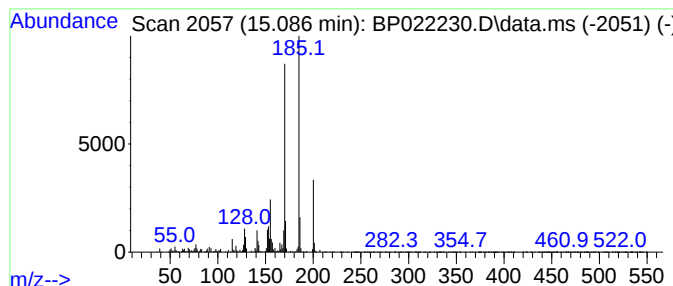

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022230.D
Acq On : 04 Oct 2024 15:43
Operator : RC/JU
Sample : P3927-08MEDL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DDC93MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	14.210	4.1	ng/u1	317081	3	14.304	1547750	20.0
4,6,8-Trimethyl...	15.086	2.0	ng/u1	156591	3	14.304	1547750	20.0