

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022238.D
 Acq On : 04 Oct 2024 21:10
 Operator : RC/JU
 Sample : P4083-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022238.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	37	39	44	rVB5	3161	4125	0.16%	0.027%
2	3.346	58	61	63	rBV3	2371	3121	0.12%	0.021%
3	3.646	107	112	119	rBV4	10377	20578	0.80%	0.136%
4	3.734	122	127	134	rVB	16337	26069	1.01%	0.172%
5	3.811	134	140	144	rVB8	3991	7668	0.30%	0.051%
6	3.952	160	164	169	rVB	7476	12216	0.47%	0.080%
7	4.311	224	225	232	rVB7	1978	3272	0.13%	0.022%
8	4.499	253	257	262	rVB8	2857	4719	0.18%	0.031%
9	4.852	312	317	324	rBV3	12177	21161	0.82%	0.139%
10	6.581	606	611	616	rVB8	1617	3784	0.15%	0.025%
11	6.881	654	662	676	rVB3	34468	75733	2.93%	0.499%
12	7.034	683	688	697	rVB	57616	90945	3.52%	0.599%
13	7.240	716	723	731	rBV	60925	105318	4.08%	0.694%
14	7.316	734	736	743	rVB8	3082	5335	0.21%	0.035%
15	7.693	793	800	813	rBV	504419	771793	29.89%	5.085%
16	8.399	913	920	928	rBV2	26045	48901	1.89%	0.322%
17	8.505	932	938	947	rVV	41215	72089	2.79%	0.475%
18	8.628	956	959	963	rVB5	2007	2740	0.11%	0.018%
19	8.834	986	994	1002	rBV	63874	120622	4.67%	0.795%
20	9.240	1060	1063	1070	rVB8	1940	3415	0.13%	0.022%
21	9.393	1084	1089	1096	rBV9	3570	7154	0.28%	0.047%
22	9.546	1109	1115	1124	rBV	50364	90739	3.51%	0.598%
23	9.716	1136	1144	1155	rBV5	6511	19454	0.75%	0.128%
24	9.899	1171	1175	1180	rBV3	5963	8677	0.34%	0.057%
25	9.952	1180	1184	1192	rVB4	3970	6619	0.26%	0.044%
26	10.081	1199	1206	1221	rBV	64880	139444	5.40%	0.919%
27	10.446	1261	1268	1279	rBV	588915	1055062	40.86%	6.951%
28	10.593	1286	1293	1299	rBV2	33600	61096	2.37%	0.402%
29	10.993	1352	1361	1368	rBV2	5757	14200	0.55%	0.094%
30	11.946	1518	1523	1529	rBV9	2044	4372	0.17%	0.029%
31	12.034	1533	1538	1542	rVB9	2108	3533	0.14%	0.023%
32	12.510	1615	1619	1623	rBV6	1299	2723	0.11%	0.018%
33	13.257	1744	1746	1753	rVB8	2102	3243	0.13%	0.021%
34	13.704	1815	1822	1834	rBV	186632	287451	11.13%	1.894%
35	13.987	1863	1870	1881	rBV	204782	317165	12.28%	2.089%
36	14.298	1915	1923	1932	rBV	1011122	1567964	60.72%	10.330%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022238.D
 Acq On : 04 Oct 2024 21:10
 Operator : RC/JU
 Sample : P4083-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

37	14.428	1943	1945	1953	rVB9	2049	3316	0.13%	0.022%
38	14.557	1962	1967	1975	rBV10	7863	21011	0.81%	0.138%
39	14.710	1985	1993	1996	rBV9	2790	6550	0.25%	0.043%
40	14.745	1996	1999	2004	rVB7	4227	5380	0.21%	0.035%
41	15.310	2088	2095	2102	rBV	279356	456830	17.69%	3.010%
42	15.440	2111	2117	2126	rBV2	26683	52808	2.05%	0.348%
43	15.563	2130	2138	2139	rBV8	2285	4636	0.18%	0.031%
44	15.587	2139	2142	2145	rVB5	3060	3777	0.15%	0.025%
45	15.681	2151	2158	2164	rBV	190359	257494	9.97%	1.696%
46	16.263	2252	2257	2262	rVV	33255	43475	1.68%	0.286%
47	16.592	2311	2313	2317	rBV5	2177	2714	0.11%	0.018%
48	16.639	2317	2321	2325	rVV7	3990	6074	0.24%	0.040%
49	16.751	2336	2340	2349	rVB7	6861	13408	0.52%	0.088%
50	16.828	2349	2353	2355	rBV5	2271	3258	0.13%	0.021%
51	16.928	2367	2370	2375	rVB5	4988	7159	0.28%	0.047%
52	16.981	2375	2379	2383	rBV6	5278	8364	0.32%	0.055%
53	17.104	2392	2400	2405	rBV	1231567	2062271	79.86%	13.586%
54	17.145	2405	2407	2413	rVV	68766	98258	3.81%	0.647%
55	17.210	2413	2418	2430	rVV	291023	487355	18.87%	3.211%
56	17.298	2430	2433	2440	rVB8	9590	18317	0.71%	0.121%
57	17.534	2466	2473	2475	rBV6	4574	9268	0.36%	0.061%
58	17.622	2486	2488	2490	rBV2	3628	3453	0.13%	0.023%
59	17.728	2500	2506	2511	rVB10	13297	27824	1.08%	0.183%
60	17.804	2516	2519	2523	rVB6	6025	7341	0.28%	0.048%
61	17.910	2534	2537	2546	rBV6	5688	13653	0.53%	0.090%
62	18.034	2552	2558	2568	rBV3	78466	138892	5.38%	0.915%
63	18.110	2568	2571	2582	rVB2	12481	22144	0.86%	0.146%
64	18.210	2583	2588	2592	rBV6	14458	30562	1.18%	0.201%
65	18.286	2599	2601	2605	rVB3	5727	4257	0.16%	0.028%
66	18.322	2605	2607	2611	rBV4	6177	8571	0.33%	0.056%
67	18.757	2678	2681	2689	rVB10	14520	30024	1.16%	0.198%
68	18.928	2705	2710	2715	rBV8	13483	27956	1.08%	0.184%
69	19.233	2757	2762	2767	rVB	150104	209586	8.12%	1.381%
70	19.375	2783	2786	2793	rBV5	23908	37588	1.46%	0.248%
71	19.580	2816	2821	2825	rBV2	348423	576980	22.34%	3.801%
72	20.186	2921	2924	2928	rBV5	26645	31919	1.24%	0.210%
73	21.210	3095	3098	3104	rVB3	80602	115388	4.47%	0.760%
74	21.539	3147	3154	3160	rBV	1498207	2475927	95.88%	16.311%
75	24.592	3668	3673	3681	rVB	130540	270740	10.48%	1.784%
76	24.821	3703	3712	3725	rVB	960772	2582241	100.00%	17.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022238.D
Acq On : 04 Oct 2024 21:10
Operator : RC/JU
Sample : P4083-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EK3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 15179269

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022238.D
Acq On : 04 Oct 2024 21:10
Operator : RC/JU
Sample : P4083-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

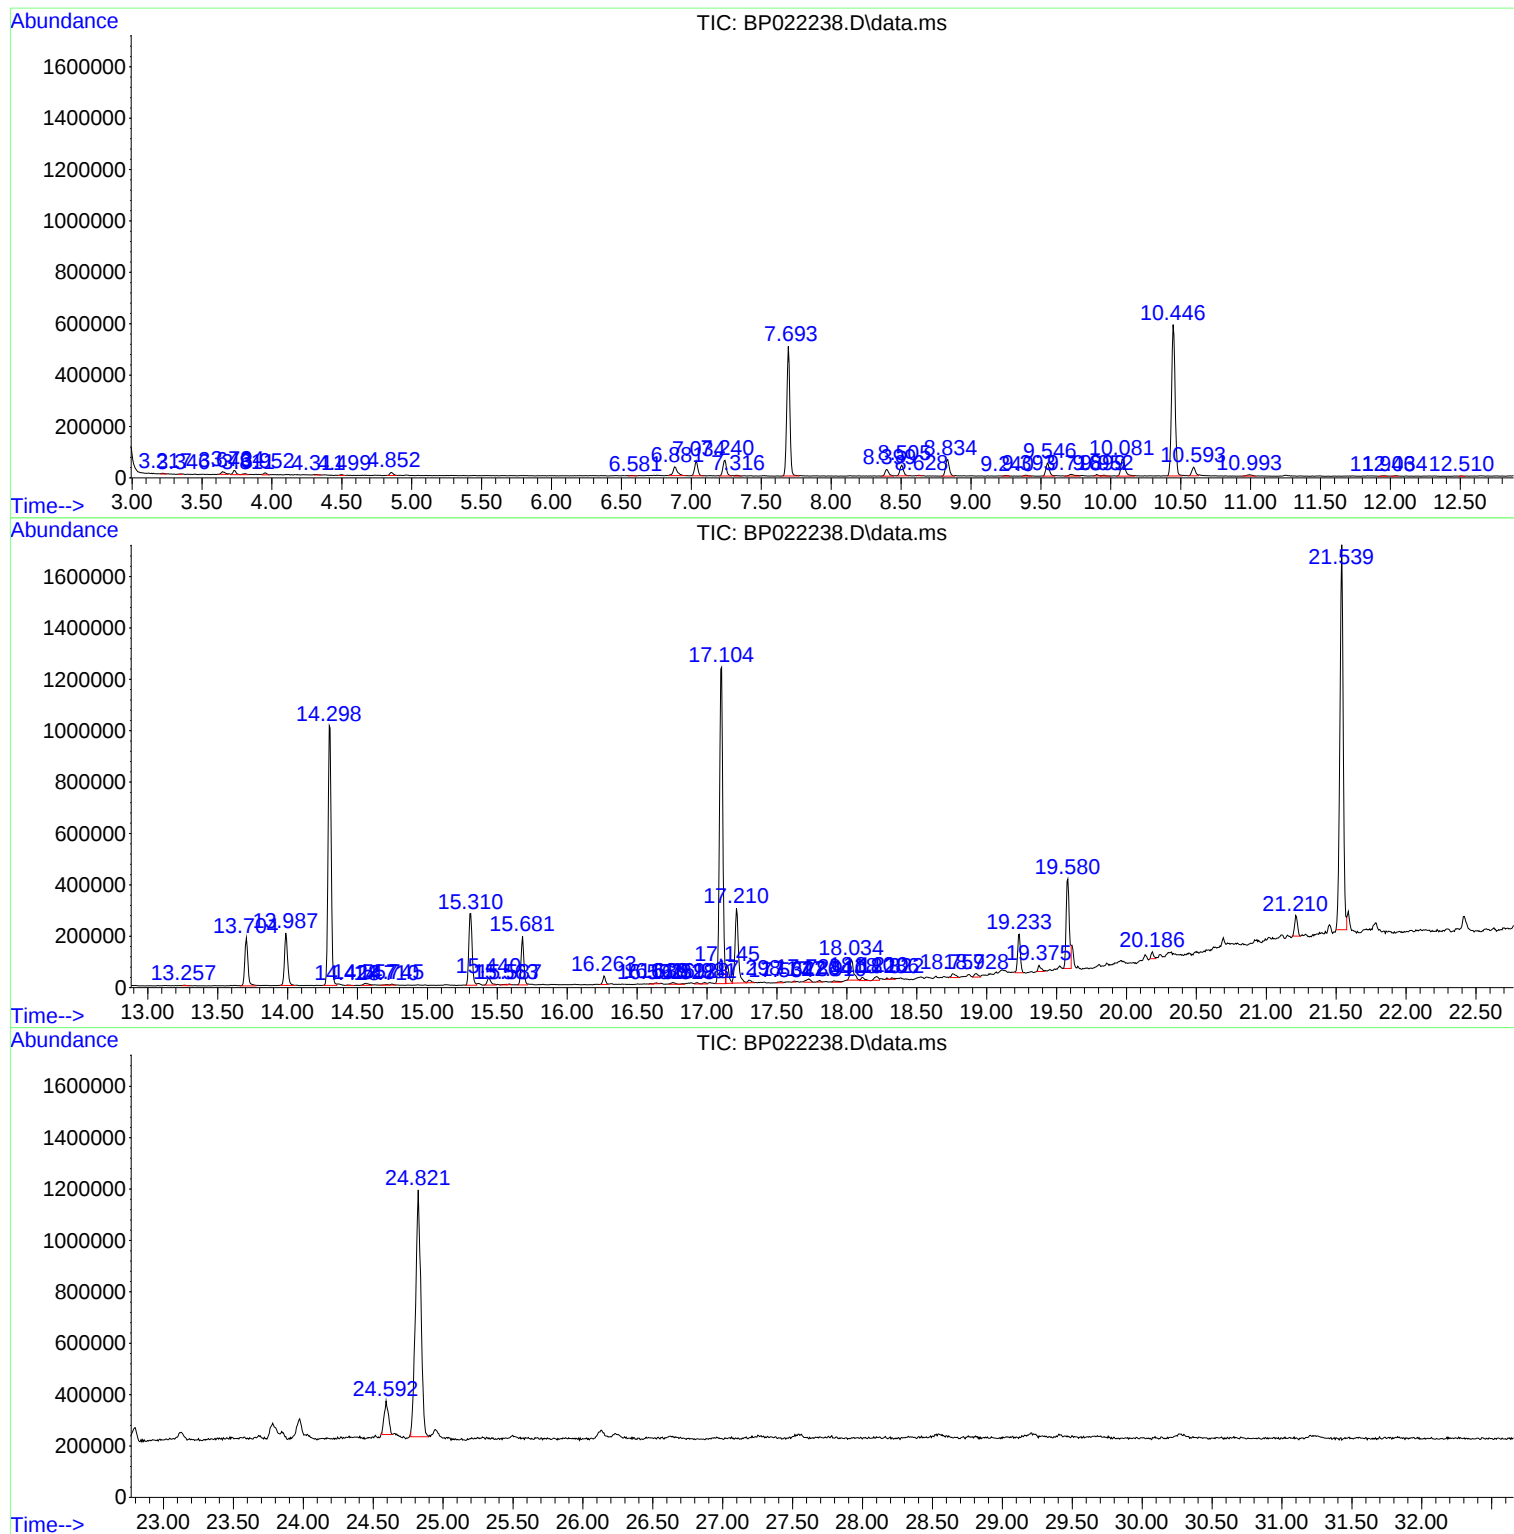

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022238.D
Acq On : 04 Oct 2024 21:10
Operator : RC/JU
Sample : P4083-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EK3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.681	3.28 ng/ul	257494	Acenaphthene-d10	14.304

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	90
4			Benzophenone	182	C13H10O	000119-61-9	89
5			Benzophenone	182	C13H10O	000119-61-9	87

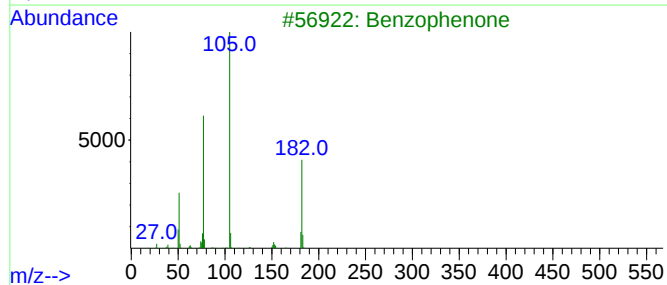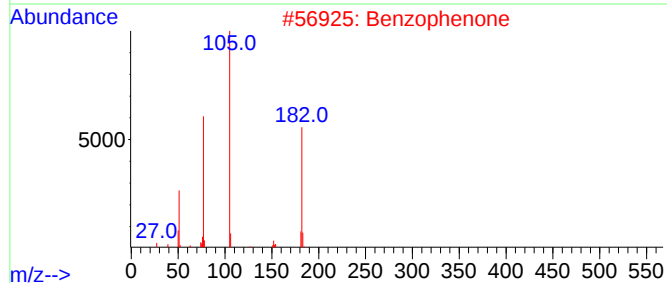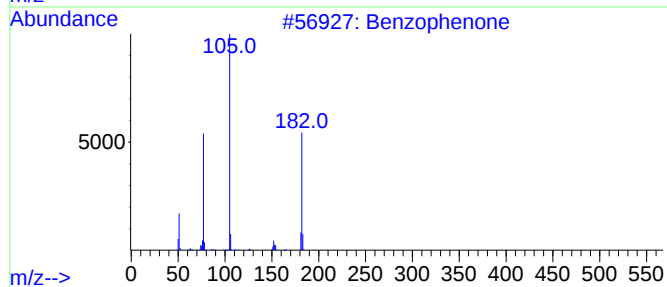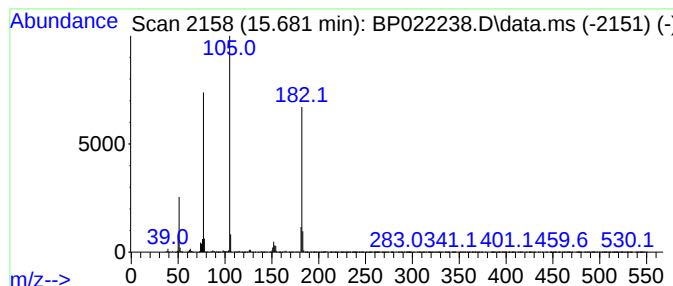

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022238.D
Acq On : 04 Oct 2024 21:10
Operator : RC/JU
Sample : P4083-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.681	3.3	ng/u1	257494	3	14.304	1567960	20.0