

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
 Data File : BP022242.D
 Acq On : 05 Oct 2024 00:35
 Operator : RC/JU
 Sample : PB163912BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK912

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	34	38	45	rVB	22641	32457	1.25%	0.122%
2	3.628	104	109	124	rBV	276120	454579	17.56%	1.708%
3	3.952	159	164	171	rVB2	6920	11979	0.46%	0.045%
4	4.793	304	307	313	rBV7	1277	2685	0.10%	0.010%
5	6.875	652	661	676	rBV	354377	582878	22.51%	2.190%
6	7.028	680	687	696	rBV	254998	419595	16.21%	1.576%
7	7.228	714	721	737	rVB	380584	597821	23.09%	2.246%
8	7.693	792	800	809	rBV	390688	642926	24.83%	2.415%
9	8.387	911	918	928	rBV	465930	733920	28.34%	2.757%
10	8.828	984	993	1005	rBV	377394	580807	22.43%	2.182%
11	9.546	1106	1115	1133	rBV	282582	507809	19.61%	1.908%
12	10.075	1197	1205	1218	rBV	455491	802890	31.01%	3.016%
13	10.452	1260	1269	1277	rBV	495406	859034	33.18%	3.227%
14	10.593	1284	1293	1307	rBV	418334	736609	28.45%	2.767%
15	12.040	1533	1539	1547	rBV2	7526	14755	0.57%	0.055%
16	13.275	1744	1749	1753	rBV8	1601	3025	0.12%	0.011%
17	13.710	1816	1823	1835	rBV	1026831	1266863	48.93%	4.759%
18	13.993	1864	1871	1892	rBV	959225	1378537	53.24%	5.178%
19	14.304	1917	1924	1937	rBV	756662	1283170	49.56%	4.820%
20	14.534	1955	1963	1976	rBV2	179622	486315	18.78%	1.827%
21	14.628	1976	1979	1987	rVV9	13118	34350	1.33%	0.129%
22	14.710	1991	1993	2002	rVB9	4232	8867	0.34%	0.033%
23	15.316	2089	2096	2105	rBV	1324108	1831189	70.72%	6.879%
24	15.434	2111	2116	2126	rBV	330466	425043	16.42%	1.597%
25	15.557	2133	2137	2143	rVB9	6138	10539	0.41%	0.040%
26	16.110	2227	2231	2235	rVB7	1922	2590	0.10%	0.010%
27	16.769	2341	2343	2346	rVB4	2688	2976	0.11%	0.011%
28	16.881	2357	2362	2368	rBV7	3272	5343	0.21%	0.020%
29	17.098	2393	2399	2409	rVV	1199167	1686718	65.14%	6.336%
30	17.198	2409	2416	2430	rVV	1230897	2090936	80.75%	7.855%
31	17.398	2448	2450	2457	rVB7	2144	3665	0.14%	0.014%
32	19.128	2740	2744	2750	rBV5	17305	31601	1.22%	0.119%
33	19.204	2753	2757	2763	rVB	21731	31462	1.22%	0.118%
34	19.575	2814	2820	2829	rBV	1901114	2510297	96.95%	9.430%
35	21.533	3147	3153	3162	rVB	1244478	1938919	74.88%	7.284%
36	24.574	3662	3670	3685	rVB	1111599	2589273	100.00%	9.727%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022242.D
Acq On : 05 Oct 2024 00:35
Operator : RC/JU
Sample : PB163912BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK912

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Title : SVOA CALIBRATION

37	24.798	3700	3708	3721	rVB	745669	2018163	77.94%	7.581%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 26620585

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022242.D
Acq On : 05 Oct 2024 00:35
Operator : RC/JU
Sample : PB163912BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK912

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

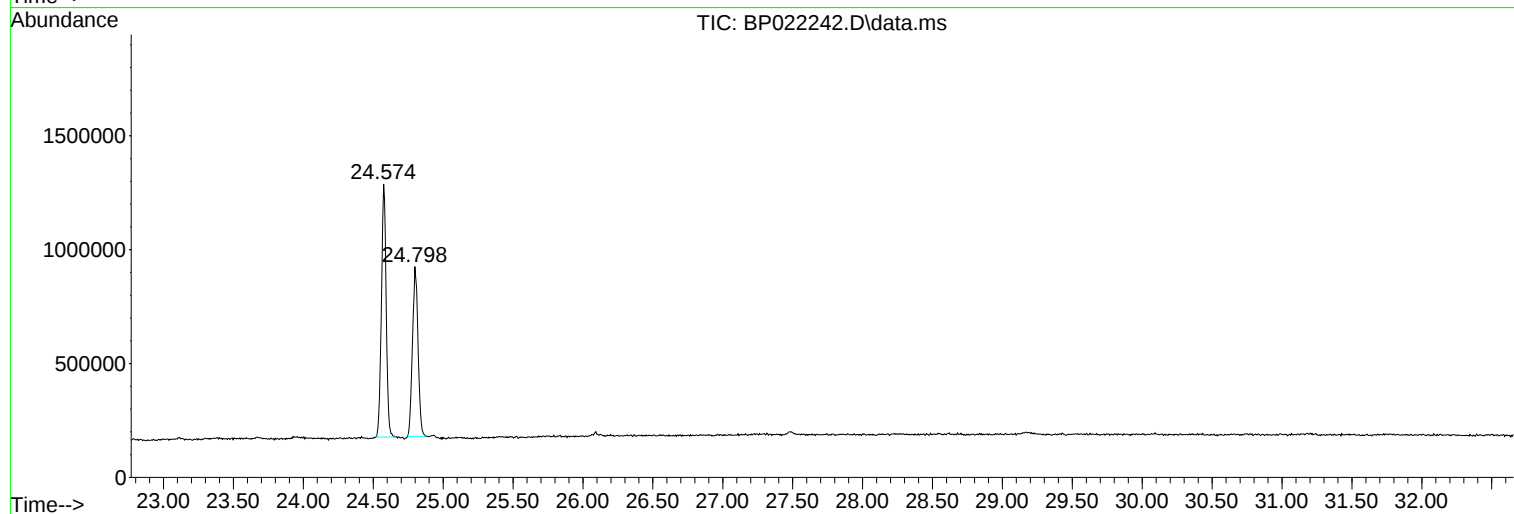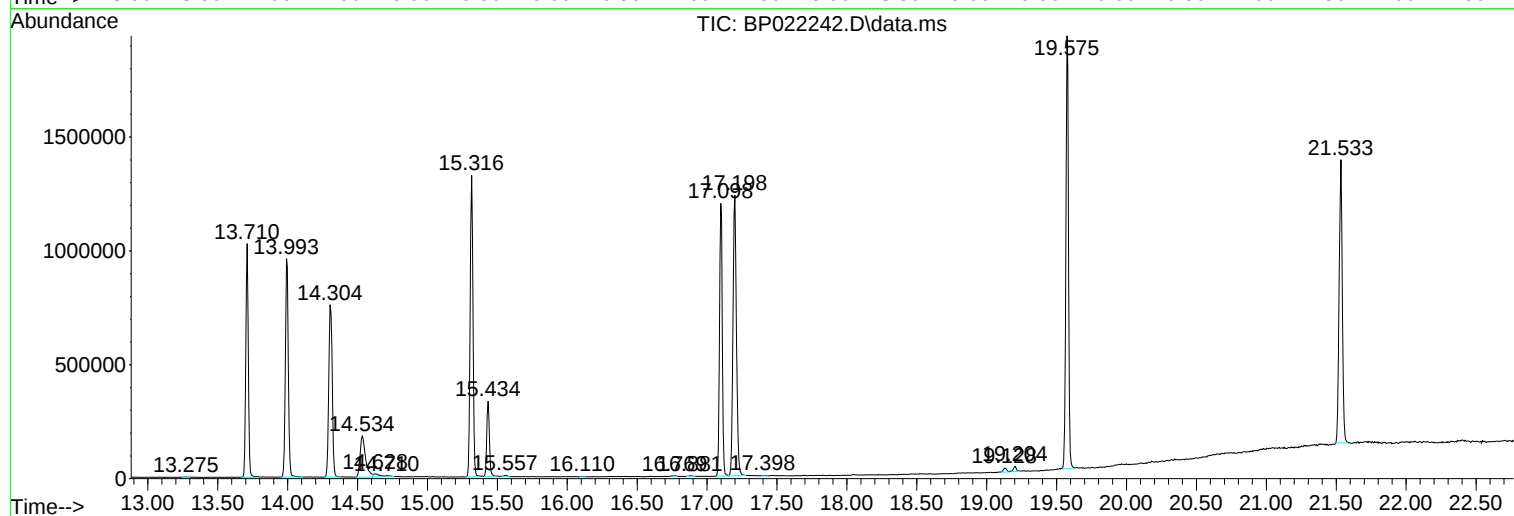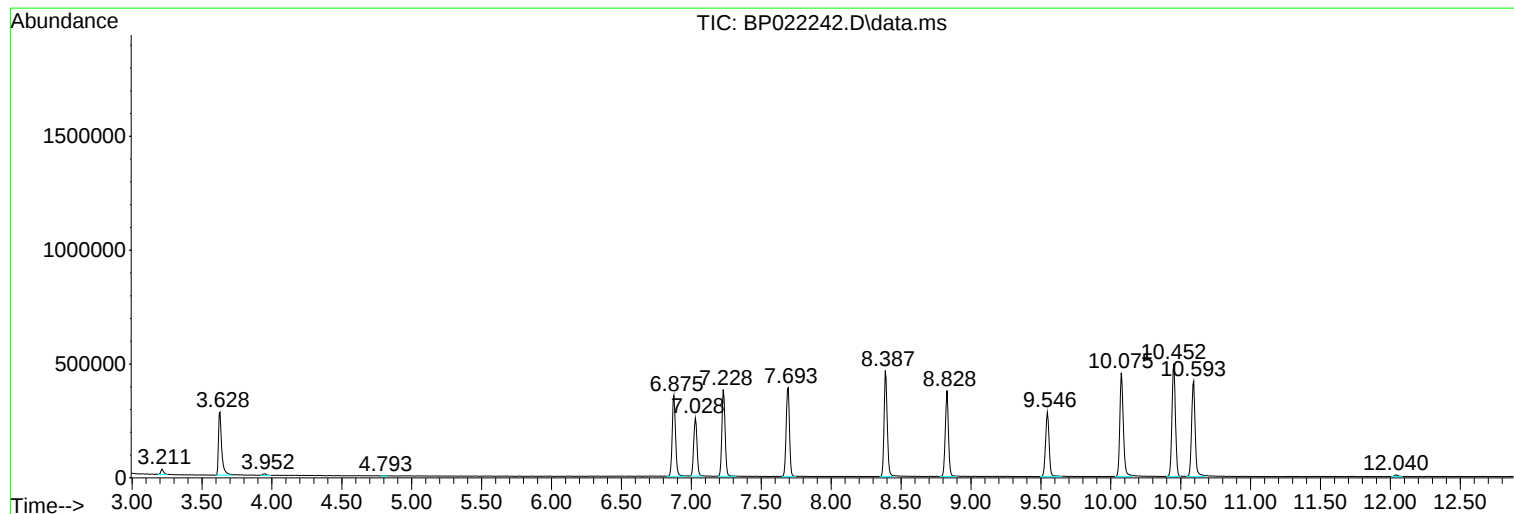

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022242.D
Acq On : 05 Oct 2024 00:35
Operator : RC/JU
Sample : PB163912BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK912

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100424\
Data File : BP022242.D
Acq On : 05 Oct 2024 00:35
Operator : RC/JU
Sample : PB163912BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK912

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------