

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
 Data File : BP003489.D
 Acq On : 05 Oct 2020 14:27
 Operator : CG/JU
 Sample : PB132085BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132085BL

Quant Time: Oct 05 15:52:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 14:33:14 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.499	152	82456	20.00	ng	0.00
21) Naphthalene-d8	10.281	136	316643	20.00	ng	# 0.00
39) Acenaphthene-d10	14.163	164	178283	20.00	ng	0.00
64) Phenanthrene-d10	16.922	188	355904	20.00	ng	# 0.00
76) Chrysene-d12	21.028	240	345318	20.00	ng	0.00
86) Perylene-d12	23.198	264	360786	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.111	112	704865	149.27	ng	0.00
7) Phenol-d6	6.705	99	863715	137.22	ng	0.00
23) Nitrobenzene-d5	8.652	82	594744	110.35	ng	0.00
42) 2,4,6-Tribromophenol	15.663	330	262116	96.39	ng	0.00
45) 2-Fluorobiphenyl	12.775	172	1197589	98.24	ng	0.00
79) Terphenyl-d14	19.504	244	1518457	91.62	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
Data File : BP003489.D
Acq On : 05 Oct 2020 14:27
Operator : CG/JU
Sample : PB132085BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132085BL

Quant Time: Oct 05 15:52:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

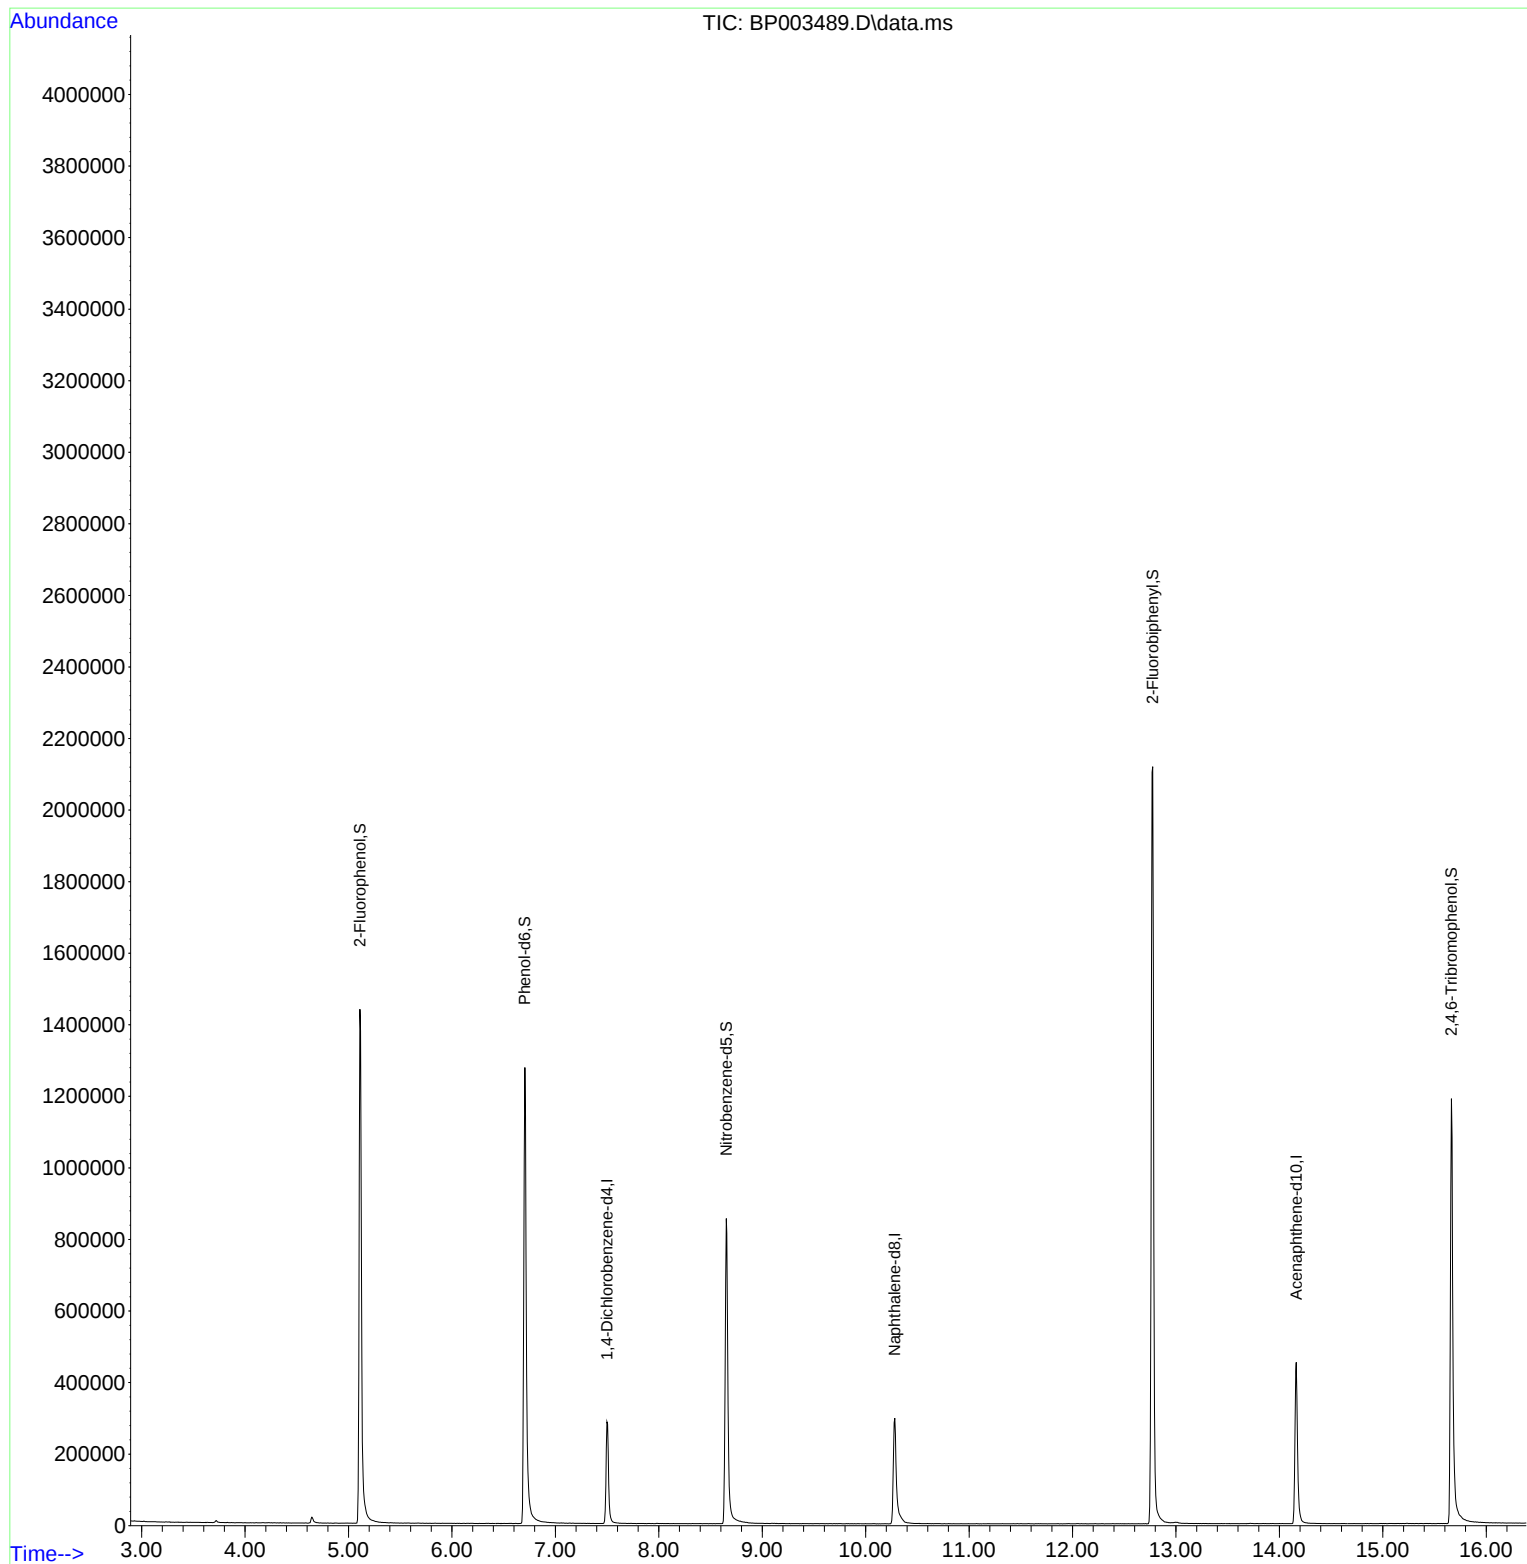

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
Data File : BP003489.D
Acq On : 05 Oct 2020 14:27
Operator : CG/JU
Sample : PB132085BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132085BL

Quant Time: Oct 05 15:52:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

