

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
 Data File : BP003493.D
 Acq On : 05 Oct 2020 16:46
 Operator : CG/JU
 Sample : L4242-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PAV-B17-100120-0-10

Quant Time: Oct 05 17:54:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 14:33:14 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.499	152	90538	20.00	ng	0.00
21) Naphthalene-d8	10.281	136	360200	20.00	ng	# 0.00
39) Acenaphthene-d10	14.157	164	225443	20.00	ng	0.00
64) Phenanthrene-d10	16.916	188	495847	20.00	ng	# 0.00
76) Chrysene-d12	21.027	240	570640	20.00	ng	0.00
86) Perylene-d12	23.198	264	594787	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.116	112	724439	139.72	ng	0.00
7) Phenol-d6	6.710	99	835932	120.95	ng	0.00
23) Nitrobenzene-d5	8.652	82	692335	112.92	ng	0.00
42) 2,4,6-Tribromophenol	15.663	330	432980	125.92	ng	0.00
45) 2-Fluorobiphenyl	12.769	172	1420999	92.19	ng	0.00
79) Terphenyl-d14	19.504	244	2390668	87.29	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
Data File : BP003493.D
Acq On : 05 Oct 2020 16:46
Operator : CG/JU
Sample : L4242-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PAV-B17-100120-0-10


Quant Time: Oct 05 17:54:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

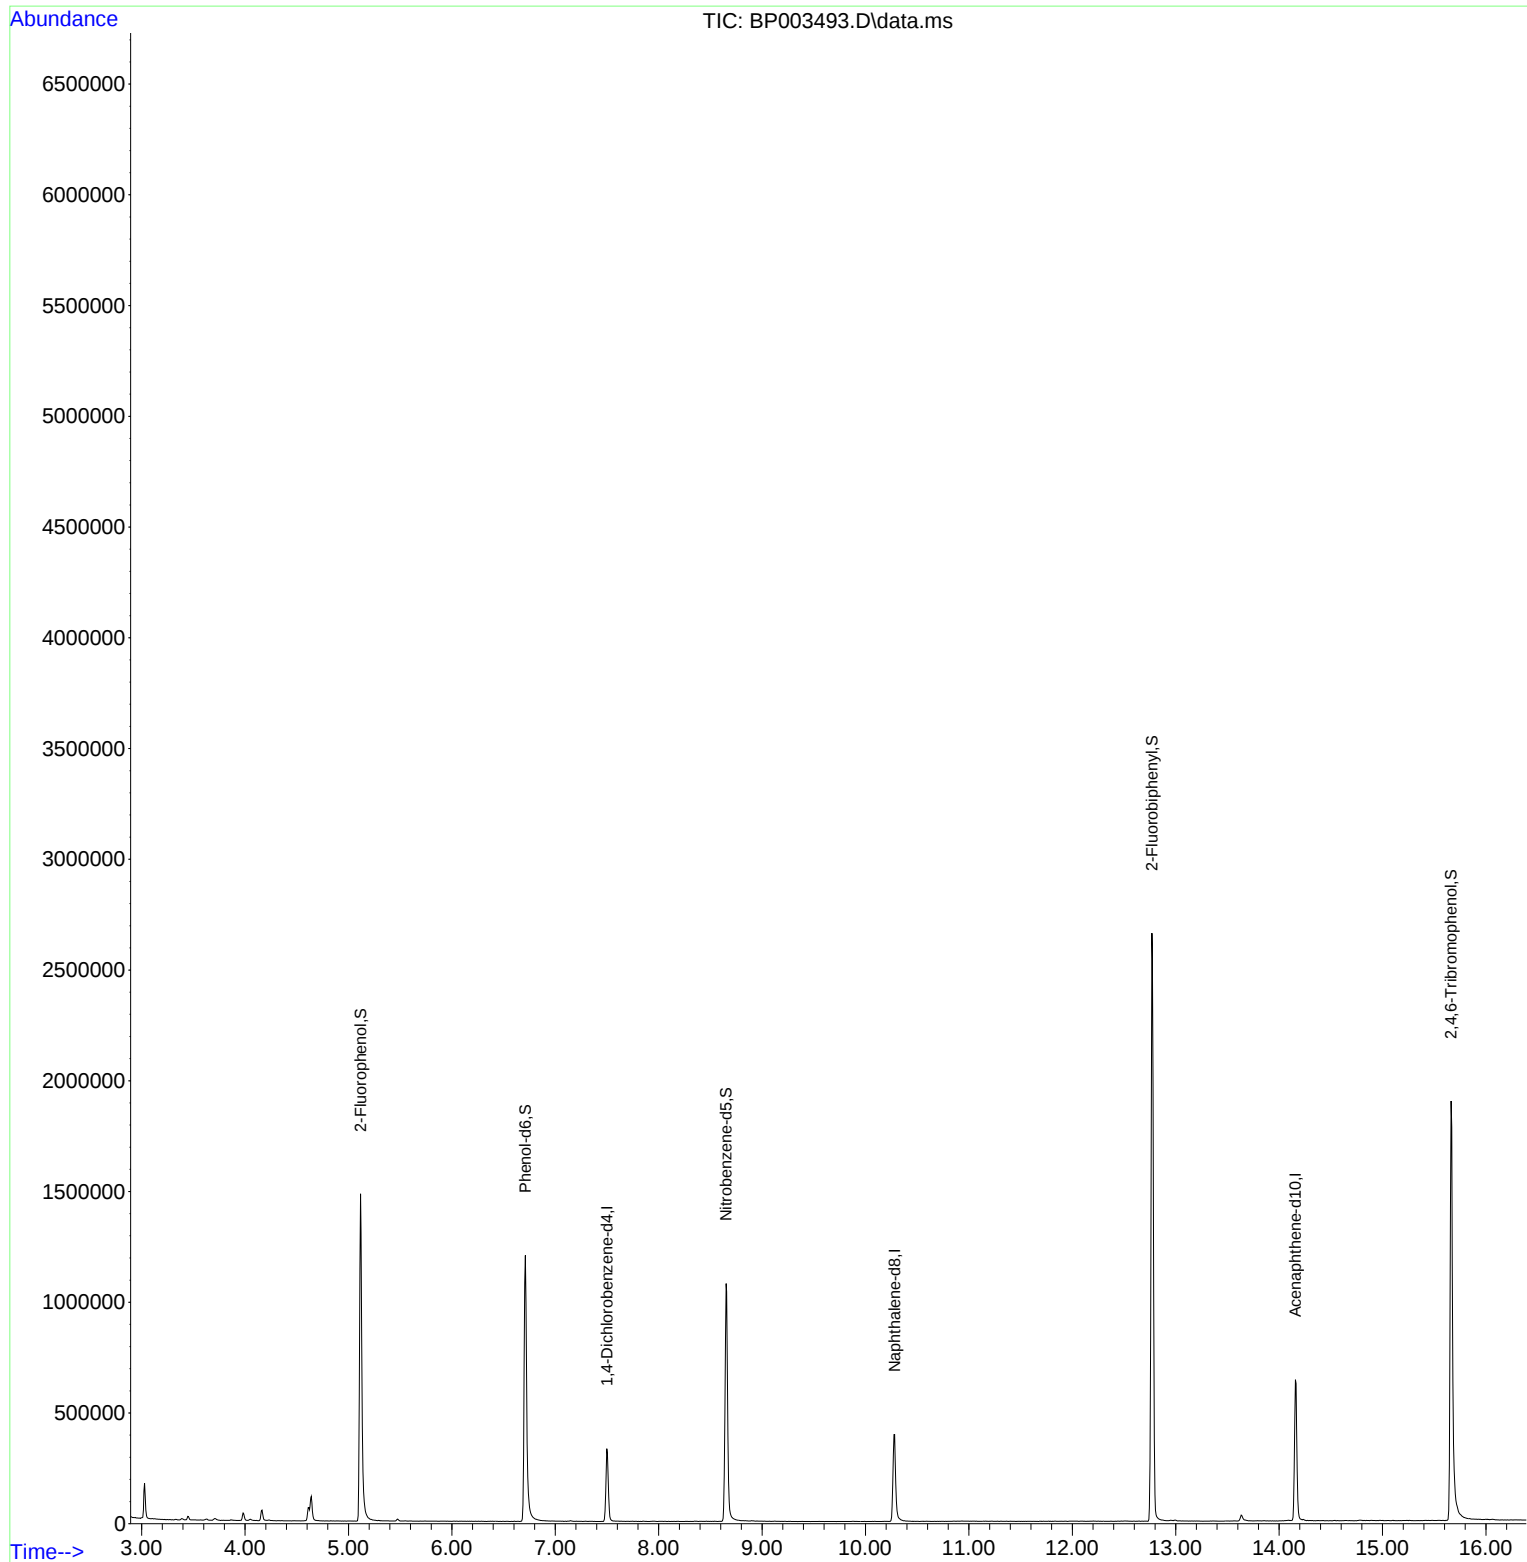

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
Data File : BP003493.D
Acq On : 05 Oct 2020 16:46
Operator : CG/JU
Sample : L4242-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PAV-B17-100120-0-10

Quant Time: Oct 05 17:54:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration




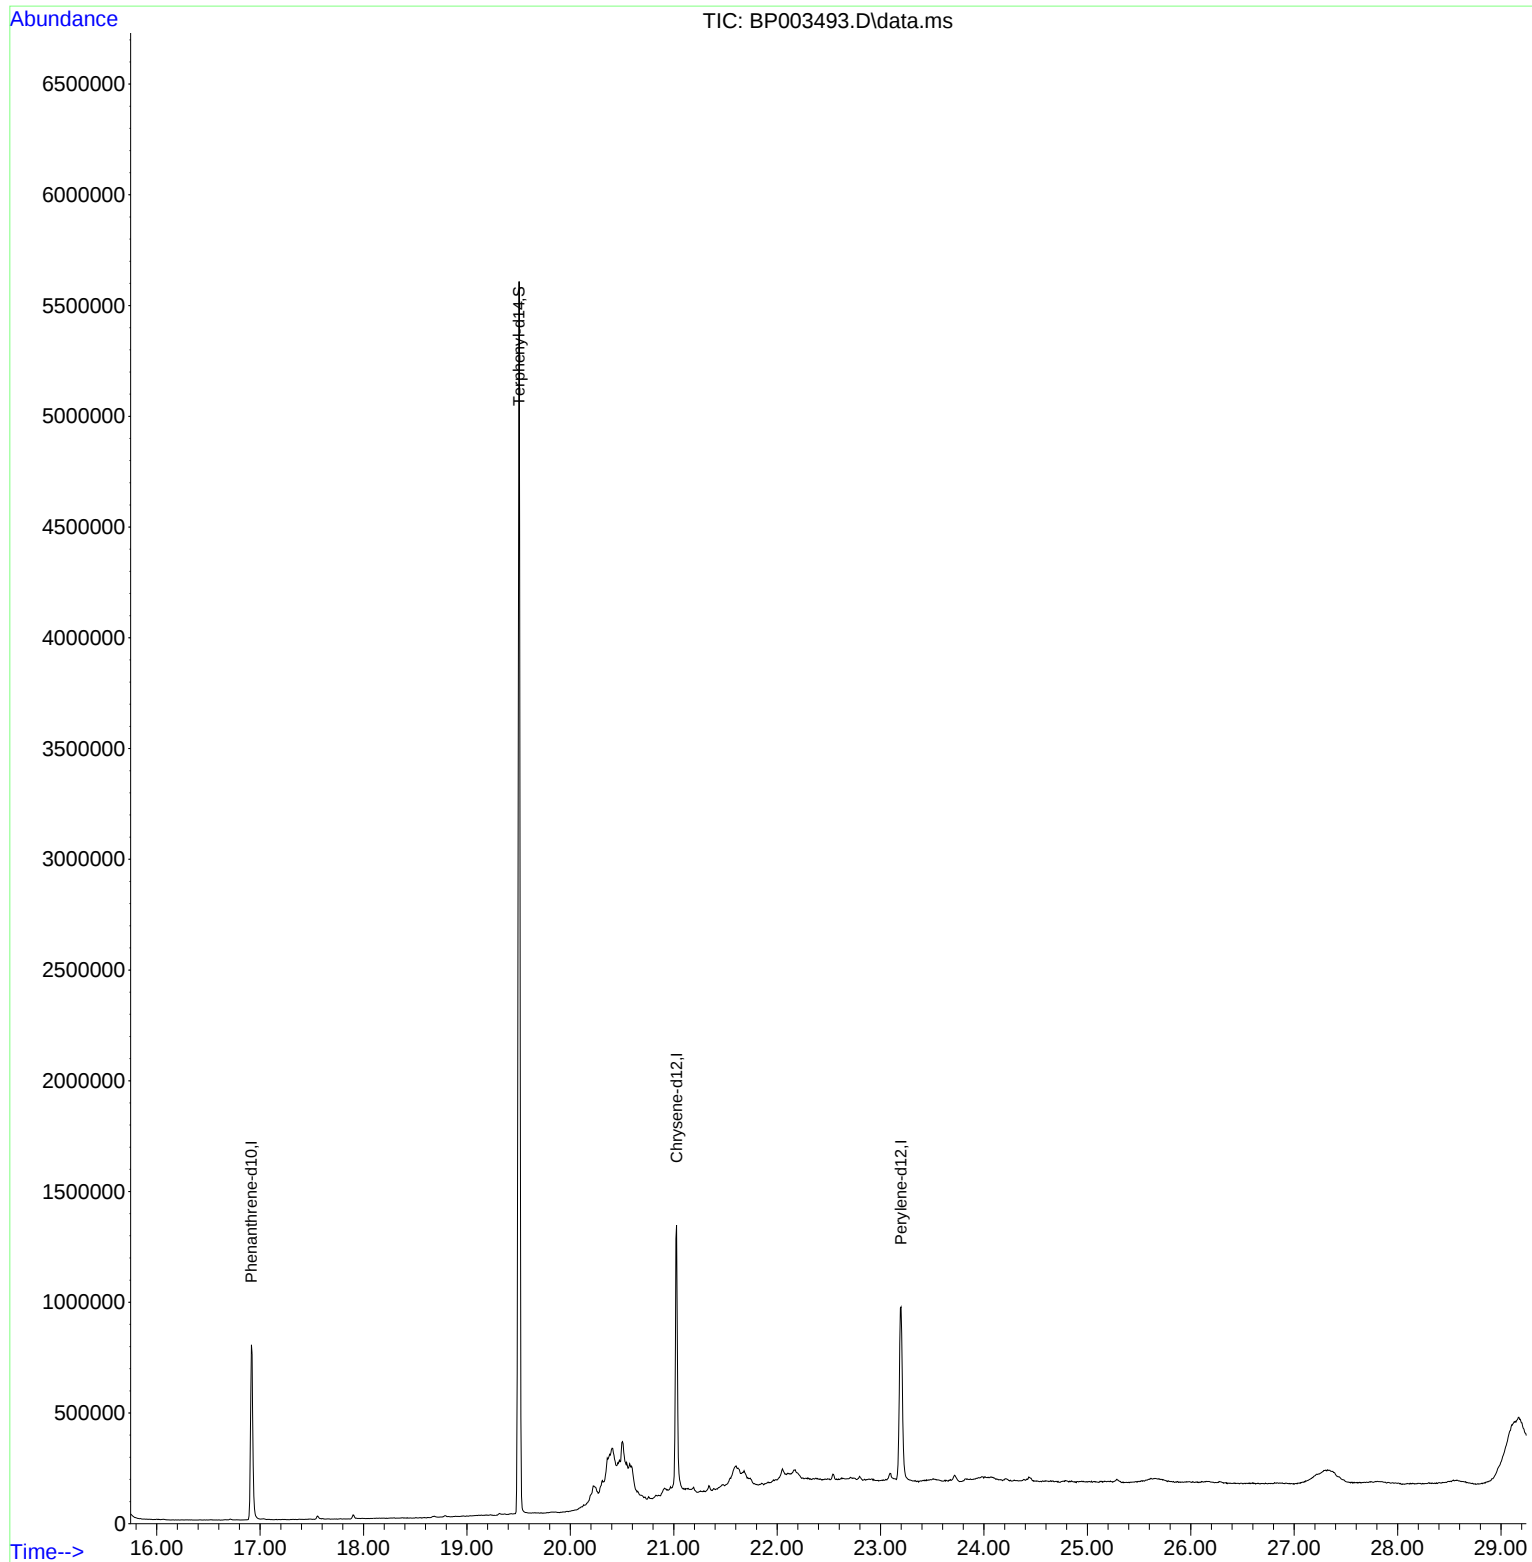




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.499 min Scan# 784
Delta R.T. 0.001 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46




Instrument :
BNA_P
ClientSampleId :
PAV-B17-100120-0-10


Tgt Ion:152 Resp: 90538
Ion Ratio Lower Upper
152 100
150 156.2 123.8 185.6
115 63.2 43.8 65.6

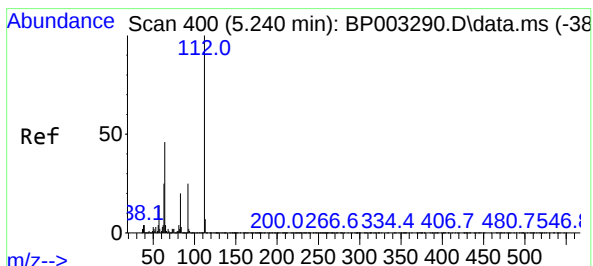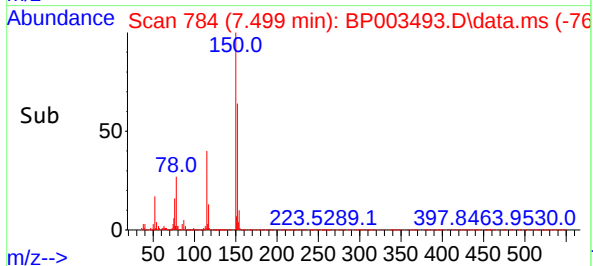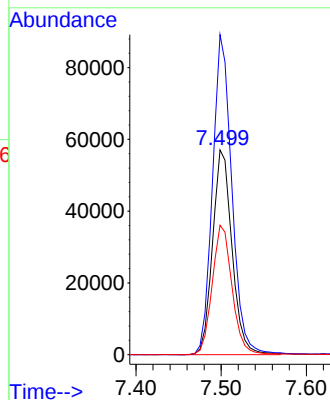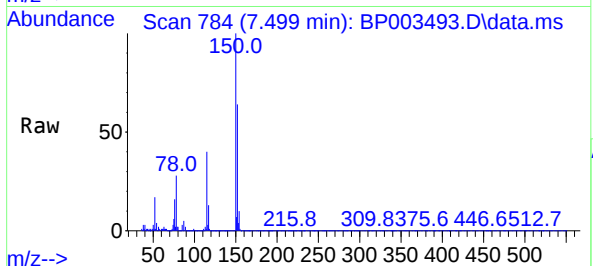

#5
2-Fluorophenol
Concen: 139.72 ng
RT: 5.116 min Scan# 379
Delta R.T. 0.006 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46

Tgt Ion:112 Resp: 724439
Ion Ratio Lower Upper
112 100
64 50.8 32.8 49.2#
63 27.8 17.0 25.4#


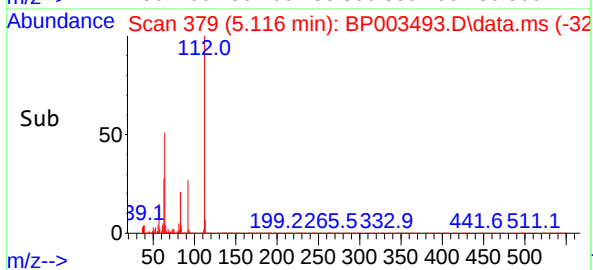
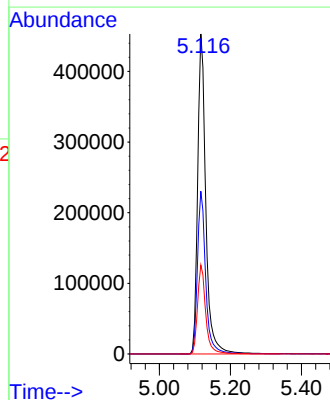
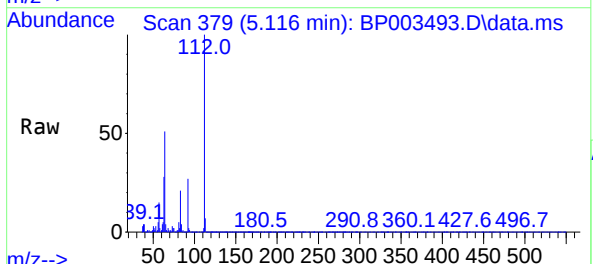


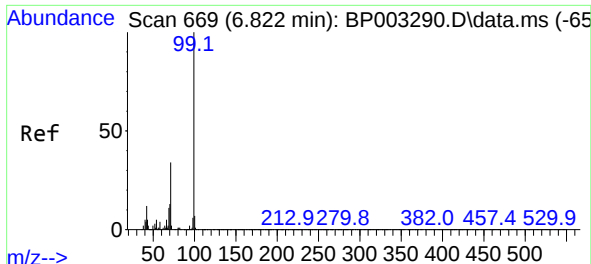

#7
Phenol-d6
Concen: 120.95 ng
RT: 6.710 min Scan# 650
Delta R.T. 0.006 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46




Instrument :
BNA_P
ClientSampleId :
PAV-B17-100120-0-10


Tgt Ion: 99 Resp: 835932
Ion Ratio Lower Upper
99 100
42 12.8 8.6 13.0
71 36.1 23.4 35.2#

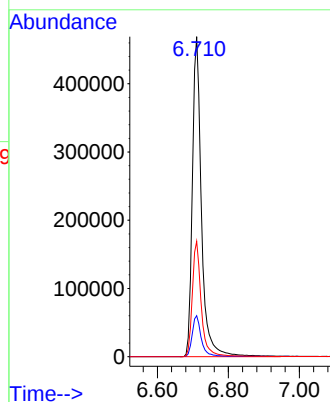

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.281 min Scan# 1257
Delta R.T. 0.006 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46

Tgt Ion: 136 Resp: 360200
Ion Ratio Lower Upper
136 100
137 10.9 8.6 13.0
54 5.6 3.6 5.4#
68 6.0 3.3 4.9#


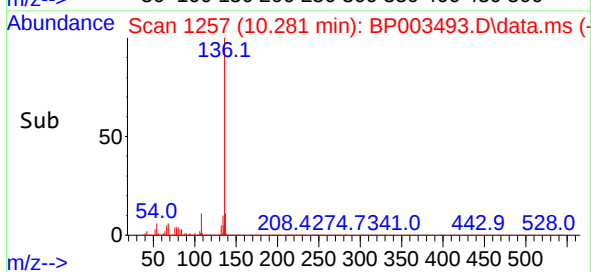
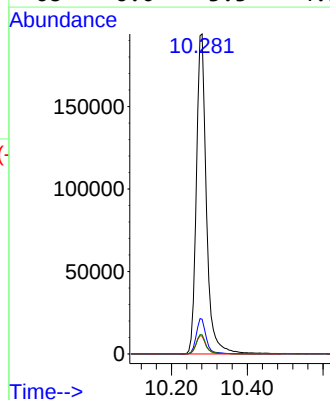
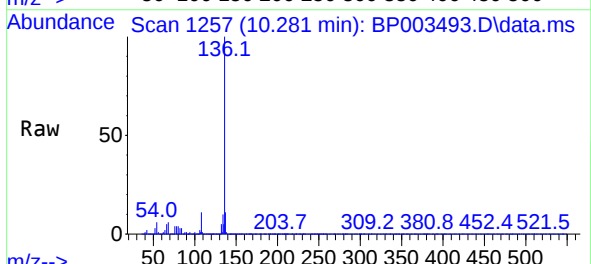


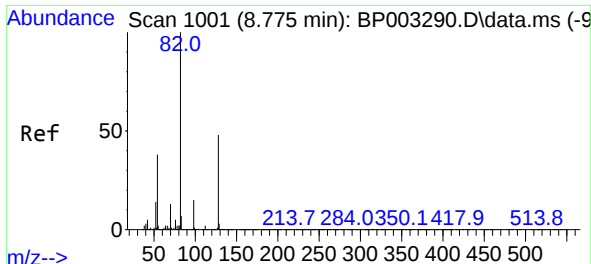

#23
Nitrobenzene-d5
Concen: 112.92 ng
RT: 8.652 min Scan# 980
Delta R.T. 0.000 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46




Instrument :
BNA_P
ClientSampleId :
PAV-B17-100120-0-10


Tgt Ion: 82 Resp: 692335
Ion Ratio Lower Upper
82 100
128 42.2 45.6 68.4#
54 38.0 30.1 45.1

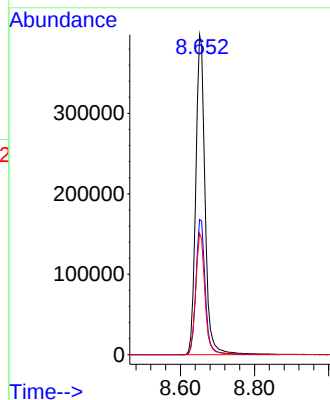

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.157 min Scan# 1916
Delta R.T. 0.000 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46

Tgt Ion: 164 Resp: 225443
Ion Ratio Lower Upper
164 100
162 101.0 79.4 119.2
160 44.2 36.1 54.1


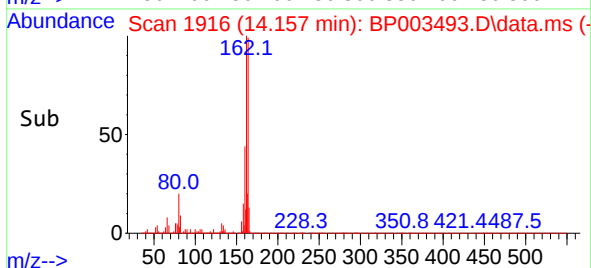
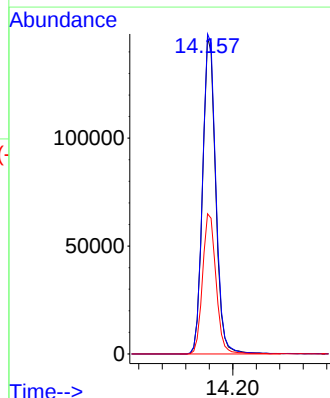
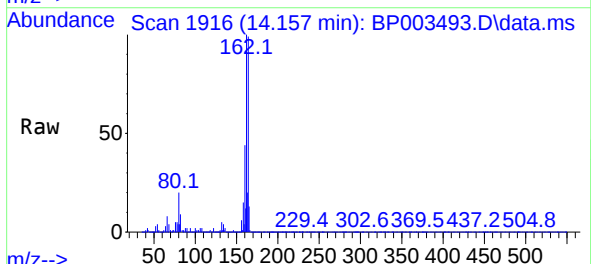


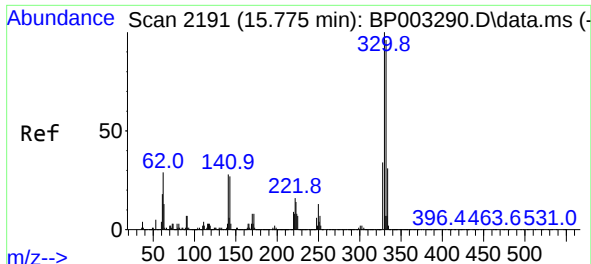

#42
2,4,6-Tribromophenol
Concen: 125.92 ng
RT: 15.663 min Scan# 2172
Delta R.T. 0.000 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46




Instrument :
BNA_P
ClientSampleId :
PAV-B17-100120-0-10


Tgt Ion:330 Resp: 432980
Ion Ratio Lower Upper
330 100
332 96.7 77.1 115.7
141 36.2 23.4 35.2#

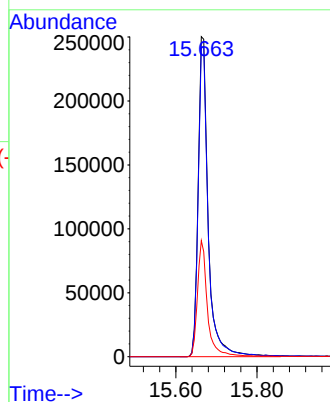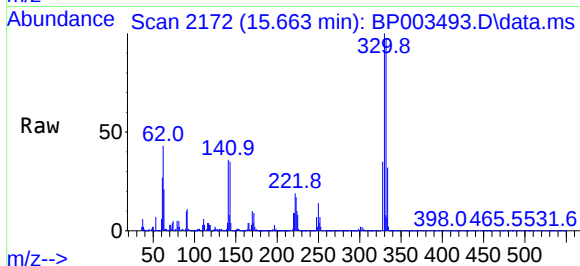

#45
2-Fluorobiphenyl
Concen: 92.19 ng
RT: 12.769 min Scan# 1680
Delta R.T. -0.006 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46

Tgt Ion:172 Resp: 1420999
Ion Ratio Lower Upper
172 100
171 35.8 28.5 42.7
170 23.7 19.2 28.8


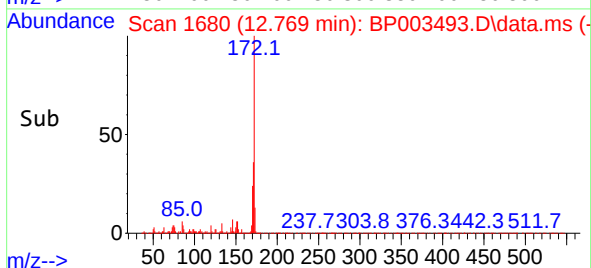
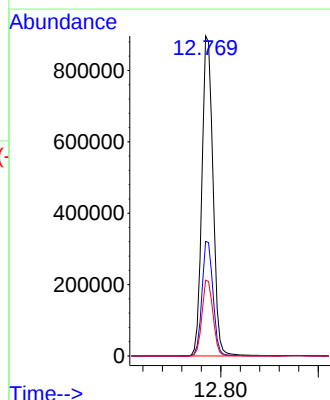
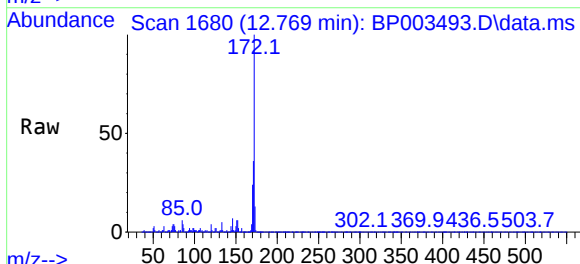




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.916 min Scan# 2385
Delta R.T. 0.000 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46




Instrument :
BNA_P
ClientSampleId :
PAV-B17-100120-0-10


Tgt Ion:188 Resp: 495847
Ion Ratio Lower Upper
188 100
94 9.5 6.2 9.2#
80 10.6 6.2 9.2#

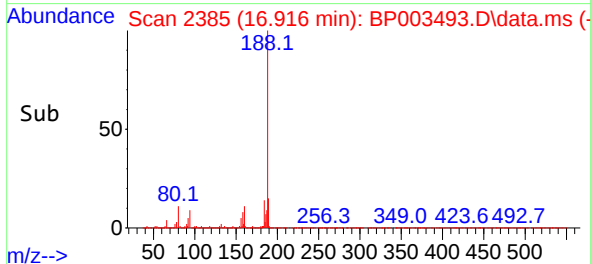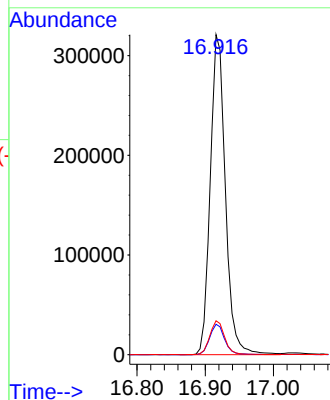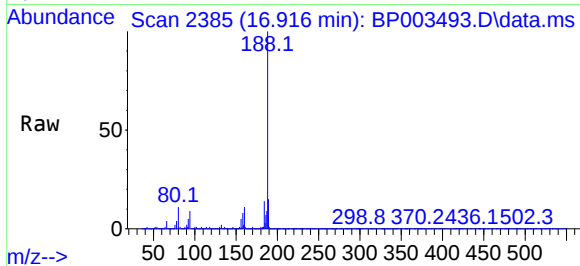

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.027 min Scan# 3084
Delta R.T. 0.000 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46

Tgt Ion:240 Resp: 570640
Ion Ratio Lower Upper
240 100
120 10.1 7.8 11.6
236 26.6 20.8 31.2

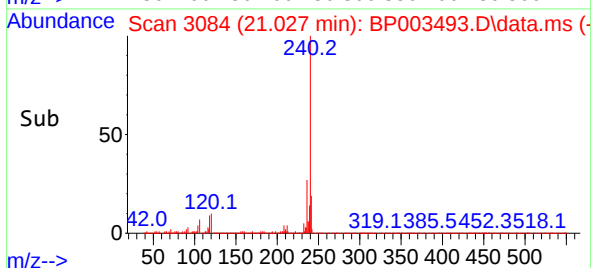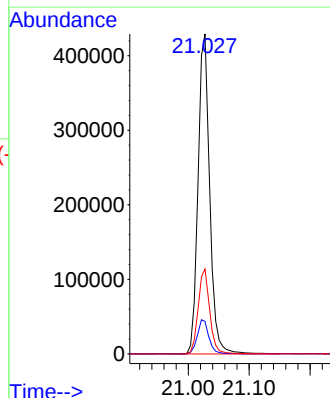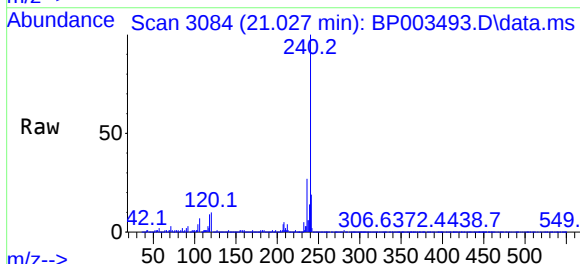







#79
Terphenyl-d14
Concen: 87.29 ng
RT: 19.504 min Scan# 2825
Delta R.T. 0.000 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46

Instrument :
BNA_P
ClientSampleId :
PAV-B17-100120-0-10

Tgt Ion:244 Resp: 2390668

Ion	Ratio	Lower	Upper
244	100		
212	7.7	5.8	8.6
122	8.5	7.8	11.8

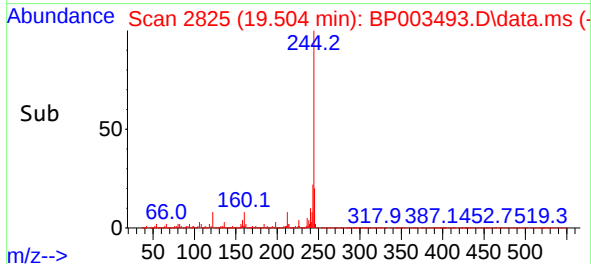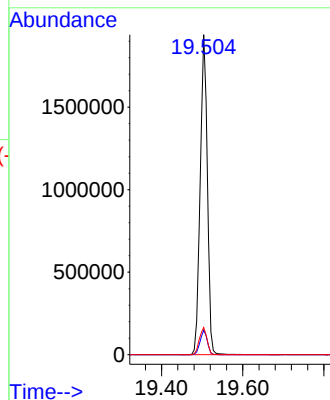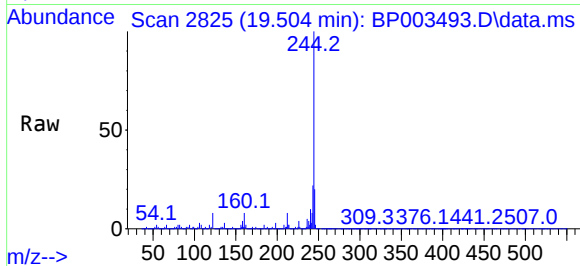

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.198 min Scan# 3453
Delta R.T. 0.000 min
Lab File: BP003493.D
Acq: 05 Oct 2020 16:46

Tgt Ion:264 Resp: 594787

Ion	Ratio	Lower	Upper
264	100		
260	24.6	18.8	28.2
265	21.4	17.4	26.2

