

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
 Data File : BP003496.D
 Acq On : 05 Oct 2020 18:29
 Operator : CG/JU
 Sample : L4221-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OK-02-100120

Quant Time: Oct 06 04:18:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 14:33:14 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.499	152	95925	20.00	ng	0.00
21) Naphthalene-d8	10.275	136	383951	20.00	ng	# 0.00
39) Acenaphthene-d10	14.157	164	238714	20.00	ng	0.00
64) Phenanthrene-d10	16.916	188	533890	20.00	ng	# 0.00
76) Chrysene-d12	21.027	240	610821	20.00	ng	0.00
86) Perylene-d12	23.198	264	561405	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.116	112	710532	129.34	ng	0.00
7) Phenol-d6	6.710	99	875939	119.62	ng	0.00
23) Nitrobenzene-d5	8.652	82	733635	112.25	ng	0.00
42) 2,4,6-Tribromophenol	15.663	330	466878	128.23	ng	0.00
45) 2-Fluorobiphenyl	12.775	172	1506035	92.27	ng	0.00
79) Terphenyl-d14	19.504	244	2549775	86.98	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
Data File : BP003496.D
Acq On : 05 Oct 2020 18:29
Operator : CG/JU
Sample : L4221-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-02-100120


Quant Time: Oct 06 04:18:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

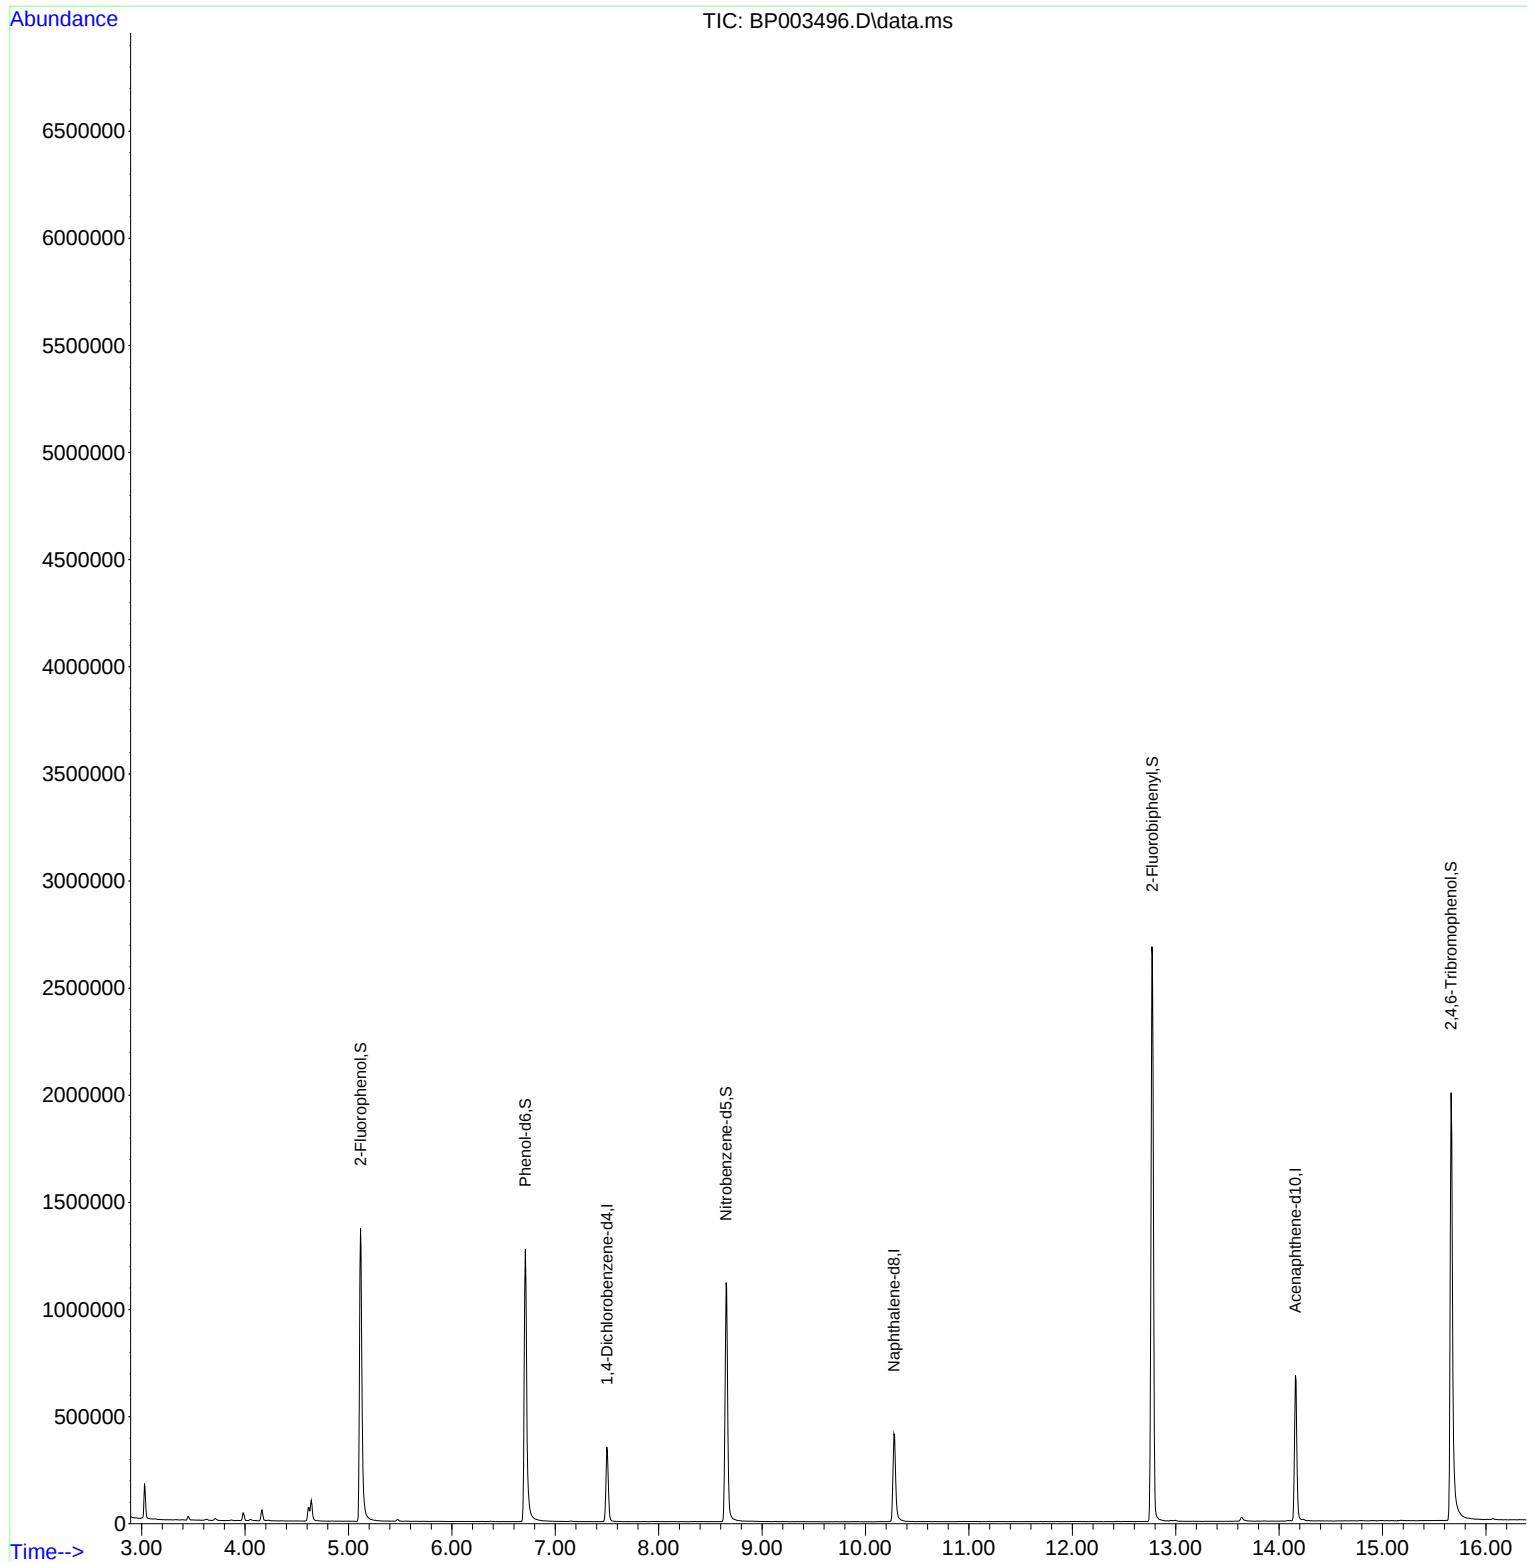

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
Data File : BP003496.D
Acq On : 05 Oct 2020 18:29
Operator : CG/JU
Sample : L4221-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-02-100120

Quant Time: Oct 06 04:18:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

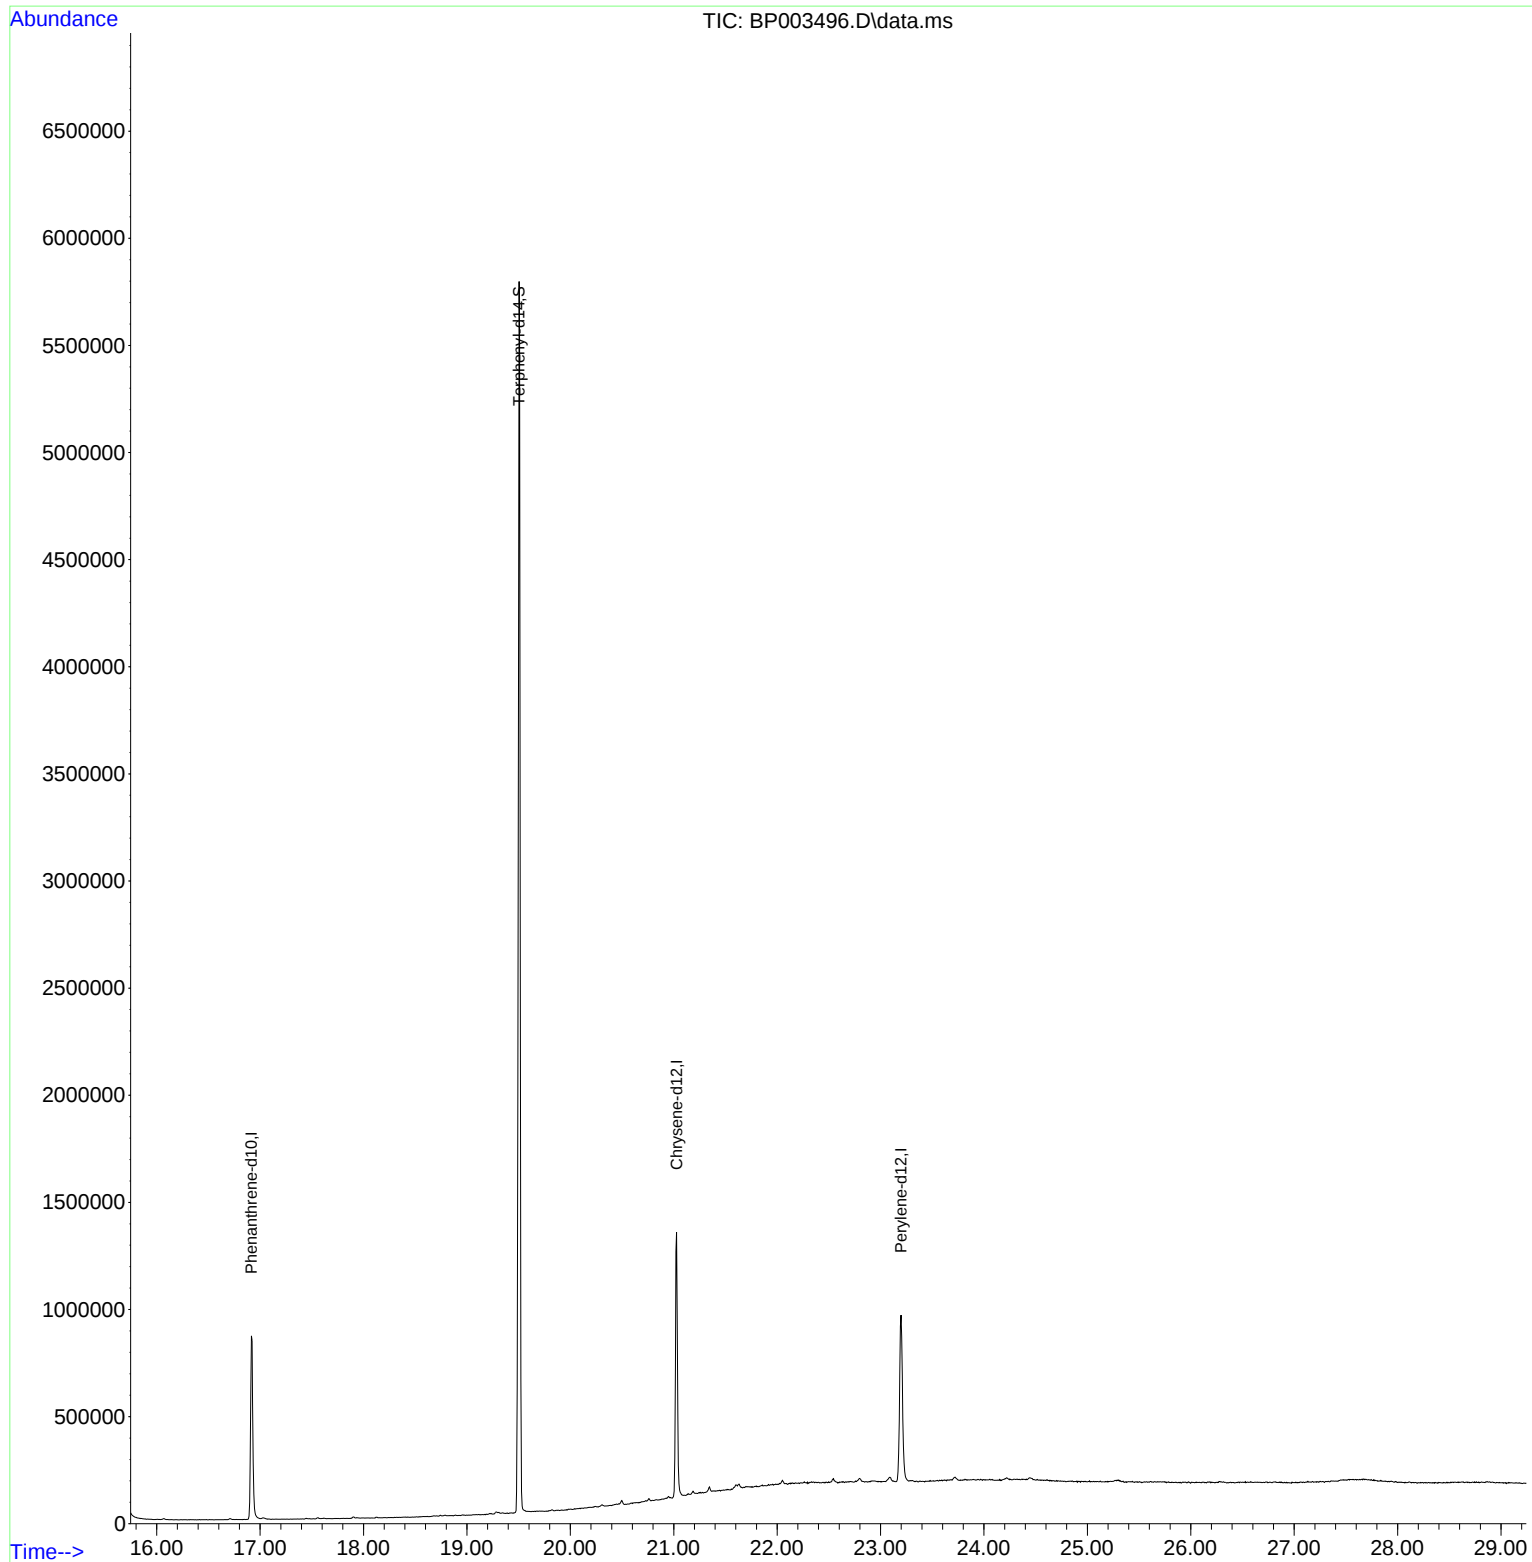







#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.499 min Scan# 784
Delta R.T. 0.001 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29

Instrument :
BNA_P
ClientSampleId :
OK-02-100120

Tgt Ion:152 Resp: 95925




Ion	Ratio	Lower	Upper
152	100		
150	155.7	123.8	185.6
115	65.5	43.8	65.6

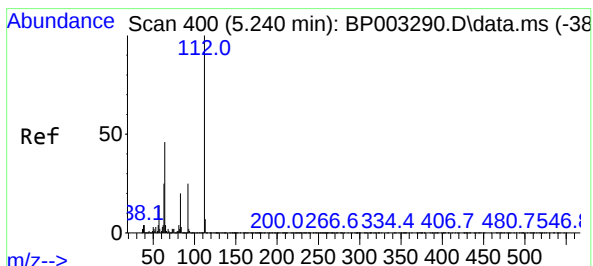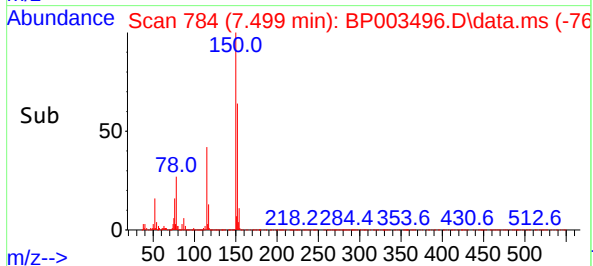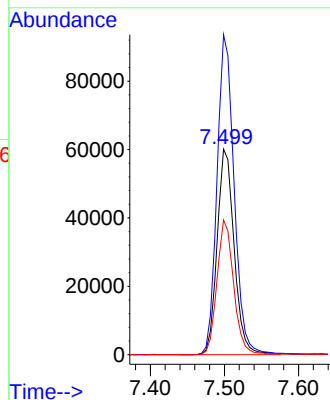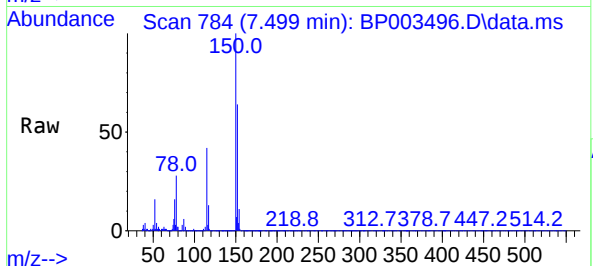


#5
2-Fluorophenol
Concen: 129.34 ng
RT: 5.116 min Scan# 379
Delta R.T. 0.006 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29

Tgt Ion:112 Resp: 710532

Ion	Ratio	Lower	Upper
112	100		
64	51.4	32.8	49.2#
63	28.8	17.0	25.4#


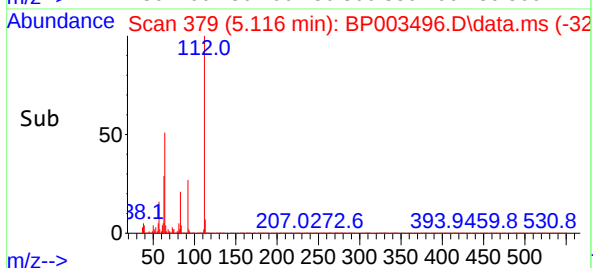
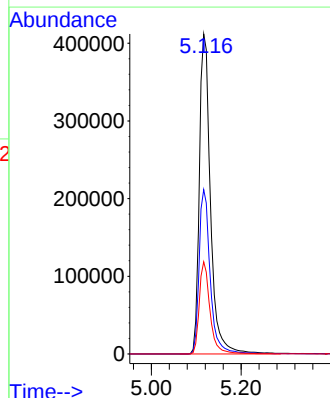
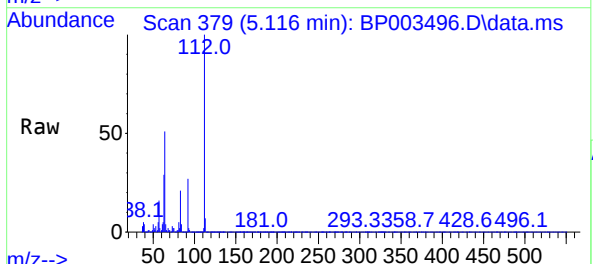


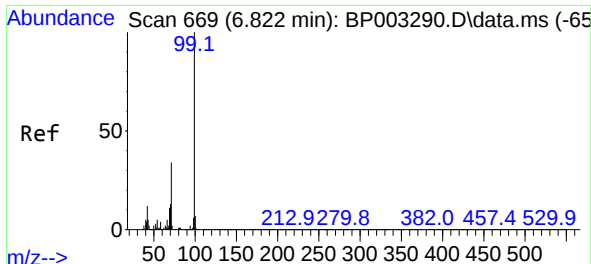

#7
Phenol-d6
Concen: 119.62 ng
RT: 6.710 min Scan# 650
Delta R.T. 0.006 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29




Instrument :
BNA_P
ClientSampleId :
OK-02-100120


Tgt Ion: 99 Resp: 875939
Ion Ratio Lower Upper
99 100
42 13.0 8.6 13.0#
71 36.0 23.4 35.2#

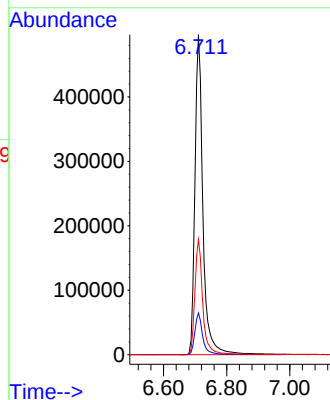

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.275 min Scan# 1256
Delta R.T. 0.000 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29

Tgt Ion: 136 Resp: 383951
Ion Ratio Lower Upper
136 100
137 11.0 8.6 13.0
54 5.5 3.6 5.4#
68 5.7 3.3 4.9#


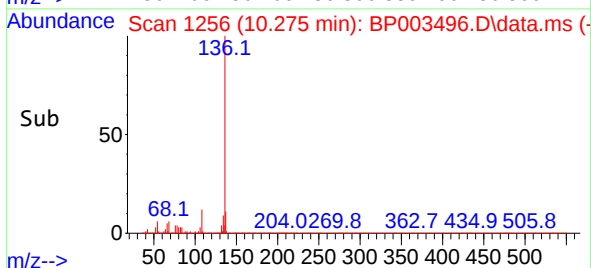
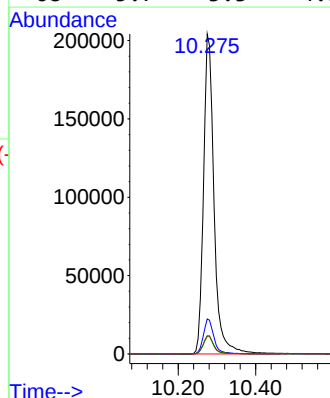
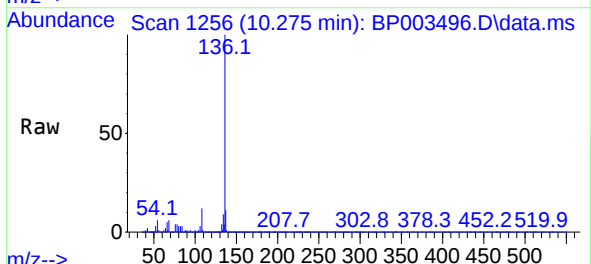


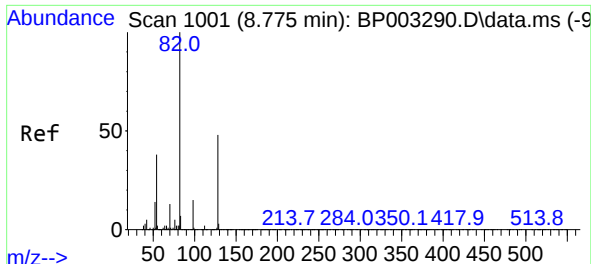

#23
Nitrobenzene-d5
Concen: 112.25 ng
RT: 8.652 min Scan# 980
Delta R.T. 0.000 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29




Instrument :
BNA_P
ClientSampleId :
OK-02-100120

Tgt Ion: 82 Resp: 733635
Ion Ratio Lower Upper
82 100
128 42.2 45.6 68.4#
54 38.6 30.1 45.1

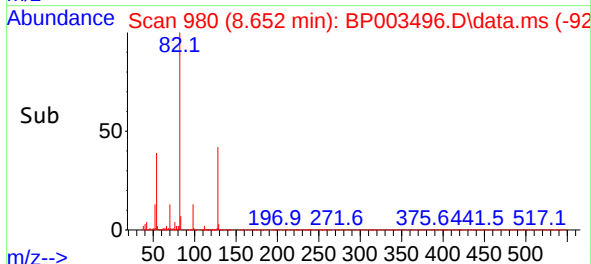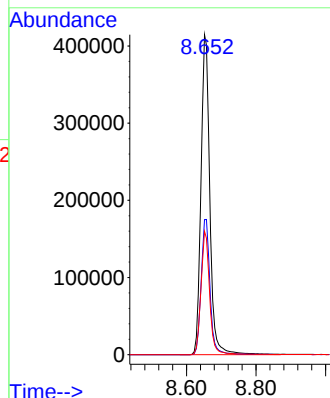

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.157 min Scan# 1916
Delta R.T. 0.000 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29

Tgt Ion: 164 Resp: 238714
Ion Ratio Lower Upper
164 100
162 100.4 79.4 119.2
160 45.7 36.1 54.1


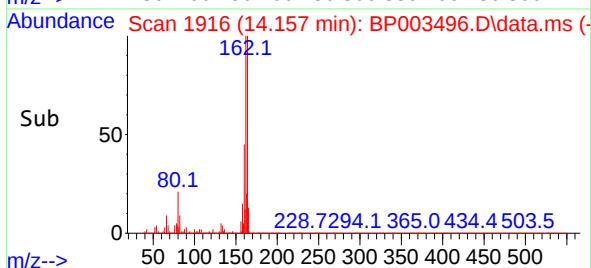
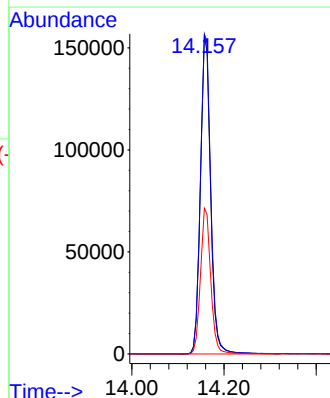
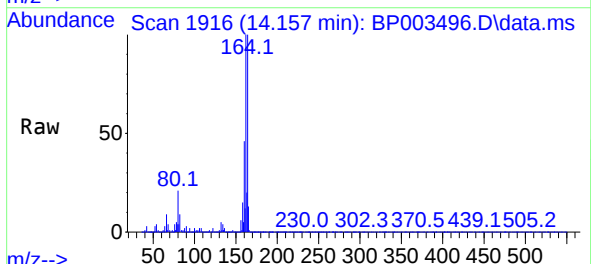




#42
2,4,6-Tribromophenol
Concen: 128.23 ng
RT: 15.663 min Scan# 2172
Delta R.T. 0.000 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29




Instrument :
BNA_P
ClientSampleId :
OK-02-100120


Tgt Ion:330 Resp: 466878
Ion Ratio Lower Upper
330 100
332 96.8 77.1 115.7
141 35.0 23.4 35.2

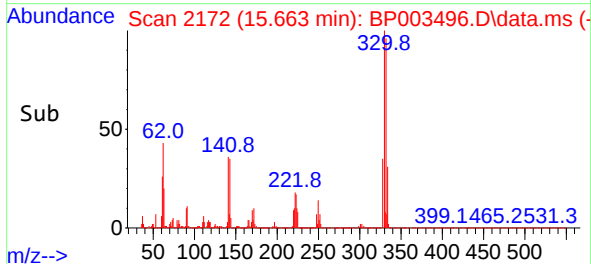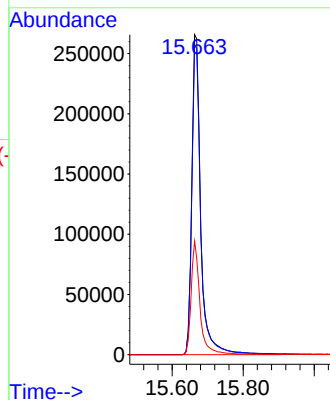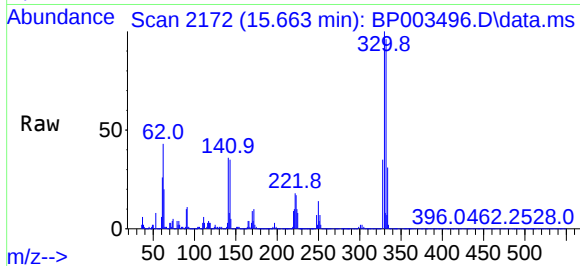

#45
2-Fluorobiphenyl
Concen: 92.27 ng
RT: 12.775 min Scan# 1681
Delta R.T. 0.000 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29

Tgt Ion:172 Resp: 1506035
Ion Ratio Lower Upper
172 100
171 36.3 28.5 42.7
170 23.7 19.2 28.8


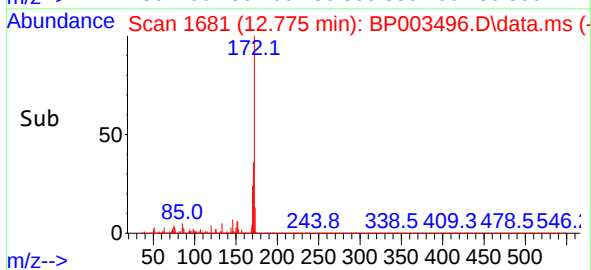
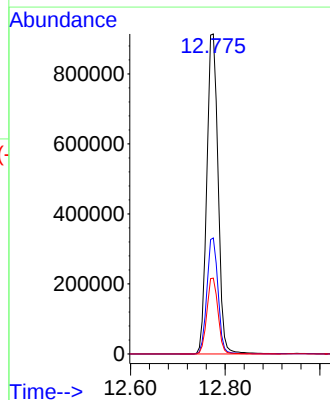
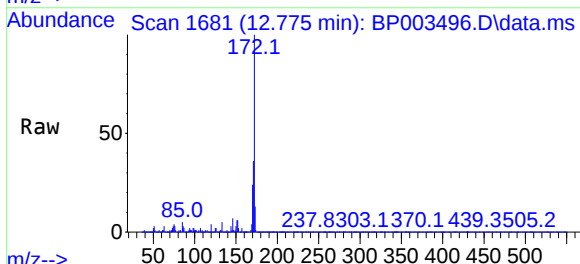




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.916 min Scan# 2385
Delta R.T. 0.000 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29




Instrument :
BNA_P
ClientSampleId :
OK-02-100120


Tgt Ion:188 Resp: 533890
Ion Ratio Lower Upper
188 100
94 9.8 6.2 9.2#
80 10.5 6.2 9.2#

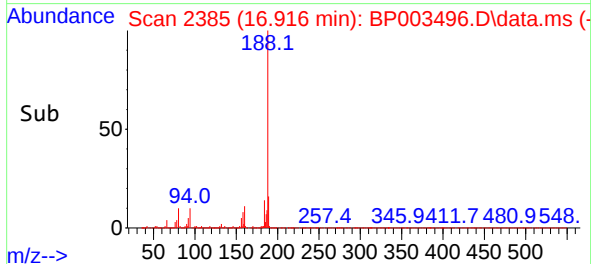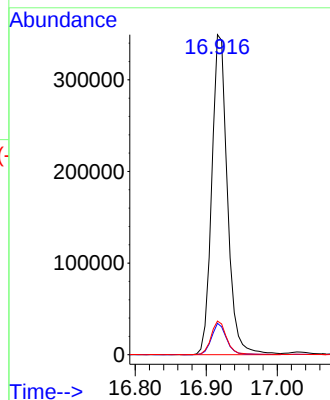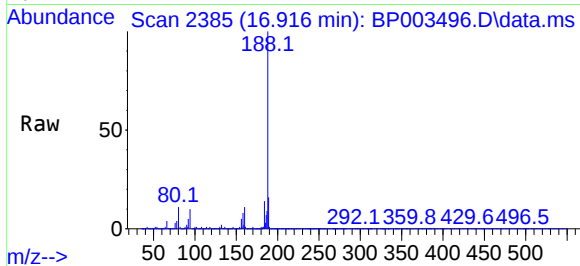

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.027 min Scan# 3084
Delta R.T. 0.000 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29

Tgt Ion:240 Resp: 610821
Ion Ratio Lower Upper
240 100
120 10.2 7.8 11.6
236 26.1 20.8 31.2


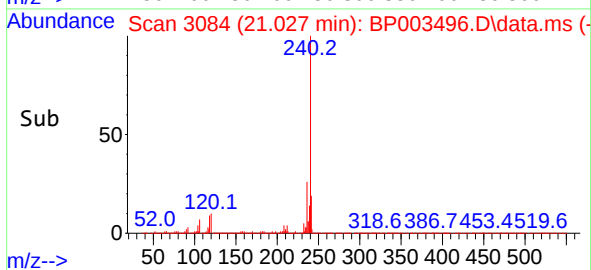
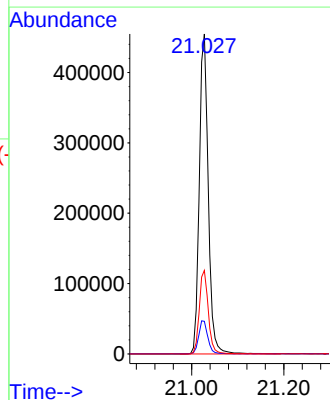
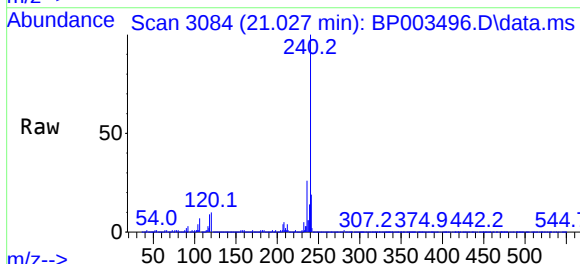


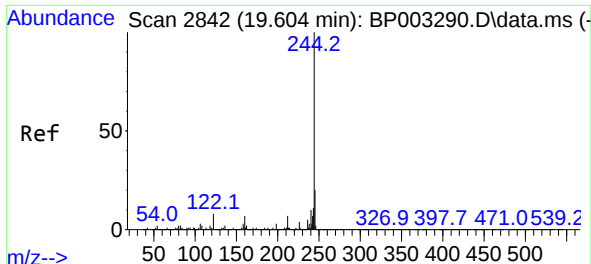

#79
Terphenyl-d14
Concen: 86.98 ng
RT: 19.504 min Scan# 2825
Delta R.T. 0.000 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29

Instrument :
BNA_P
ClientSampleId :
OK-02-100120

Tgt Ion:244 Resp: 2549775
Ion Ratio Lower Upper
244 100
212 7.9 5.8 8.6
122 8.8 7.8 11.8

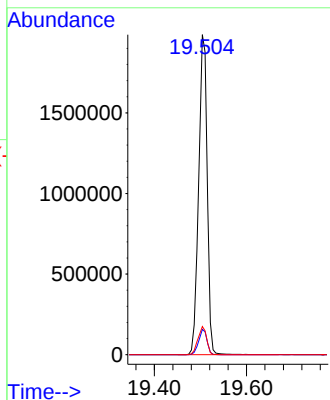

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.198 min Scan# 3453
Delta R.T. 0.000 min
Lab File: BP003496.D
Acq: 05 Oct 2020 18:29

Tgt Ion:264 Resp: 561405
Ion Ratio Lower Upper
264 100
260 24.0 18.8 28.2
265 21.1 17.4 26.2

