

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
 Data File : BP003489.D
 Acq On : 05 Oct 2020 14:27
 Operator : CG/JU
 Sample : PB132085BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132085BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.111	373	378	414	rBV	1435925	2307440	50.82%	10.986%
2	6.705	643	649	679	rBV	1274240	2236425	49.25%	10.648%
3	7.499	777	784	802	rBV	284190	485987	10.70%	2.314%
4	8.652	973	980	1002	rBV	852729	1577431	34.74%	7.510%
5	10.281	1249	1257	1278	rBV	294869	637432	14.04%	3.035%
6	12.775	1674	1681	1705	rBV	2115335	3501623	77.12%	16.671%
7	14.163	1910	1917	1933	rBV	450809	794577	17.50%	3.783%
8	15.663	2166	2172	2209	rBV	1187251	2082793	45.87%	9.916%
9	16.922	2377	2386	2406	rBV	482388	873334	19.23%	4.158%
10	19.504	2819	2825	2845	rBV	3456503	4540543	100.00%	21.617%
11	21.028	3079	3084	3097	rBV	652861	957430	21.09%	4.558%
12	23.204	3447	3454	3473	rBV2	442241	1009070	22.22%	4.804%




Sum of corrected areas: 21004085

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
Data File : BP003489.D
Acq On : 05 Oct 2020 14:27
Operator : CG/JU
Sample : PB132085BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132085BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

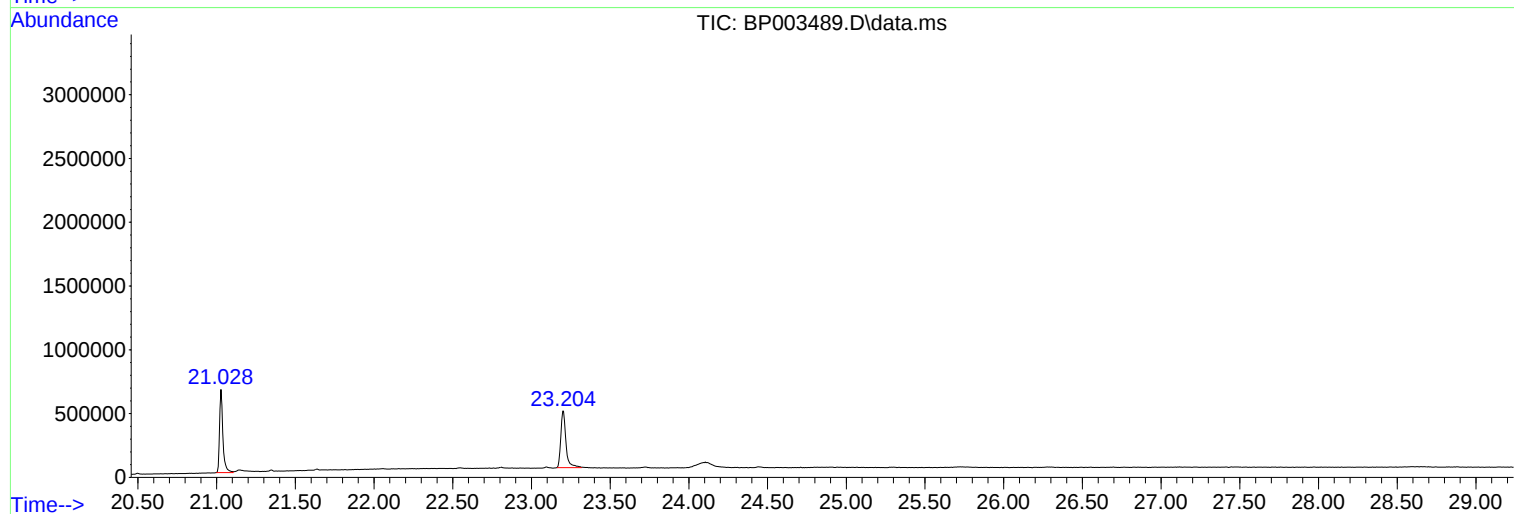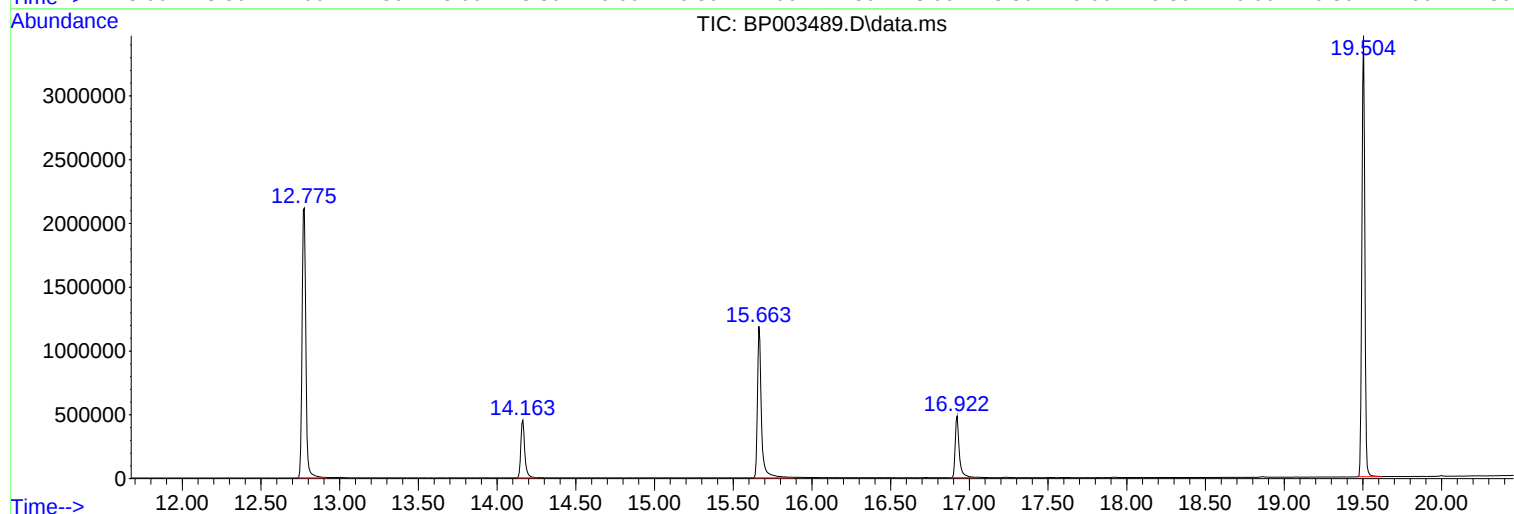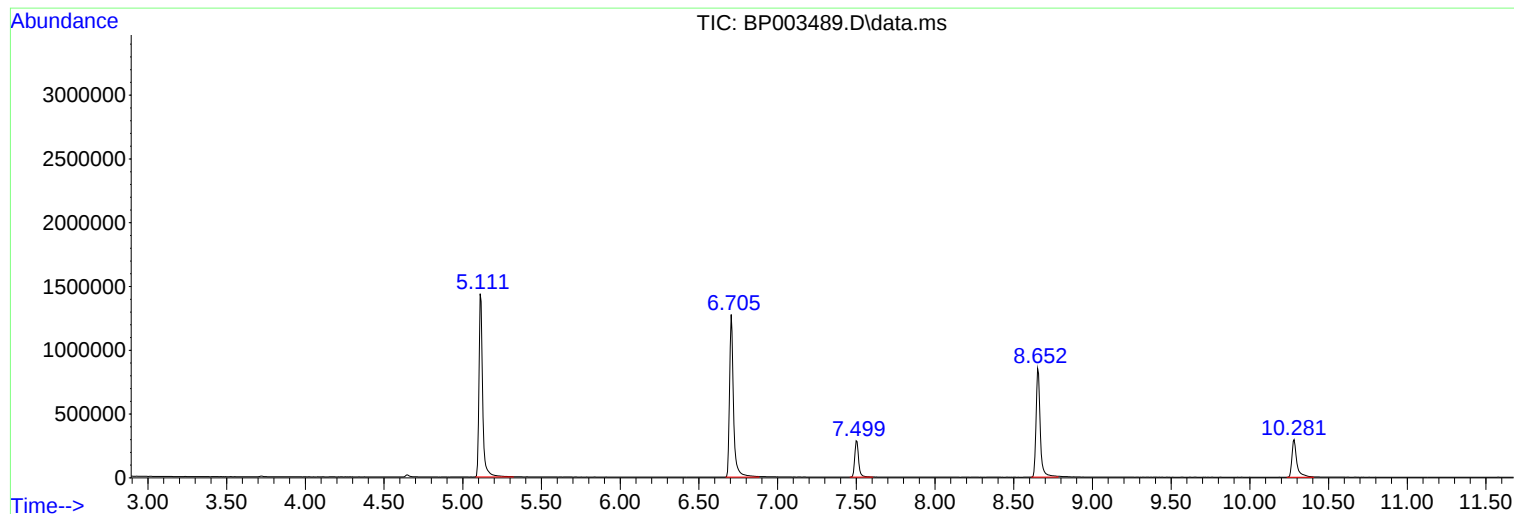

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
Data File : BP003489.D
Acq On : 05 Oct 2020 14:27
Operator : CG/JU
Sample : PB132085BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132085BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
Data File : BP003489.D
Acq On : 05 Oct 2020 14:27
Operator : CG/JU
Sample : PB132085BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132085BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------