
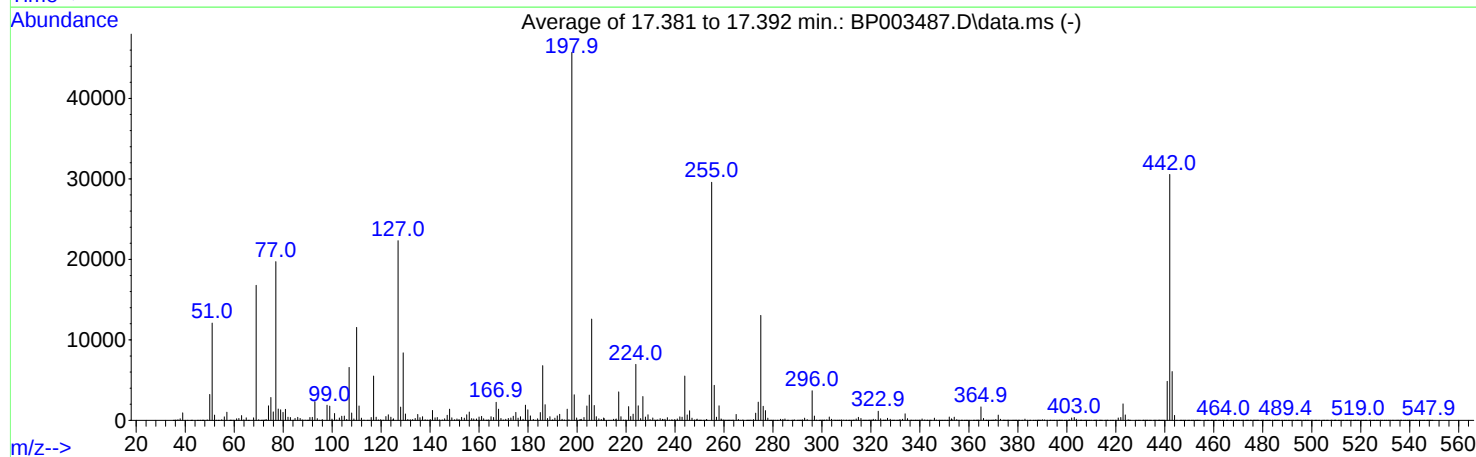


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
 Data File : BP003487.D
 Acq On : 05 Oct 2020 12:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 14:33:14 2020

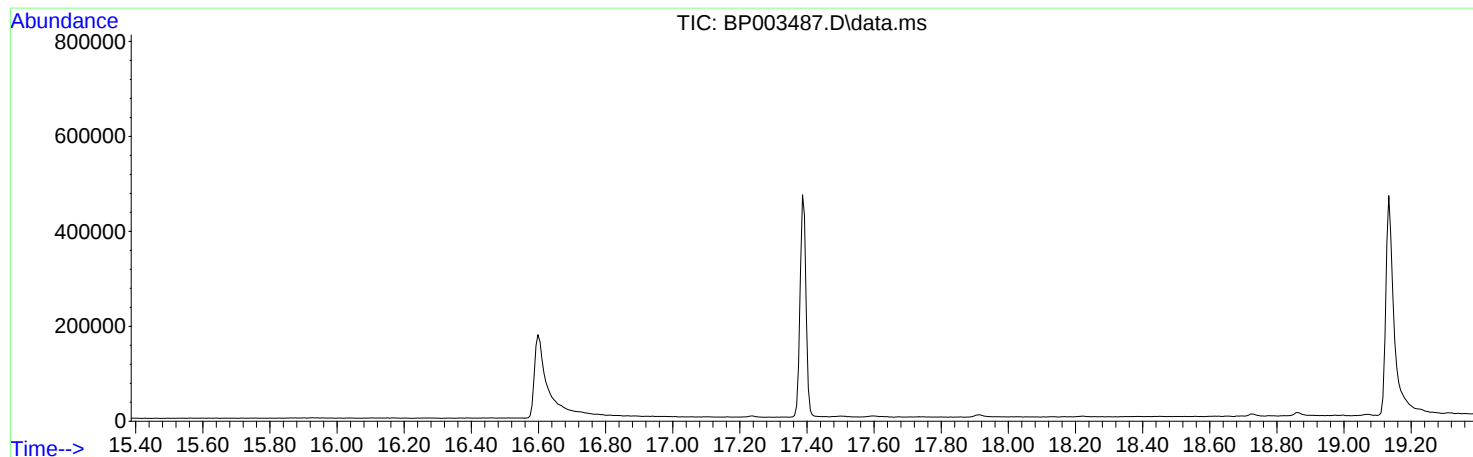

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	12088	PASS
68	69	0.00	2	1.8	310	PASS
69	198	0.00	100	36.7	16770	PASS
70	69	0.00	2	0.5	87	PASS
127	198	10	80	48.9	22333	PASS
197	198	0.00	2	0.2	75	PASS
198	198	100	100	100.0	45701	PASS
199	198	5	9	7.0	3190	PASS
275	198	10	60	28.5	13034	PASS
365	198	1	100	3.7	1669	PASS
441	198	0.01	100	10.6	4853	PASS
442	198	50	100	66.8	30544	PASS
443	442	15	24	19.9	6066	PASS