
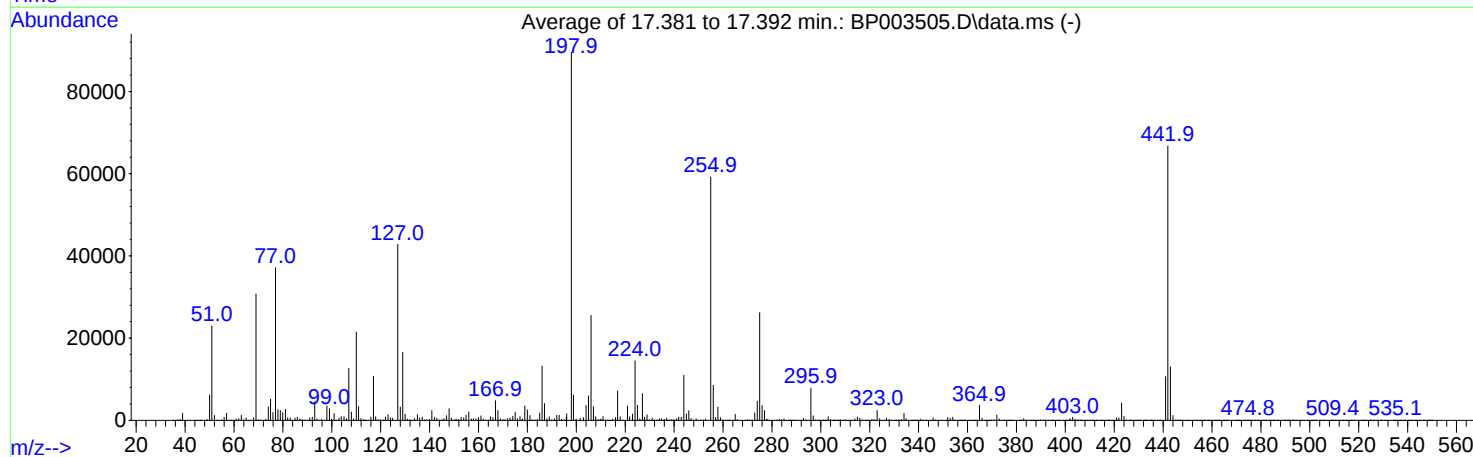


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100520\
 Data File : BP003505.D
 Acq On : 06 Oct 2020 01:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 14:33:14 2020

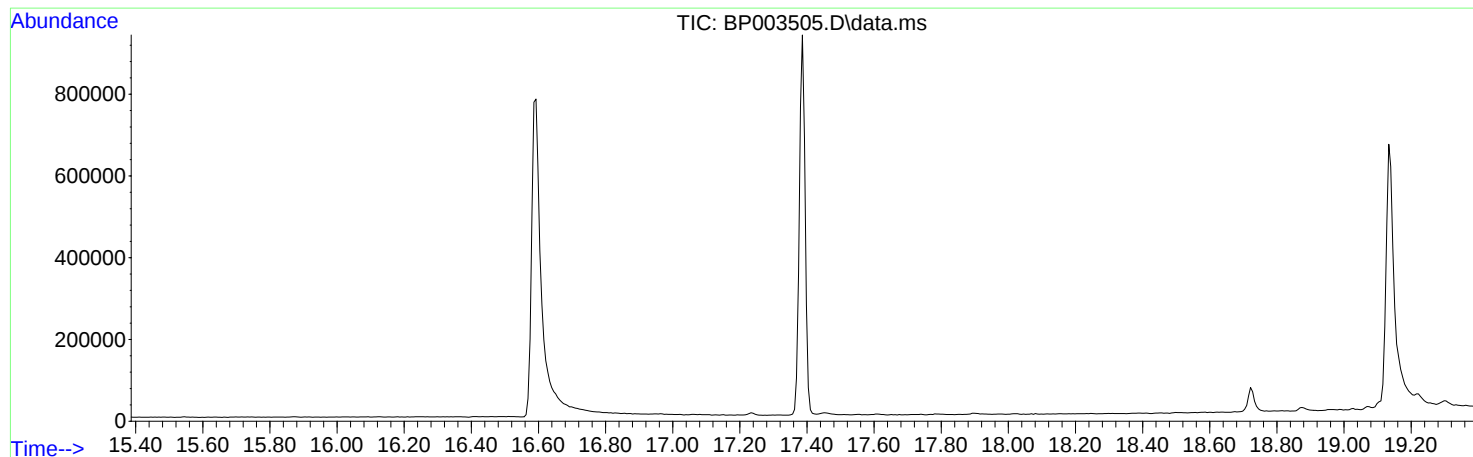

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	22975	PASS
68	69	0.00	2	2.0	627	PASS
69	198	0.00	100	34.3	30736	PASS
70	69	0.00	2	0.5	149	PASS
127	198	10	80	47.8	42801	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89481	PASS
199	198	5	9	6.9	6171	PASS
275	198	10	60	29.3	26210	PASS
365	198	1	100	4.1	3644	PASS
441	198	0.01	100	11.9	10669	PASS
442	198	50	100	74.6	66760	PASS
443	442	15	24	19.5	13044	PASS