
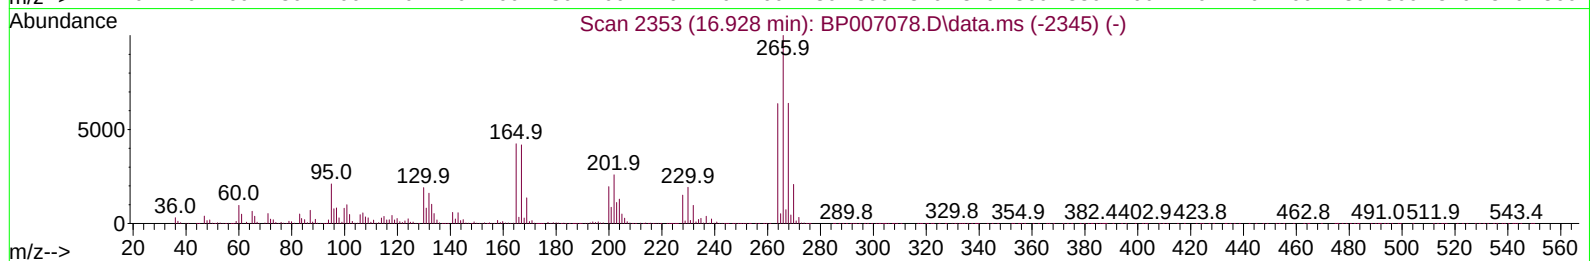
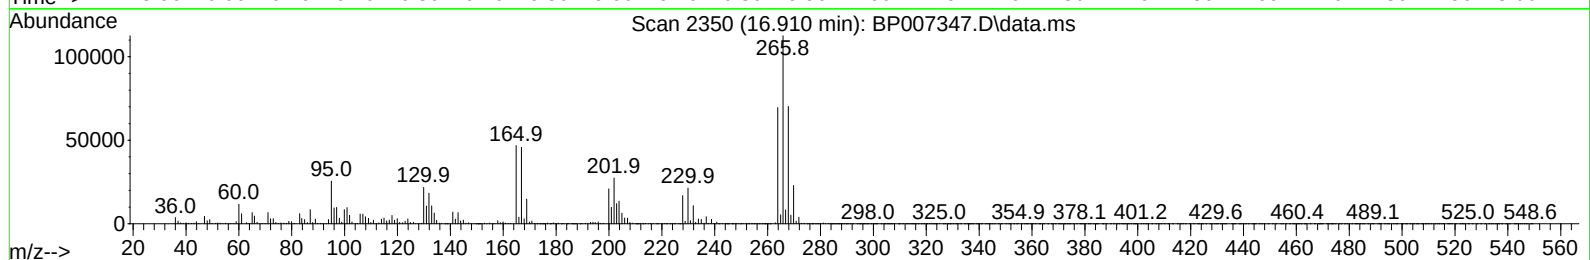


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007347.D
Acq On : 06 Oct 2021 10:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 11:20:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 12:49:05 2021
Response via : Initial Calibration

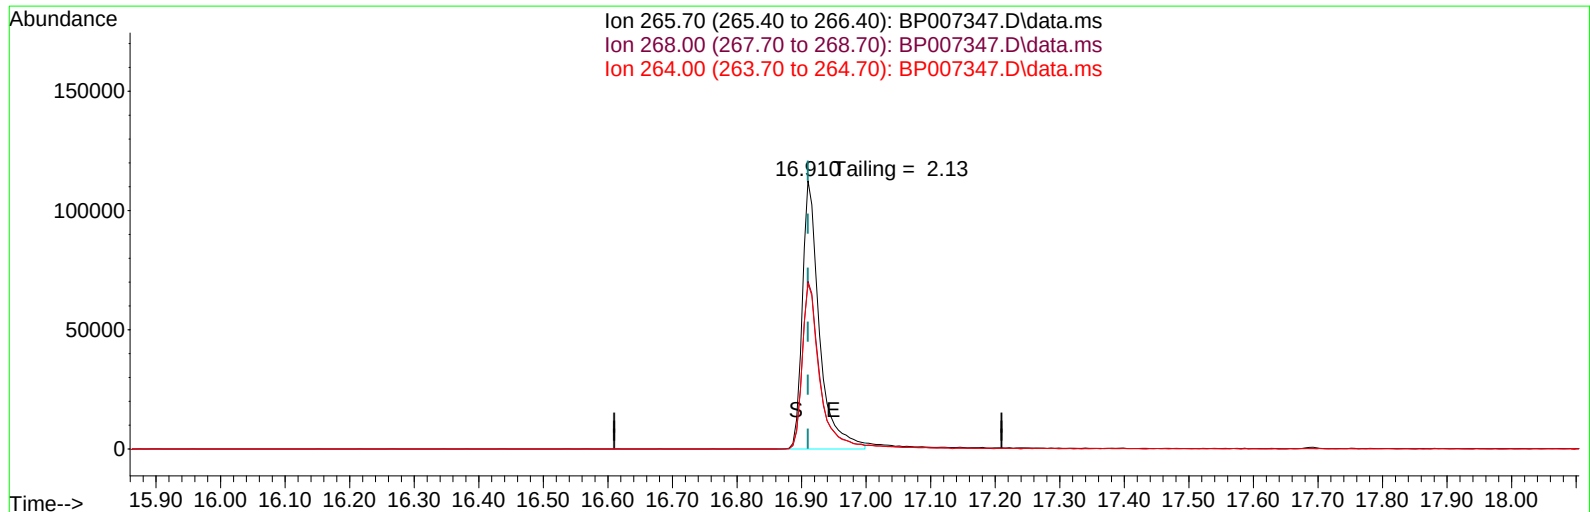

TIC: BP007347.D\data.ms

(70) Pentachlorophenol (C)




16.910min (+ 0.000) 582033.39 ng

response 210156

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.42
264.00	62.90	61.80
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\  
Data File : BP007347.D  
Acq On    : 06 Oct 2021  10:07  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Oct 06 11:20:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 01 12:49:05 2021
Response via : Initial Calibration

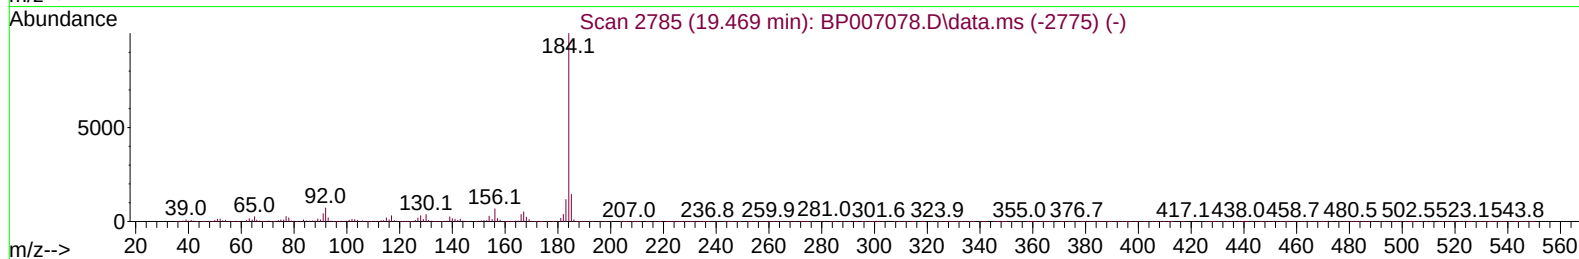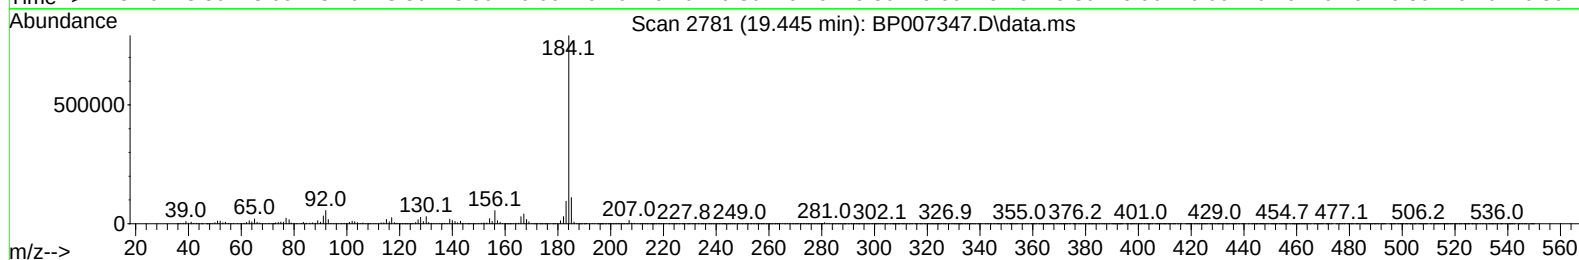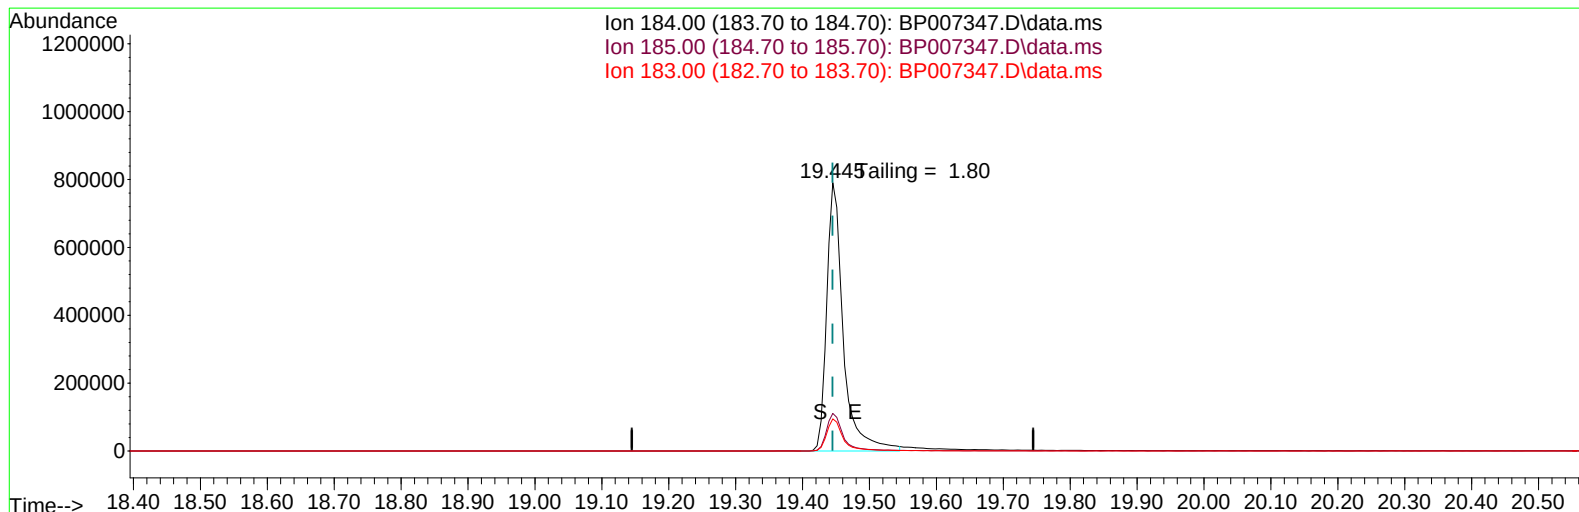

TIC: BP007347.D\data.ms

(77) Benzidine

19.445min (+ 0.000) 389068.04 ng m

response **1375017**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.00
183.00	11.90	11.98
0.00	0.00	0.00