

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
 Data File : BP007354.D
 Acq On : 06 Oct 2021 15:11
 Operator : CG/JU
 Sample : M3797-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 VB16193

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	53	rVB	135714	169023	2.09%	0.450%
2	4.487	233	238	246	rBV	152363	220133	2.72%	0.586%
3	4.940	310	315	318	rBV	78603	105861	1.31%	0.282%
4	4.981	318	322	336	rVB	106604	178824	2.21%	0.476%
5	5.440	394	400	425	rVB	2071587	3433005	42.41%	9.133%
6	7.040	665	672	702	rBV	1747730	3143300	38.83%	8.362%
7	7.858	803	811	820	rBV	476946	784234	9.69%	2.086%
8	9.022	1001	1009	1025	rBV	1342780	2439378	30.14%	6.489%
9	10.452	1244	1252	1275	rBV	265283	687901	8.50%	1.830%
10	10.657	1280	1287	1300	rVV	573189	1006878	12.44%	2.679%
11	13.122	1697	1706	1728	rBV	3402181	5586020	69.01%	14.860%
12	13.963	1843	1849	1863	rBV	93910	183884	2.27%	0.489%
13	14.498	1932	1940	1958	rBV	733284	1278170	15.79%	3.400%
14	15.316	2069	2079	2098	rBV	178739	359983	4.45%	0.958%
15	15.992	2187	2194	2218	rBV	2170233	3845788	47.51%	10.231%
16	17.251	2401	2408	2421	rBV	944134	1518261	18.76%	4.039%
17	17.916	2516	2521	2530	rBV	97536	132042	1.63%	0.351%
18	18.139	2554	2559	2567	rBV	186377	310179	3.83%	0.825%
19	19.369	2765	2768	2775	rBV2	47910	83415	1.03%	0.222%
20	19.810	2837	2843	2856	rBV	6623601	8094214	100.00%	21.532%
21	20.551	2965	2969	2973	rBV	125503	156016	1.93%	0.415%
22	21.045	3051	3053	3060	rVB3	84470	112877	1.39%	0.300%
23	21.339	3098	3103	3113	rBV	1316131	1856334	22.93%	4.938%
24	23.745	3506	3512	3526	rVB2	809310	1904977	23.54%	5.068%




Sum of corrected areas: 37590697

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007354.D
Acq On : 06 Oct 2021 15:11
Operator : CG/JU
Sample : M3797-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
VB16193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

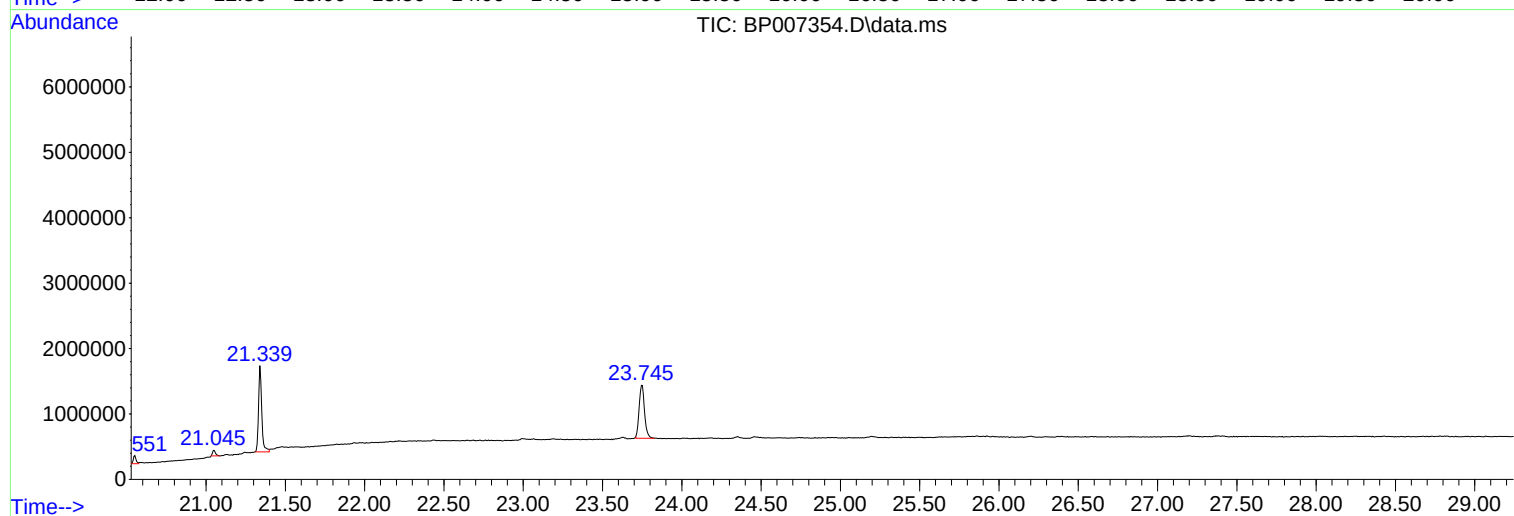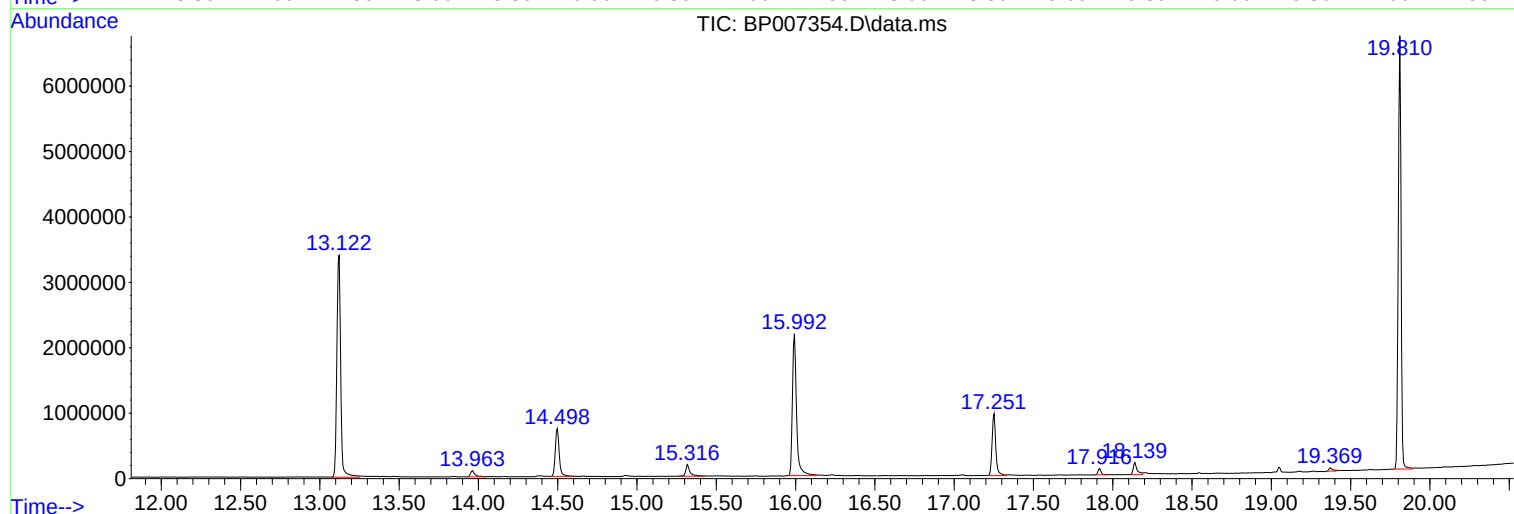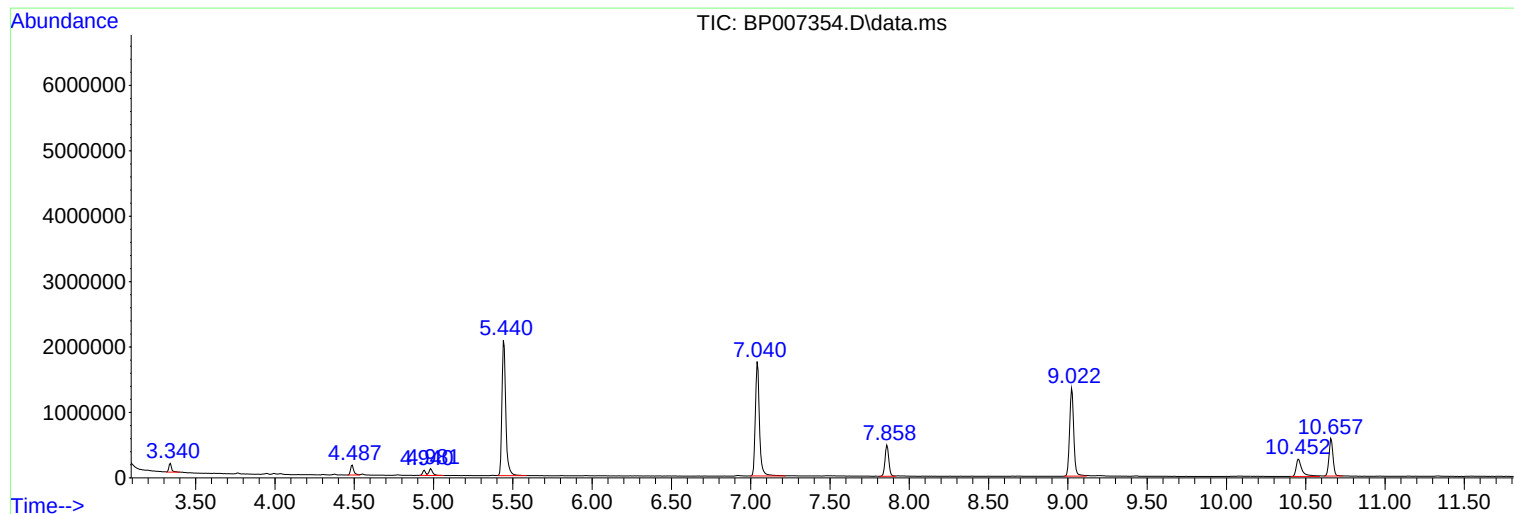

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007354.D
Acq On : 06 Oct 2021 15:11
Operator : CG/JU
Sample : M3797-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
VB16193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007354.D
Acq On : 06 Oct 2021 15:11
Operator : CG/JU
Sample : M3797-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
VB16193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------