

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
 Data File : BP007355.D
 Acq On : 06 Oct 2021 15:45
 Operator : CG/JU
 Sample : M3797-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 26598

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.487	233	238	246	rBV	183245	236384	2.93%	0.660%
2	4.940	310	315	319	rBV	128430	167058	2.07%	0.466%
3	4.981	319	322	333	rVB	102882	144467	1.79%	0.403%
4	5.440	394	400	417	rBV	2247916	3318248	41.13%	9.263%
5	7.040	665	672	697	rBV	1736518	2996492	37.14%	8.365%
6	7.857	804	811	820	rBV	464915	724741	8.98%	2.023%
7	9.022	999	1009	1024	rBV	1273189	2283332	28.30%	6.374%
8	10.457	1245	1253	1269	rBV	221509	591732	7.34%	1.652%
9	10.657	1280	1287	1295	rBV	513024	911847	11.30%	2.546%
10	13.116	1698	1705	1733	rBV	3226812	5309948	65.82%	14.823%
11	13.963	1843	1849	1858	rBV	47964	94262	1.17%	0.263%
12	14.498	1933	1940	1956	rBV	677632	1171237	14.52%	3.270%
13	15.321	2071	2080	2093	rBV	107465	215421	2.67%	0.601%
14	15.992	2187	2194	2222	rBV	2172792	3950261	48.97%	11.028%
15	17.251	2401	2408	2421	rBV	871937	1419625	17.60%	3.963%
16	17.915	2517	2521	2529	rVB	82031	109893	1.36%	0.307%
17	18.139	2554	2559	2567	rBV2	117725	205489	2.55%	0.574%
18	19.809	2837	2843	2855	rBV	6608372	8067198	100.00%	22.521%
19	20.551	2966	2969	2973	rBV	103915	115028	1.43%	0.321%
20	21.051	3050	3054	3062	rBV3	165625	254205	3.15%	0.710%
21	21.339	3099	3103	3114	rBV	1229933	1688372	20.93%	4.713%
22	23.750	3507	3513	3527	rVB2	810834	1846248	22.89%	5.154%




Sum of corrected areas: 35821488

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007355.D
Acq On : 06 Oct 2021 15:45
Operator : CG/JU
Sample : M3797-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
26598

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

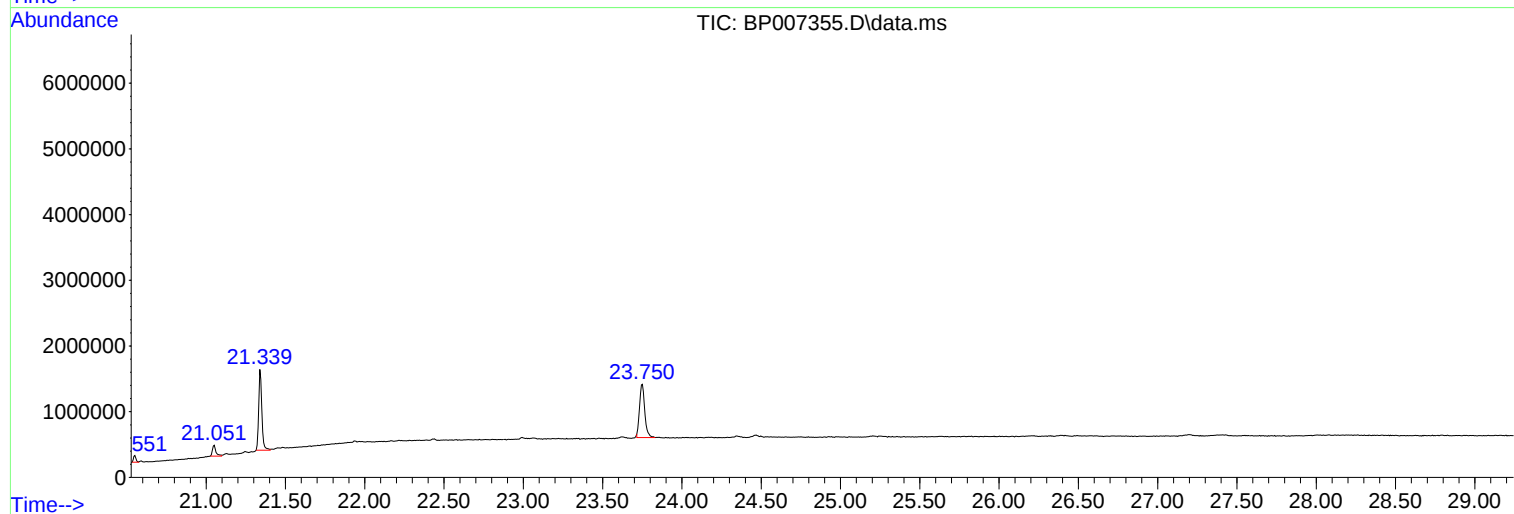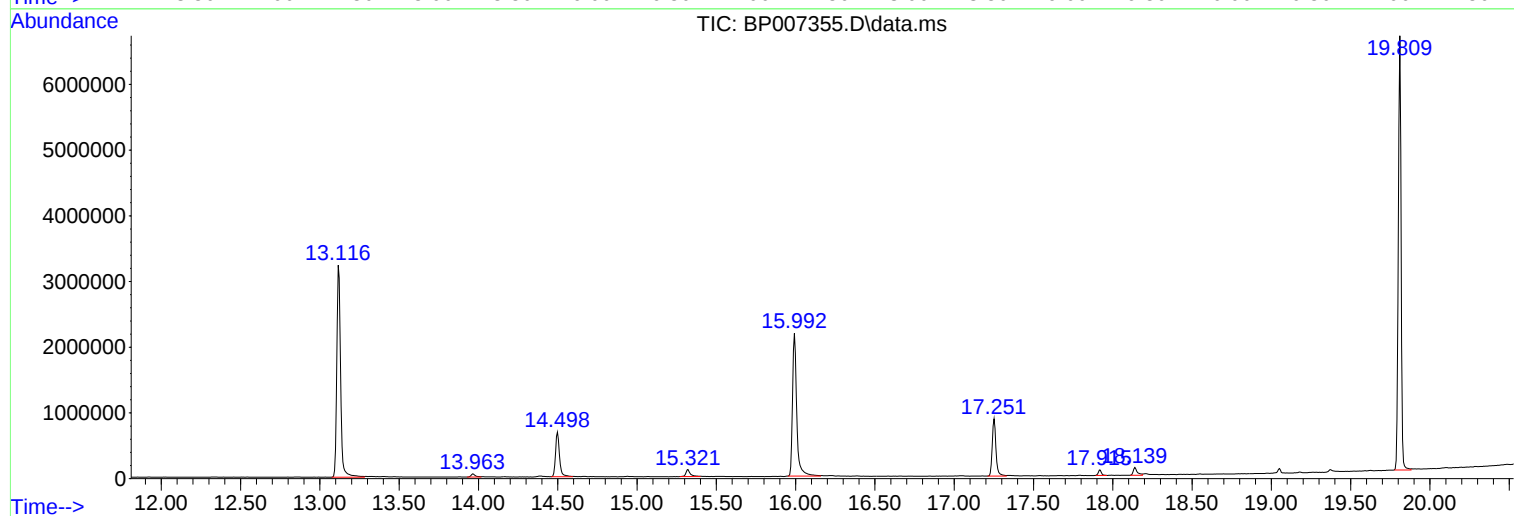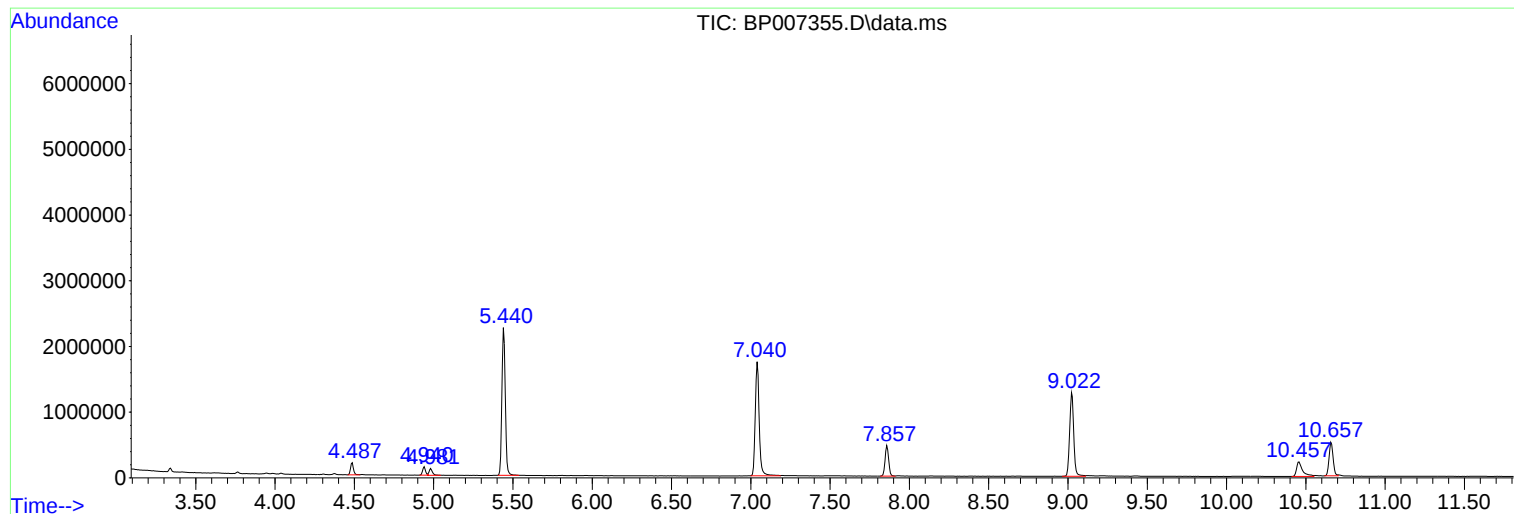

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007355.D
Acq On : 06 Oct 2021 15:45
Operator : CG/JU
Sample : M3797-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
26598

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007355.D
Acq On : 06 Oct 2021 15:45
Operator : CG/JU
Sample : M3797-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
26598

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------