

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
 Data File : BP007363.D
 Acq On : 06 Oct 2021 20:17
 Operator : CG/JU
 Sample : M4057-01 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SHAFT-17B-SP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	393	400	420	rBV	960138	1465942	45.39%	6.106%
2	7.040	664	672	694	rBV	749649	1360078	42.11%	5.665%
3	7.857	803	811	820	rBV	558031	898870	27.83%	3.744%
4	9.022	1002	1009	1024	rBV	478518	880835	27.28%	3.669%
5	10.469	1246	1255	1273	rBV2	33078	121381	3.76%	0.506%
6	10.657	1278	1287	1294	rBV	650072	1142579	35.38%	4.759%
7	13.116	1697	1705	1720	rBV	1263156	2038915	63.14%	8.493%
8	14.216	1887	1892	1902	rBV	44926	80119	2.48%	0.334%
9	14.386	1913	1921	1930	rBV3	19540	60462	1.87%	0.252%
10	14.492	1933	1939	1948	rBV	891571	1434701	44.43%	5.976%
11	15.992	2187	2194	2213	rBV	874336	1559234	48.28%	6.495%
12	17.245	2401	2407	2412	rBV	1148566	1780992	55.15%	7.419%
13	17.286	2412	2414	2426	rVV	260338	428343	13.26%	1.784%
14	17.380	2426	2430	2437	rVB	81690	126065	3.90%	0.525%
15	17.916	2518	2521	2526	rBV2	30488	35410	1.10%	0.147%
16	18.133	2552	2558	2561	rBV2	87344	158189	4.90%	0.659%
17	18.163	2561	2563	2568	rVB	57146	73183	2.27%	0.305%
18	18.304	2583	2587	2591	rBV2	68063	114202	3.54%	0.476%
19	19.004	2703	2706	2708	rBV	31801	43558	1.35%	0.181%
20	19.257	2744	2749	2755	rBV	729108	974979	30.19%	4.061%
21	19.610	2805	2809	2818	rVB	658205	929388	28.78%	3.871%
22	19.804	2837	2842	2848	rBV	2506105	3229443	100.00%	13.452%
23	21.333	3097	3102	3107	rBV2	1735666	2744436	84.98%	11.432%
24	21.374	3107	3109	3116	rVB	388604	419578	12.99%	1.748%
25	23.745	3506	3512	3518	rBV2	969300	1906359	59.03%	7.941%




Sum of corrected areas: 24007241

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007363.D
Acq On : 06 Oct 2021 20:17
Operator : CG/JU
Sample : M4057-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SHAFT-17B-SP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

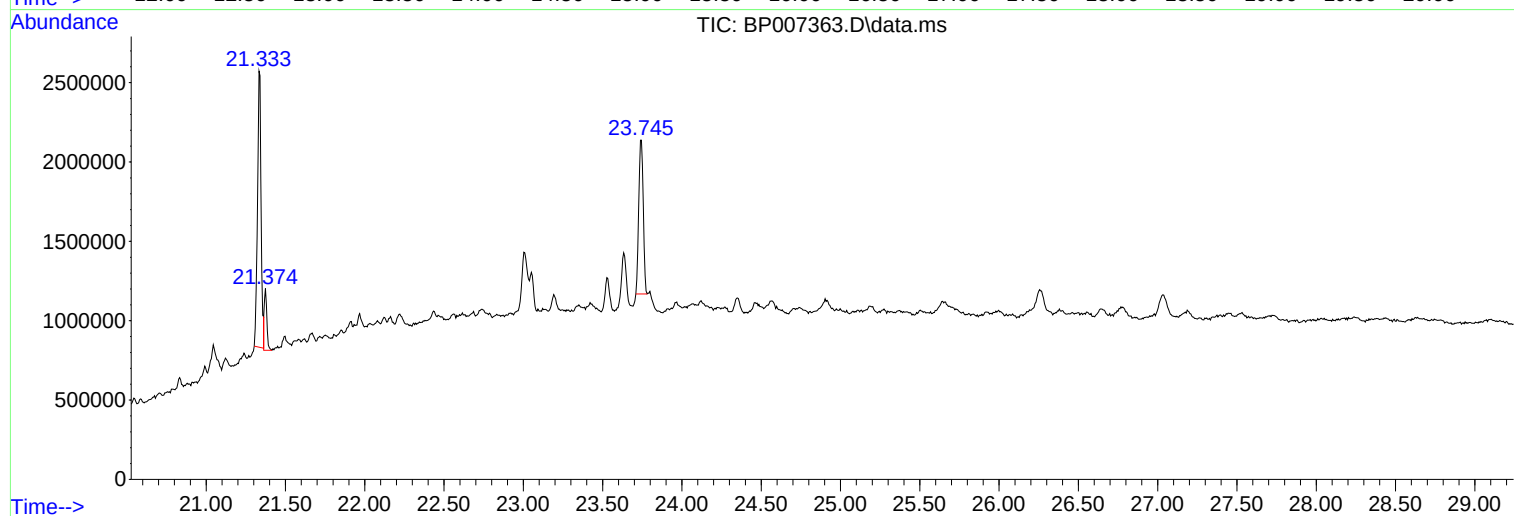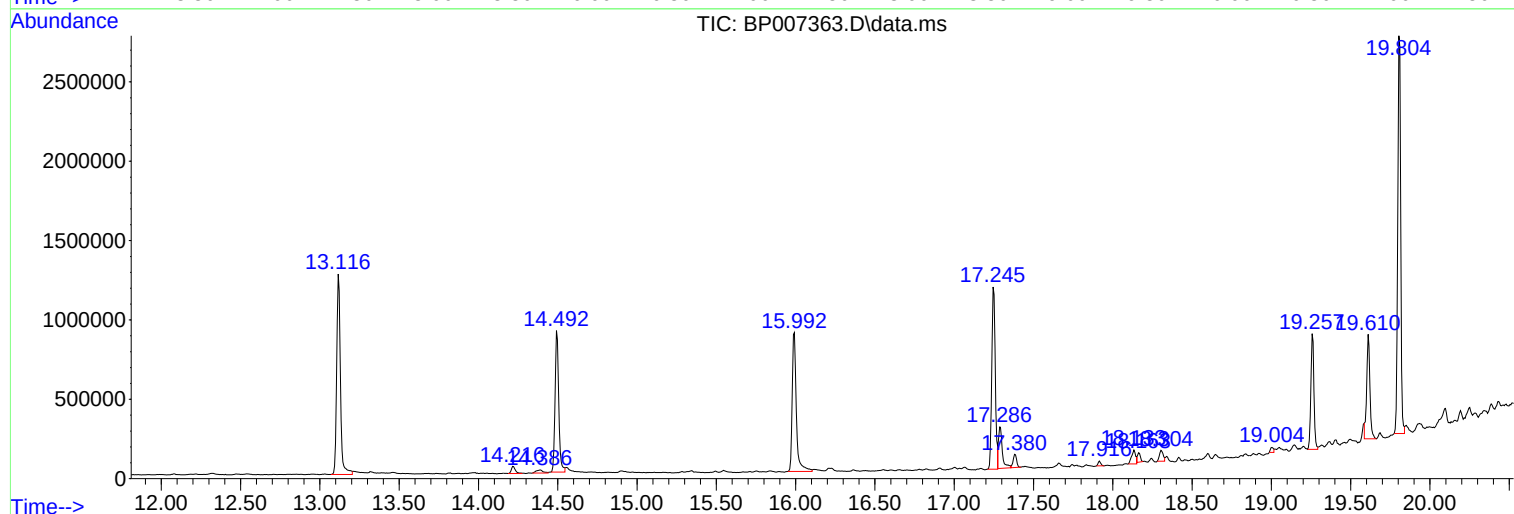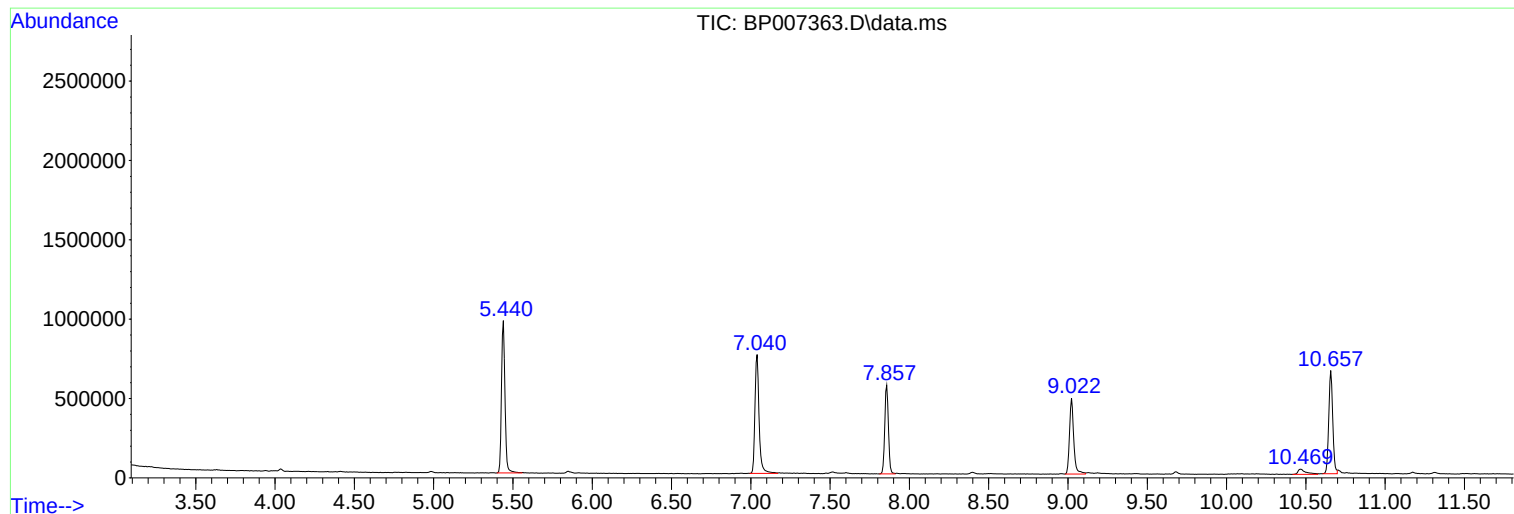

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007363.D
Acq On : 06 Oct 2021 20:17
Operator : CG/JU
Sample : M4057-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SHAFT-17B-SP










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.469	2.12 ng	121381	Naphthalene-d8	10.657

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	86
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	78
3			Ethanol, 2-[2-(2-methylpropoxy)e...	162	C8H18O3	018912-80-6	64
4			4-Octanone, 5-hydroxy-3,6-dimethyl-	172	C10H20O2	062759-47-1	59
5			Pentaethylene glycol monododecyl...	406	C22H46O6	003055-95-6	53

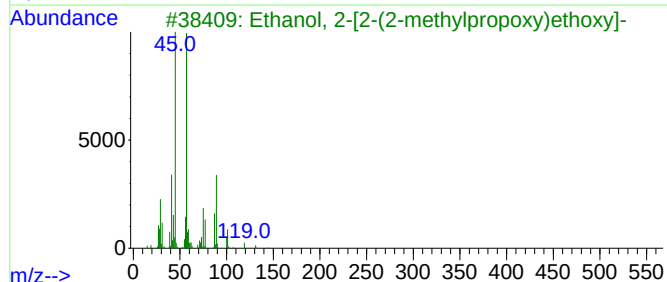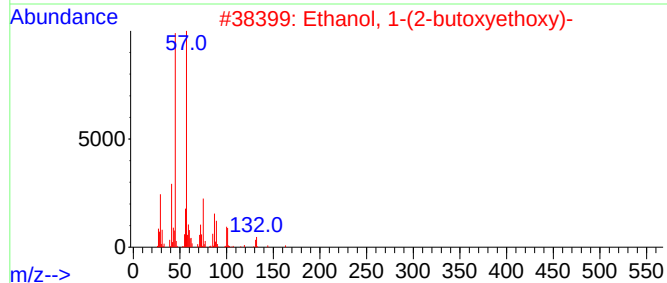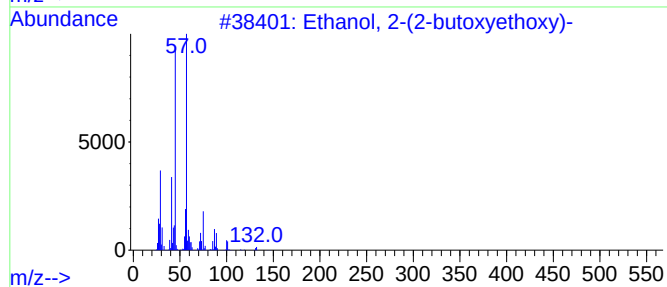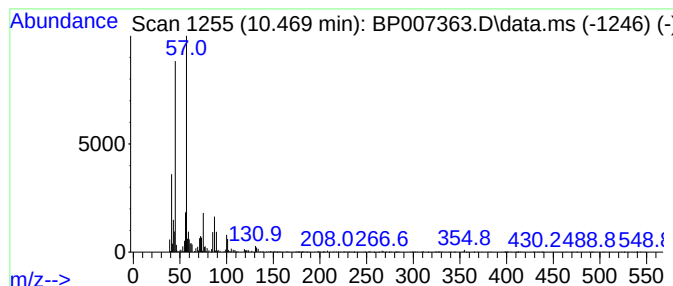

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
Data File : BP007363.D
Acq On : 06 Oct 2021 20:17
Operator : CG/JU
Sample : M4057-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SHAFT-17B-SP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.469	2.1	ng	121381	2	10.657	1142580	20.0