
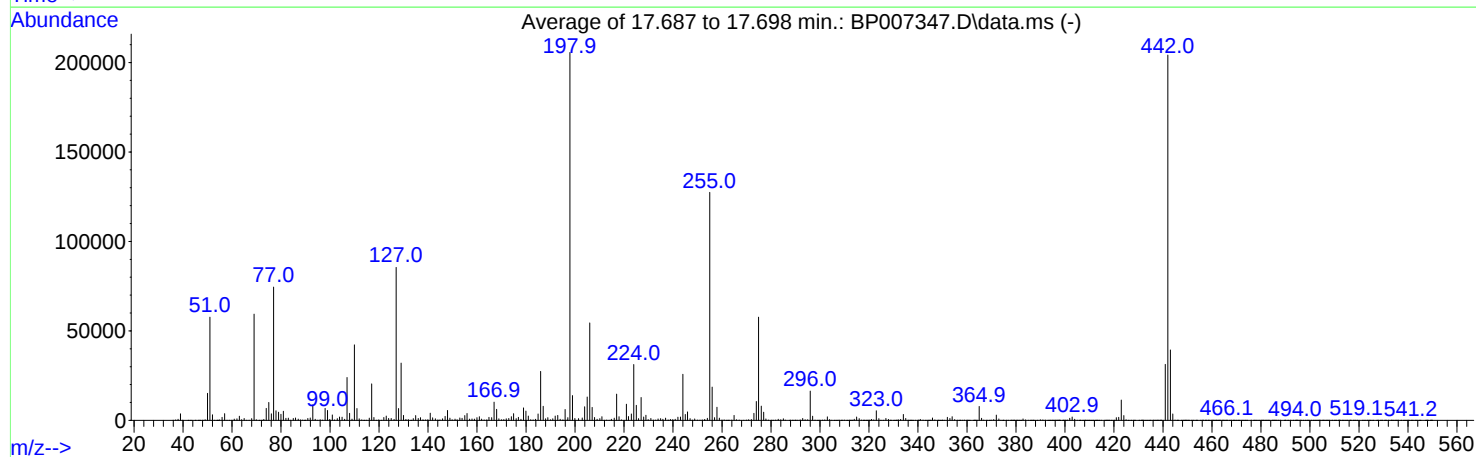


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
 Data File : BP007347.D
 Acq On : 06 Oct 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 12:49:05 2021

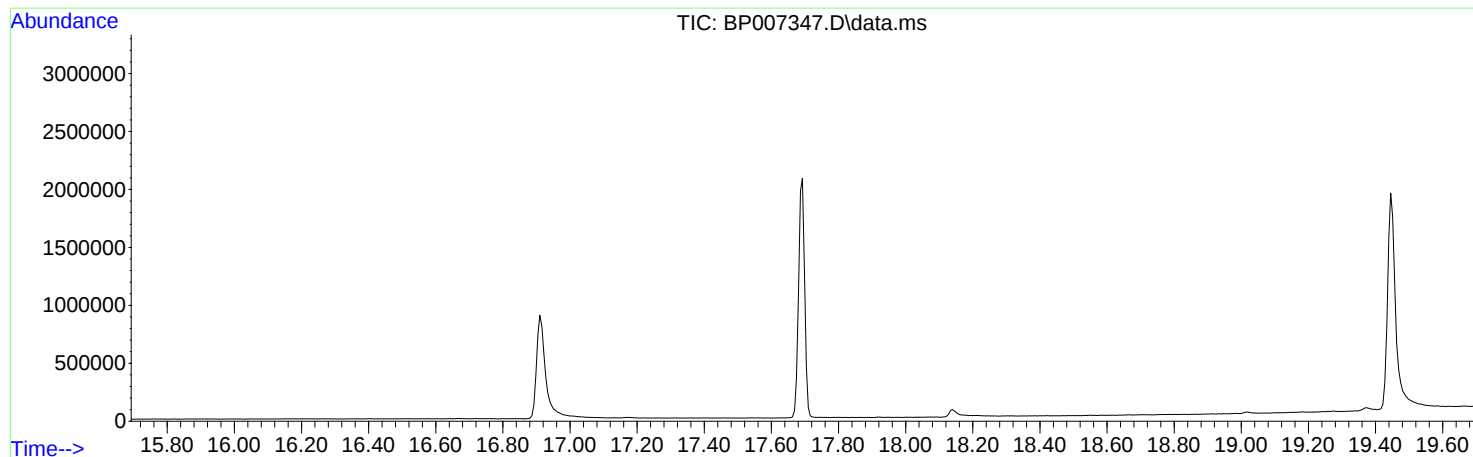




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	57725	PASS
68	69	0.00	2	1.7	1014	PASS
69	198	0.00	100	28.9	59359	PASS
70	69	0.00	2	0.6	380	PASS
127	198	10	80	41.6	85508	PASS
197	198	0.00	2	0.7	1493	PASS
198	198	100	100	100.0	205593	PASS
199	198	5	9	6.7	13828	PASS
275	198	10	60	28.1	57697	PASS
365	198	1	100	3.8	7761	PASS
441	198	0.01	100	15.2	31317	PASS
442	442	100	100	100.0	204203	PASS
443	442	15	24	19.3	39360	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100621\
 Data File : BP007347.D
 Acq On : 06 Oct 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Oct 06 11:20:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 01 12:49:05 2021
 Response via : Initial Calibration

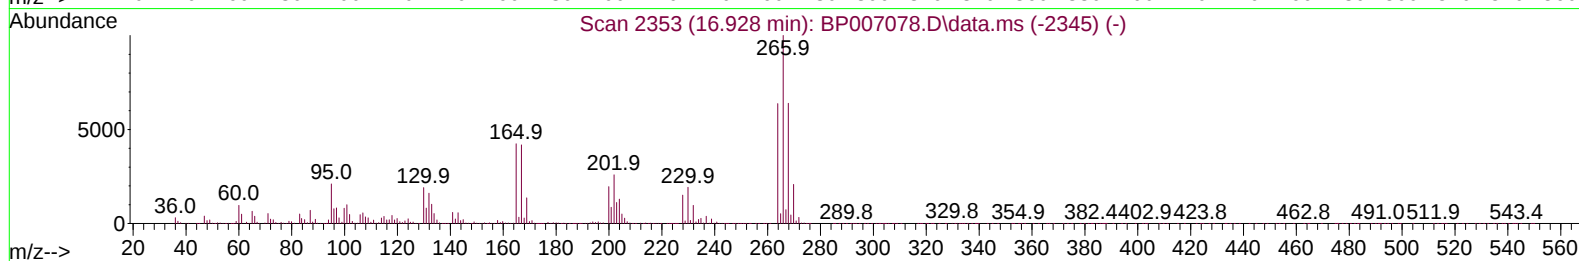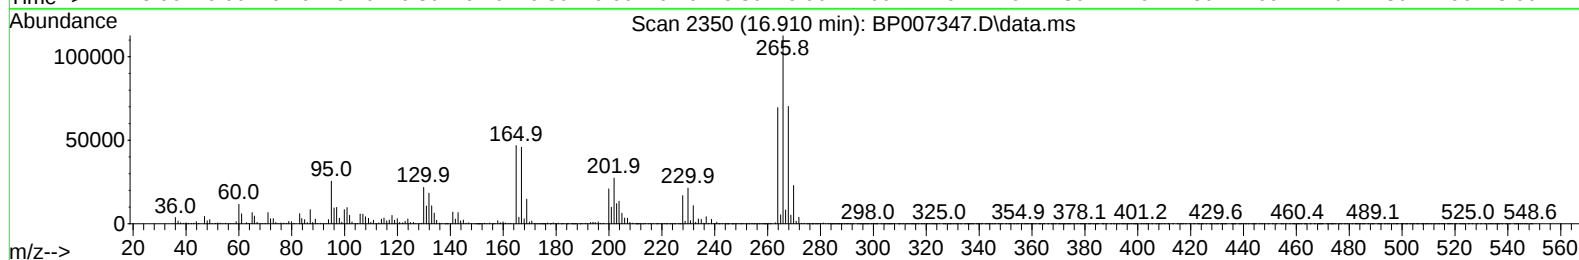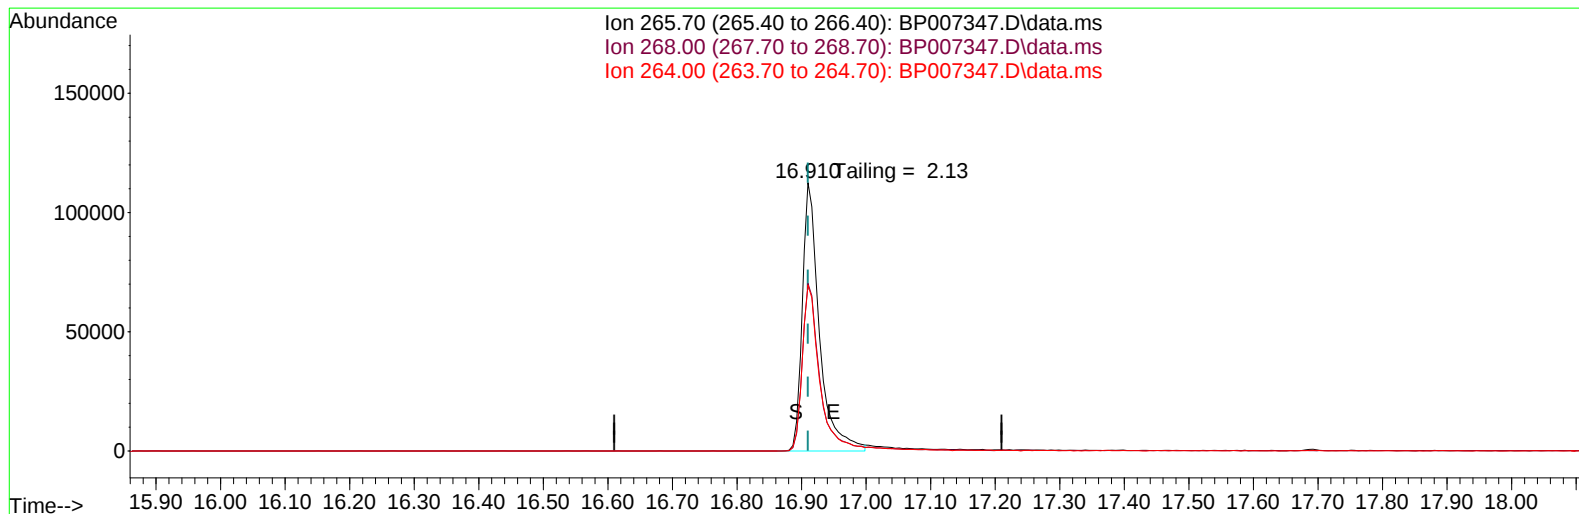

TIC: BP007347.D\data.ms

(70) Pentachlorophenol (C)

16.910min (+ 0.000) 582033.39 ng

response 210156

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.42
264.00	62.90	61.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/6/2021	BNA_P	<u>BP007347.D</u>
Compound Name	Response	Retention Time
DDT	746084	20.63
DDD	13948	20.21
DDE	1493	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15441	761525	2.03

Instrument :
BNA_P
ClientSampleId :
DFTPP