
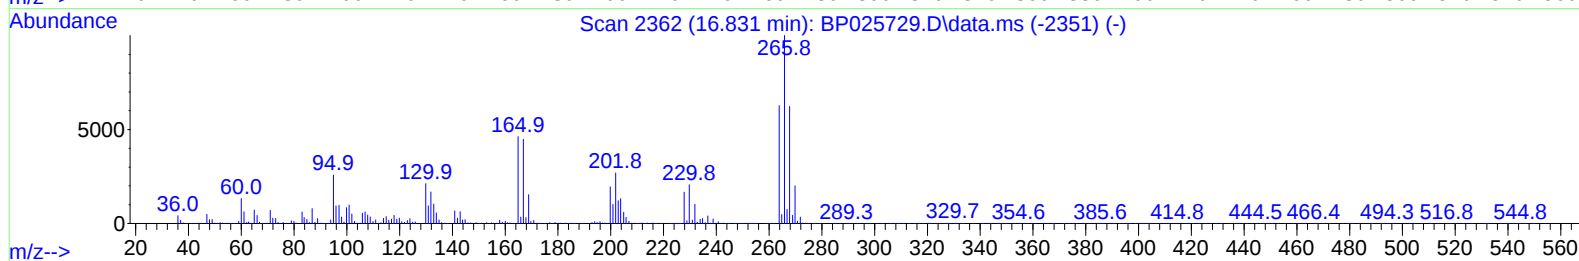
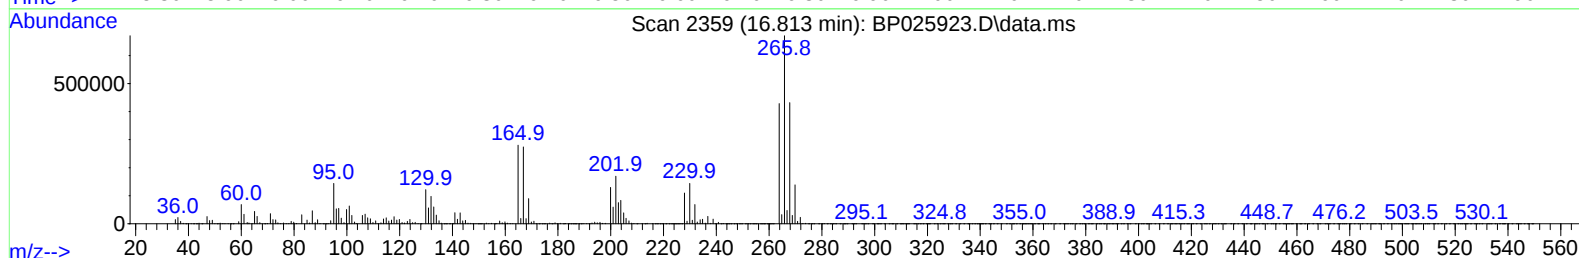


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100625\
Data File : BP025923.D
Acq On : 06 Oct 2025 14:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 14:34:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

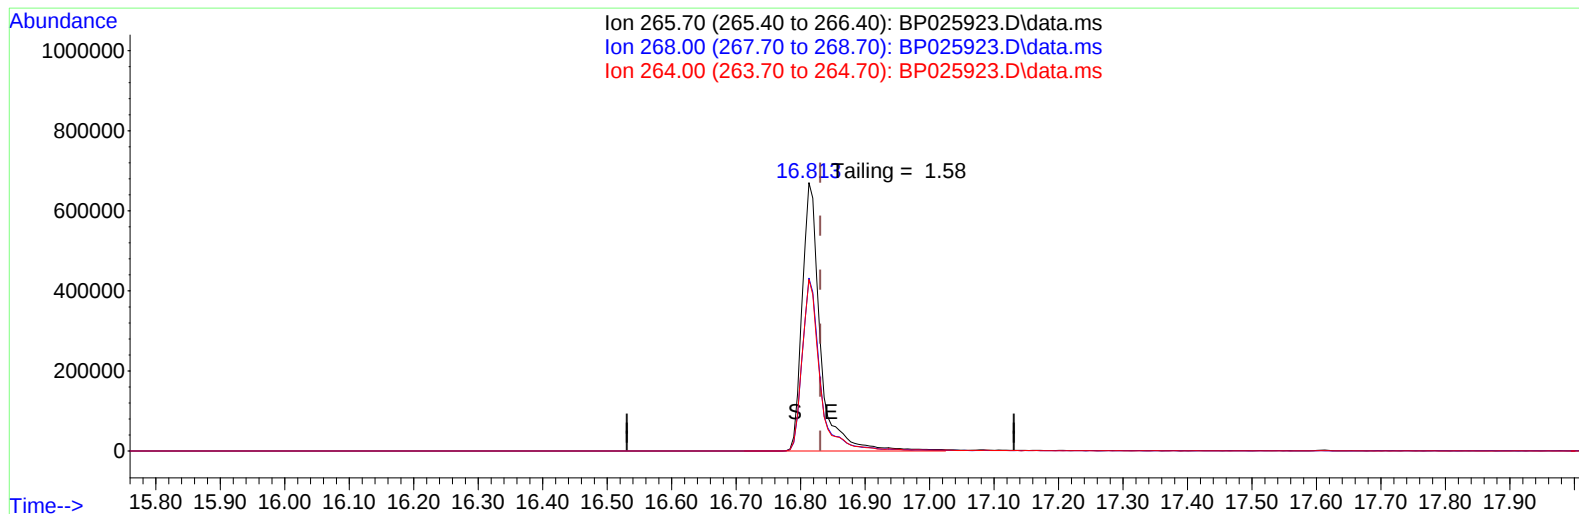

TIC: BP025923.D\data.ms

(70) Pentachlorophenol (C)




16.813min (-0.018) 3783600.35 ng

response 1315500

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.39
264.00	62.70	63.92
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100625\  
Data File : BP025923.D  
Acq On    : 06 Oct 2025  14:12  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Oct 06 14:34:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

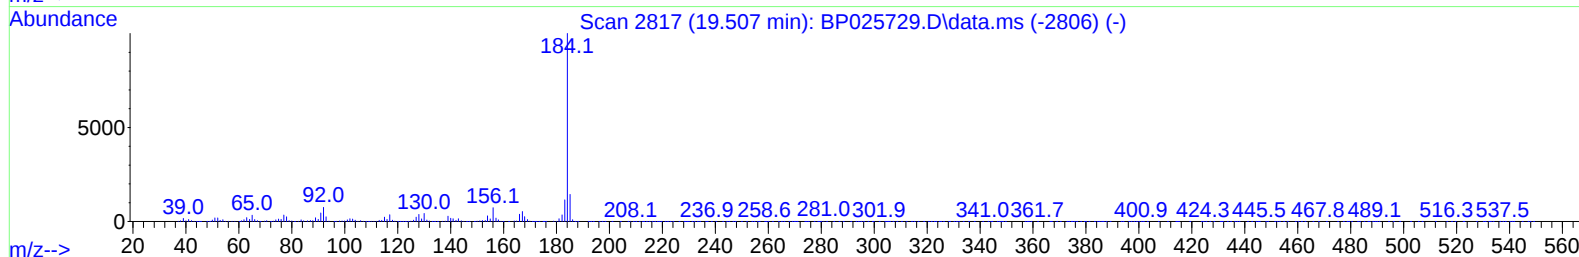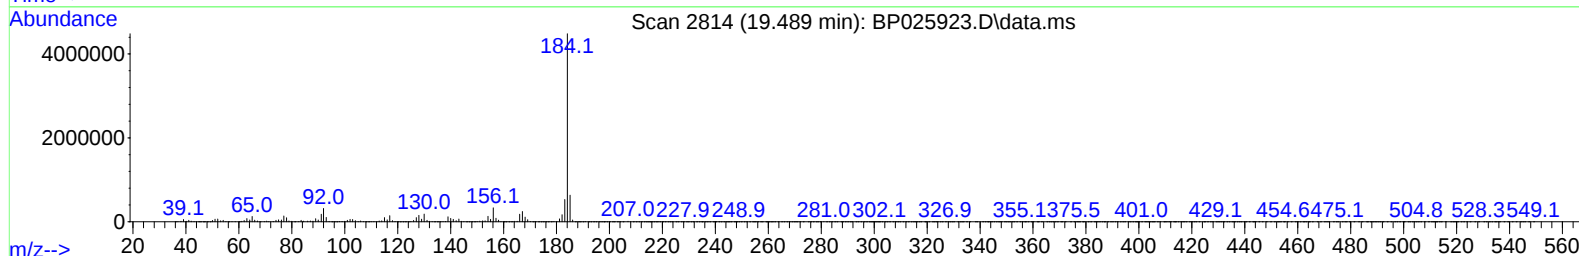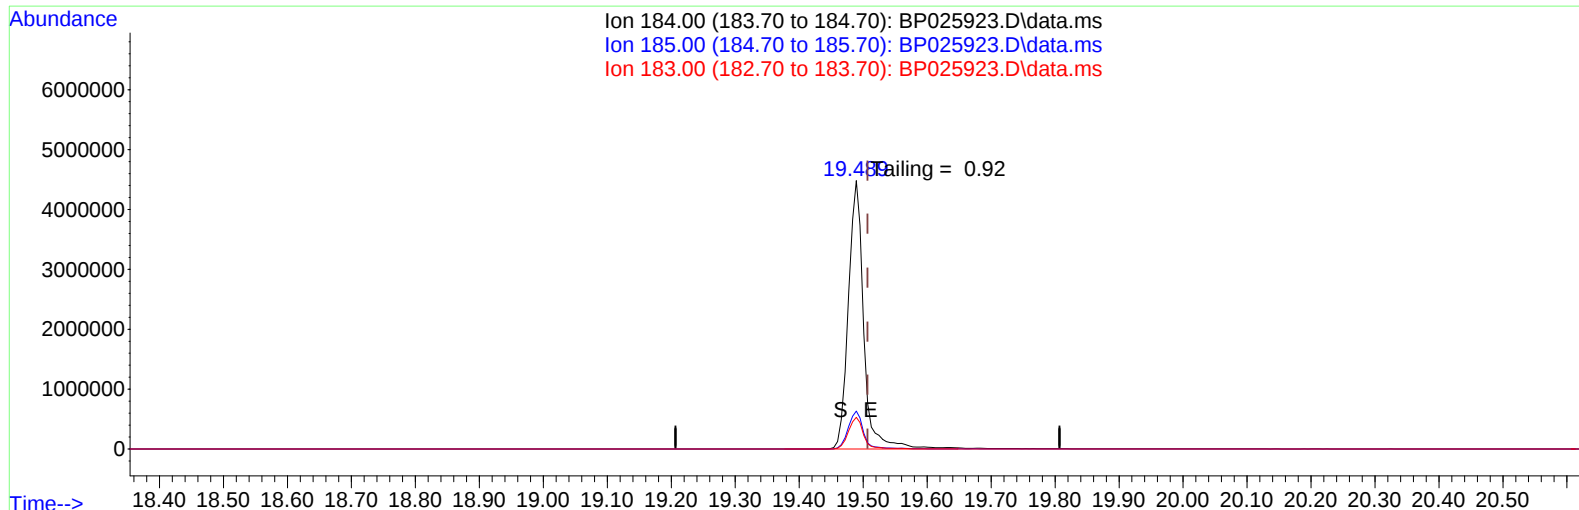

TIC: BP025923.D\data.ms

(77) Benzidine

19.489min (-0.018) 1941205.77 ng

response 7492893

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.14
183.00	11.50	11.84
0.00	0.00	0.00