
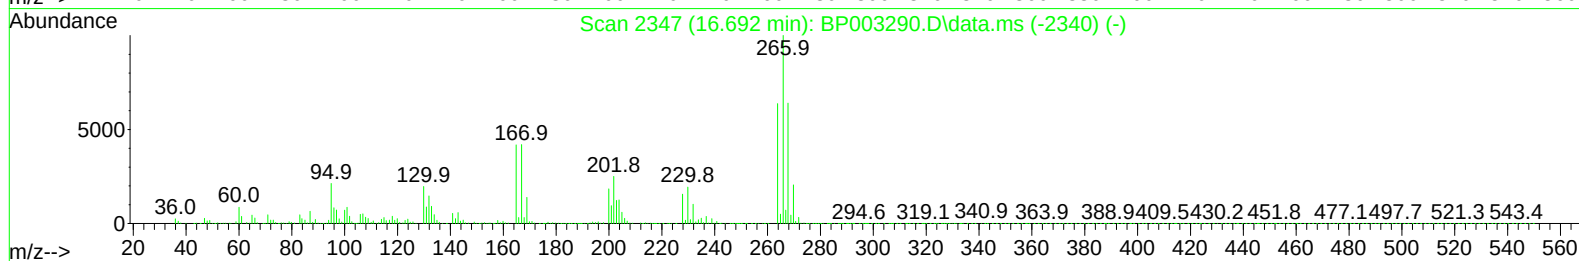
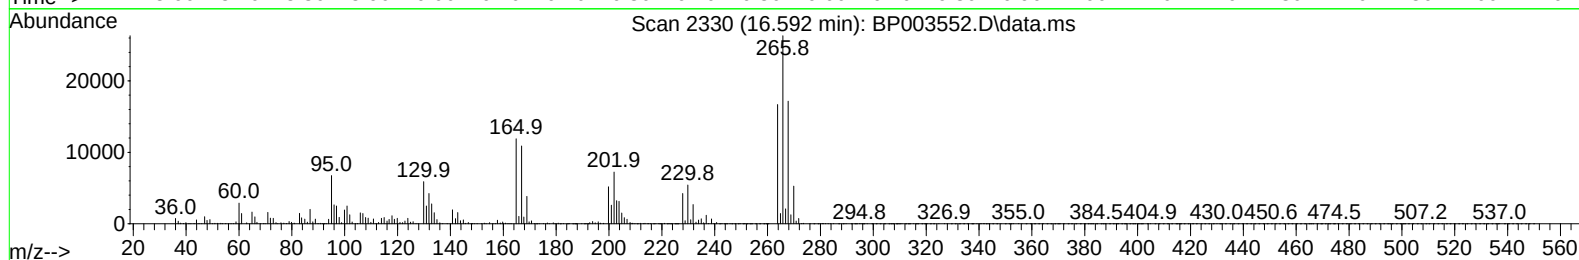


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100720\
Data File : BP003552.D
Acq On : 07 Oct 2020 14:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 05:35:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

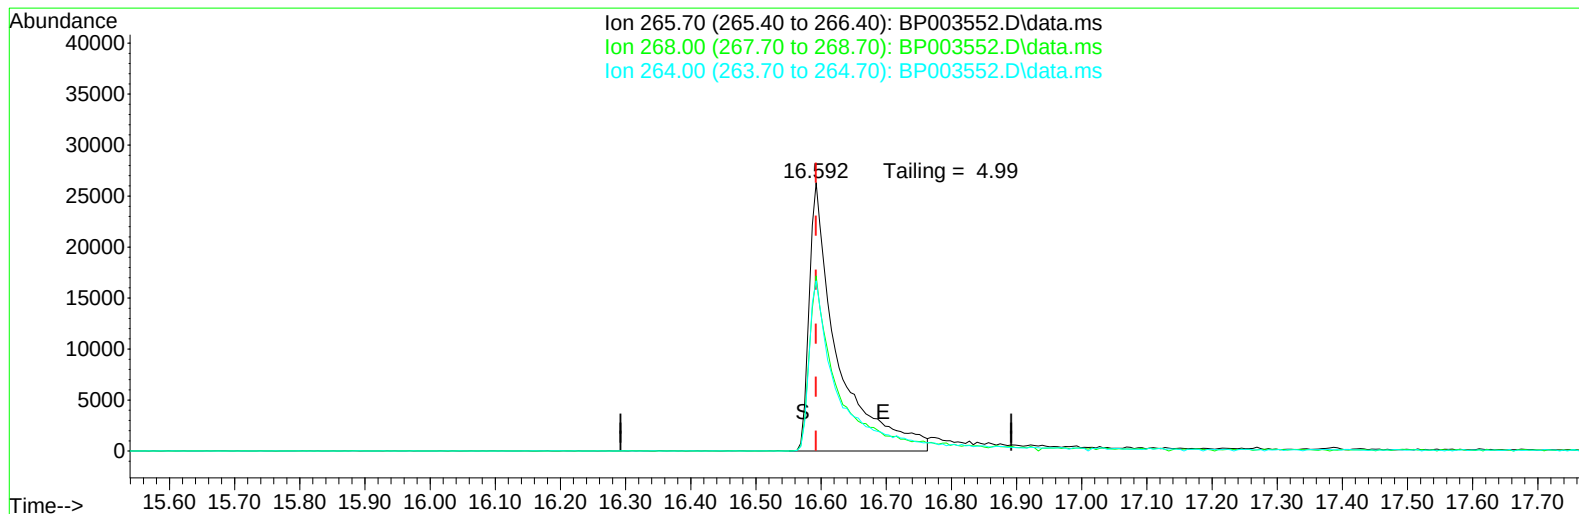

TIC: BP003552.D\data.ms

(70) Pentachlorophenol (C)




16.592min (+ 0.000) 585870.82 ng

response 78902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.23
264.00	63.30	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100720\
Data File : BP003552.D
Acq On : 07 Oct 2020 14:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 05:35:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 14:33:14 2020
Response via : Initial Calibration

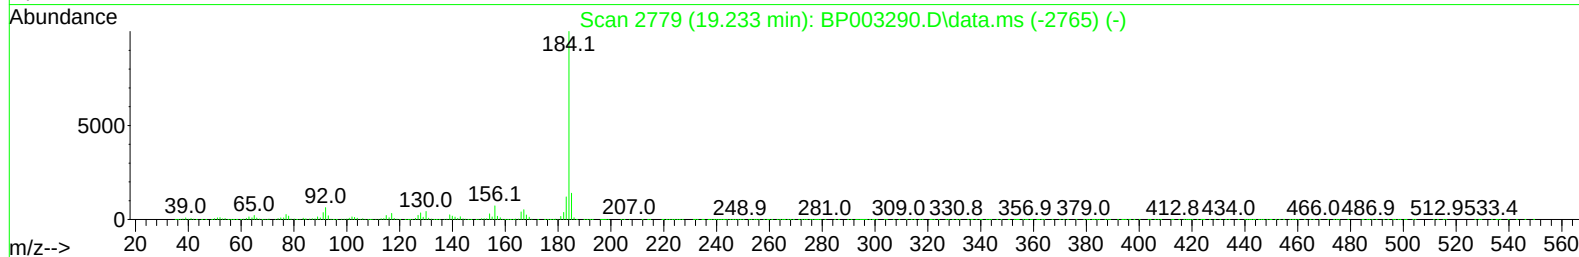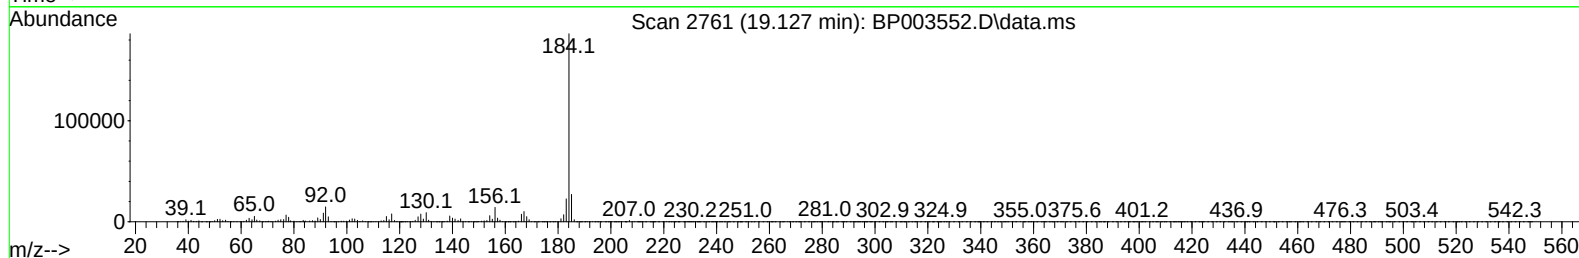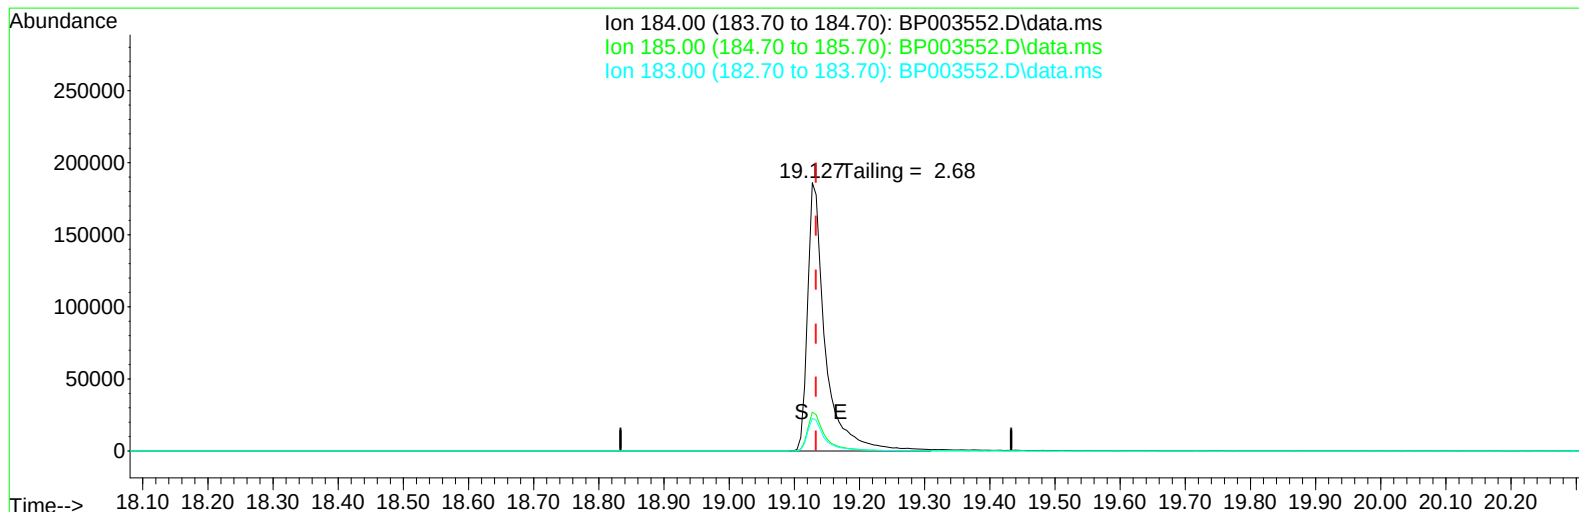

TIC: BP003552.D\data.ms

(77) Benzidine**19.127min (-0.006) 365438.23 ng****response 351286**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.53
183.00	12.00	12.20
0.00	0.00	0.00