
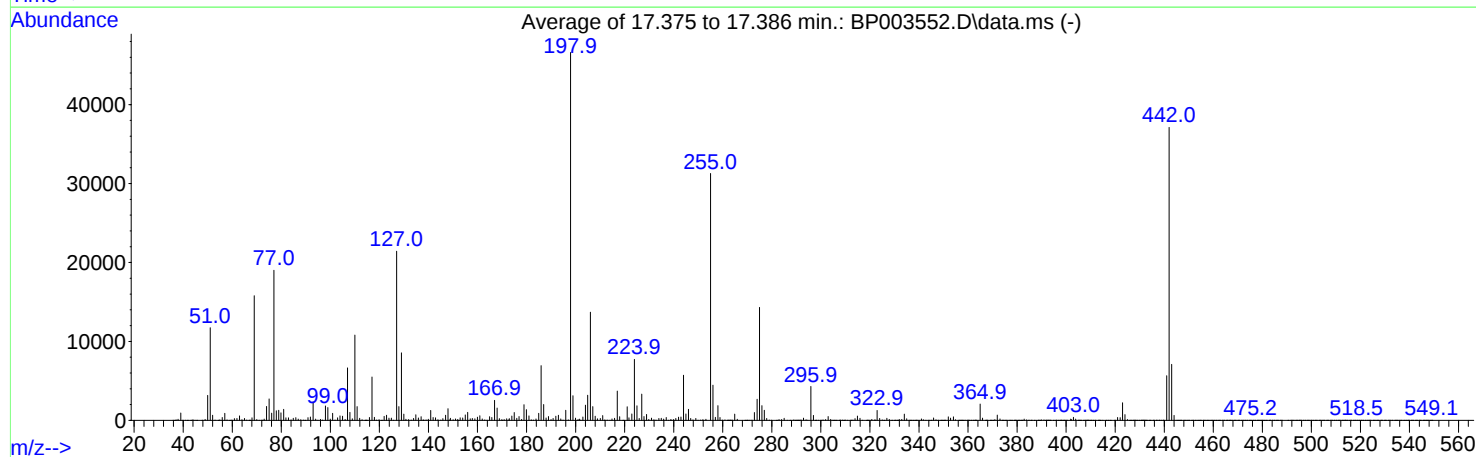


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100720\
Data File : BP003552.D
Acq On : 07 Oct 2020 14:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 05 14:33:14 2020

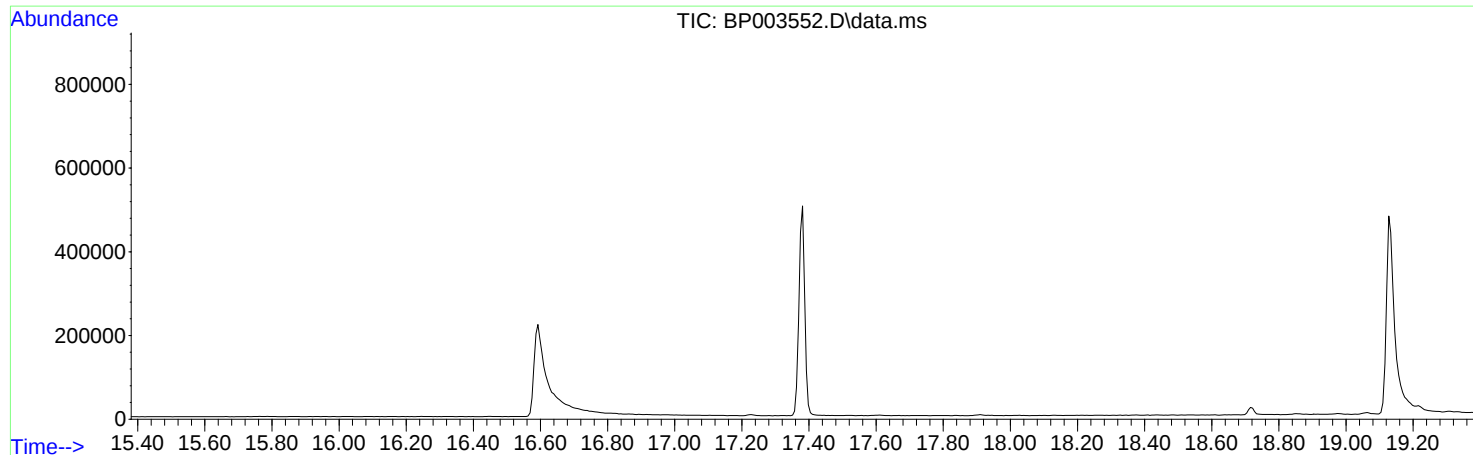

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	11738	PASS
68	69	0.00	2	2.0	319	PASS
69	198	0.00	100	33.9	15782	PASS
70	69	0.00	2	0.6	97	PASS
127	198	10	80	46.0	21420	PASS
197	198	0.00	2	0.1	55	PASS
198	198	100	100	100.0	46600	PASS
199	198	5	9	6.7	3114	PASS
275	198	10	60	30.7	14308	PASS
365	198	1	100	4.4	2072	PASS
441	198	0.01	100	12.1	5647	PASS
442	198	50	100	79.7	37117	PASS
443	442	15	24	19.1	7087	PASS