
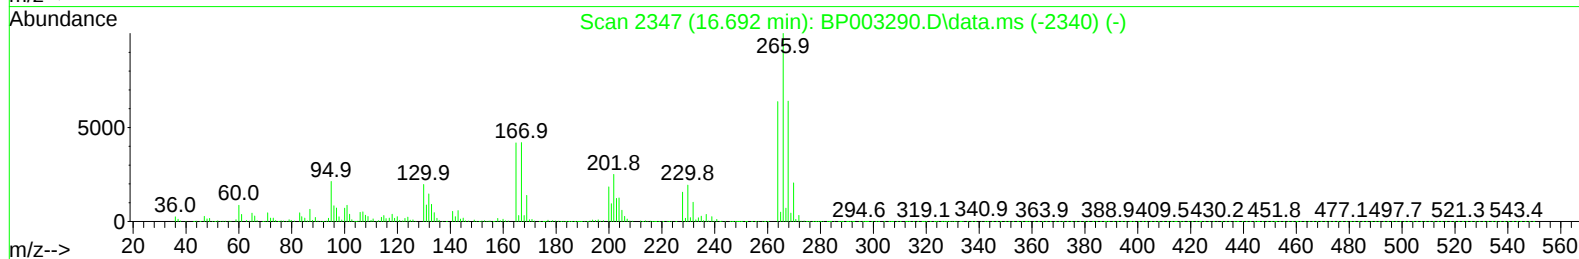
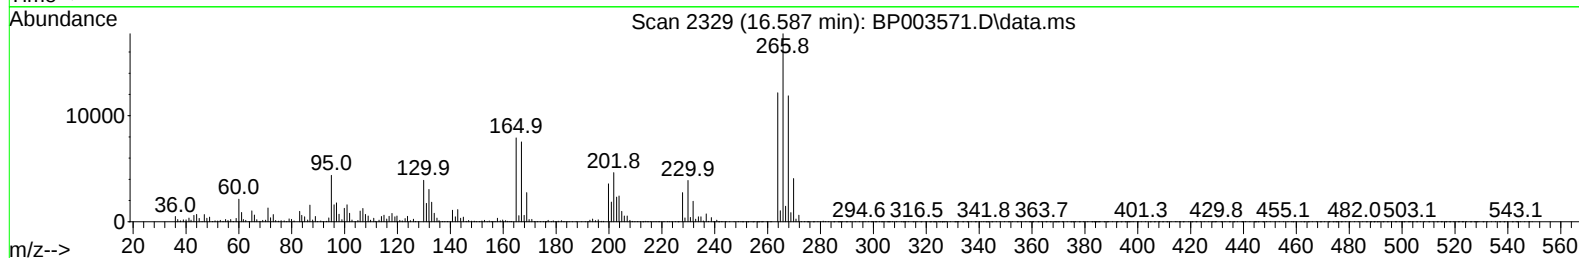


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100820\
Data File : BP003571.D
Acq On : 08 Oct 2020 14:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 05:38:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 08 15:55:58 2020
Response via : Initial Calibration

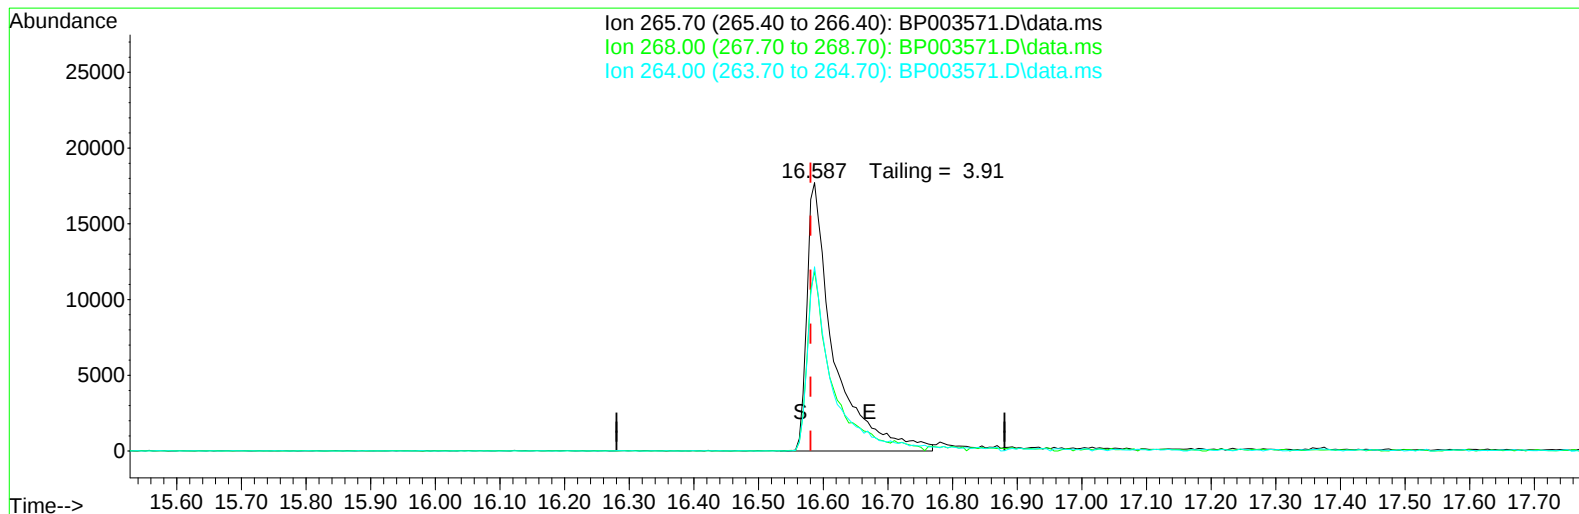

TIC: BP003571.D\data.ms

(70) Pentachlorophenol (C)




16.587min (+ 0.006) 840771.73 ng

response 50954

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	66.98
264.00	63.30	68.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100820\
Data File : BP003571.D
Acq On : 08 Oct 2020 14:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 05:38:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 08 15:55:58 2020
Response via : Initial Calibration

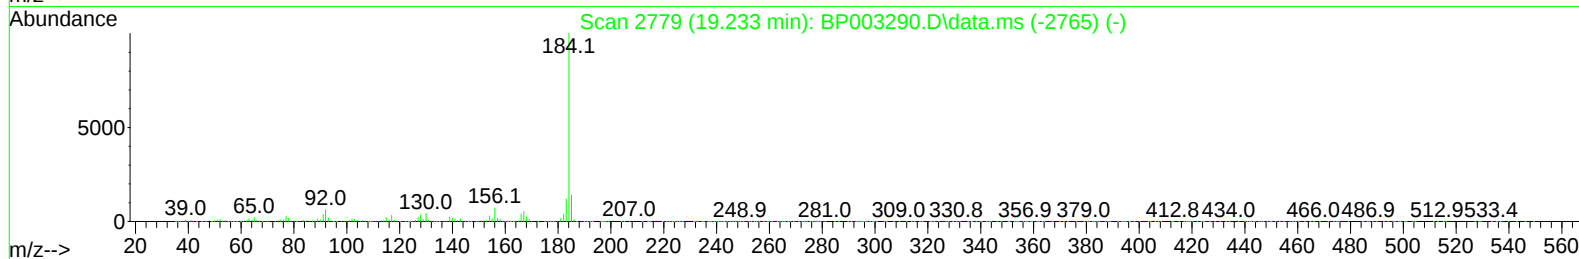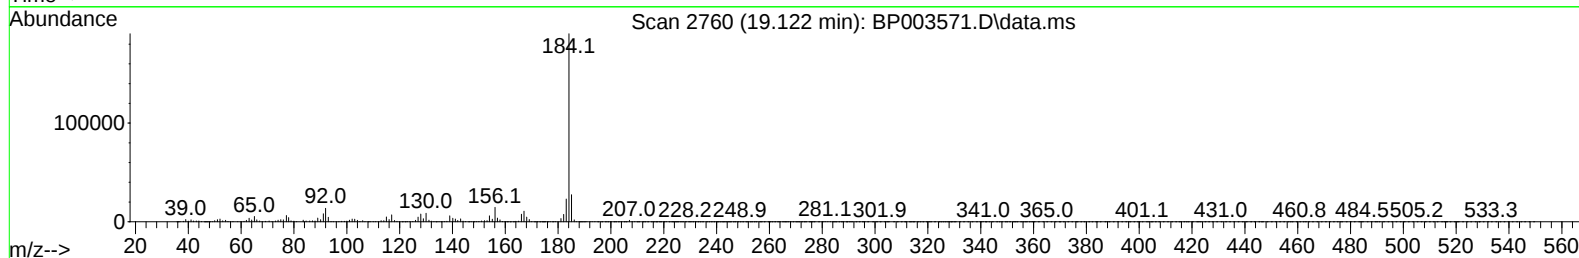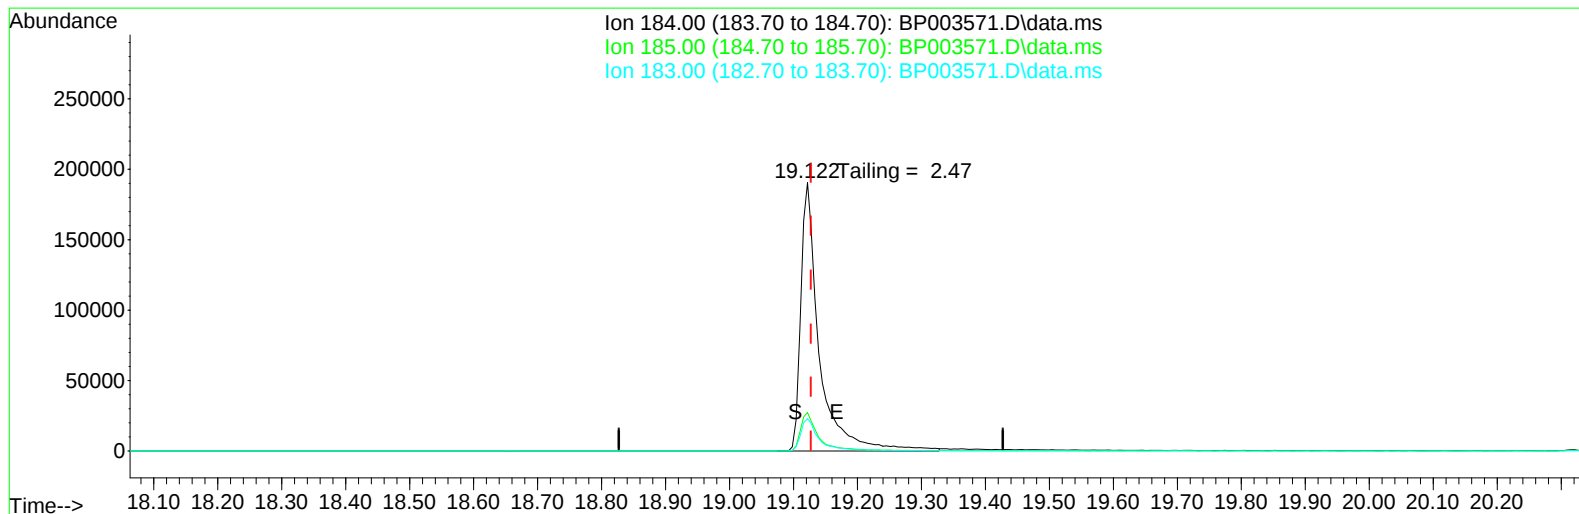

TIC: BP003571.D\data.ms

(77) Benzidine**19.122min (-0.006) 224971.81 ng****response 383686**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.39
183.00	12.00	12.09
0.00	0.00	0.00