
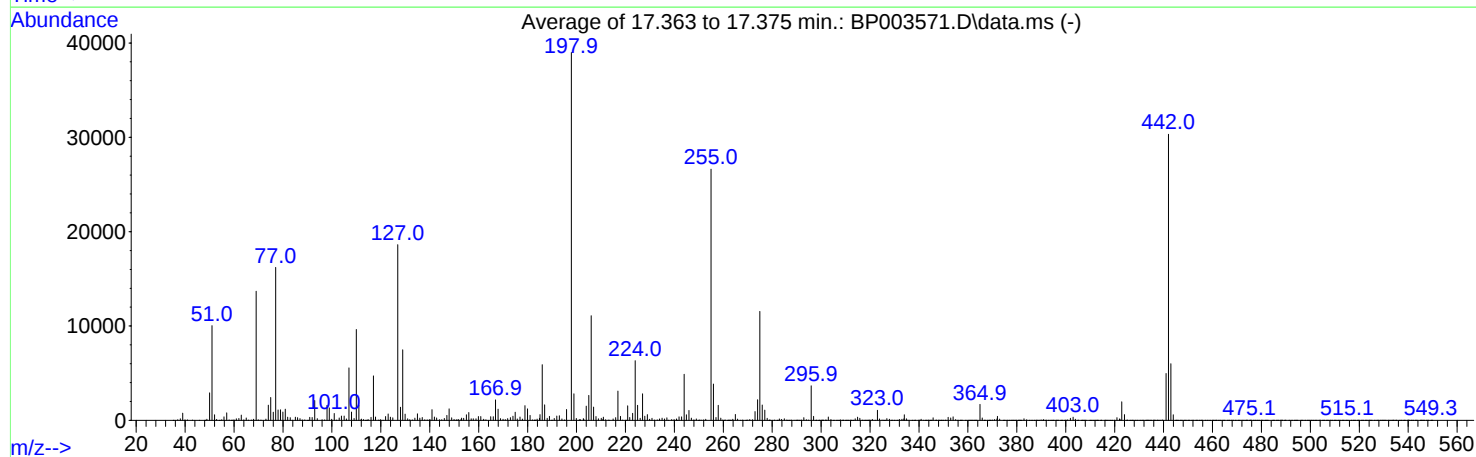


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100820\
Data File : BP003571.D
Acq On : 08 Oct 2020 14:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP091520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 08 15:55:58 2020

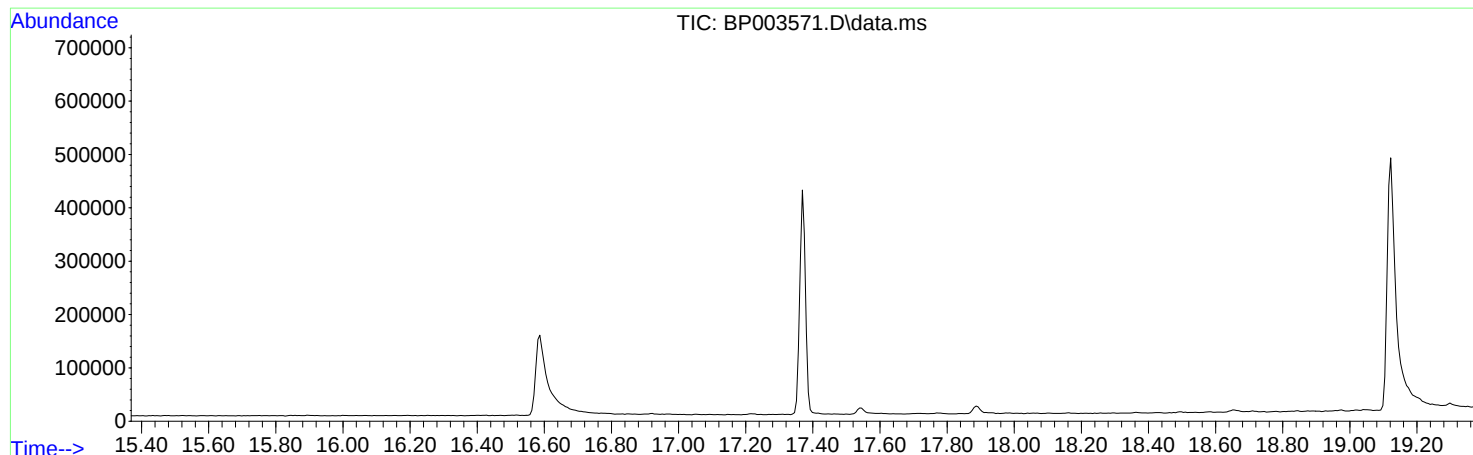

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	10047	PASS
68	69	0.00	2	0.9	117	PASS
69	198	0.00	100	35.1	13683	PASS
70	69	0.00	2	0.5	75	PASS
127	198	10	80	47.8	18619	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38992	PASS
199	198	5	9	7.2	2822	PASS
275	198	10	60	29.6	11551	PASS
365	198	1	100	4.3	1690	PASS
441	198	0.01	100	12.8	4974	PASS
442	198	50	100	77.8	30331	PASS
443	442	15	24	19.8	5996	PASS