


1,4-Dioxane

Response Ratio

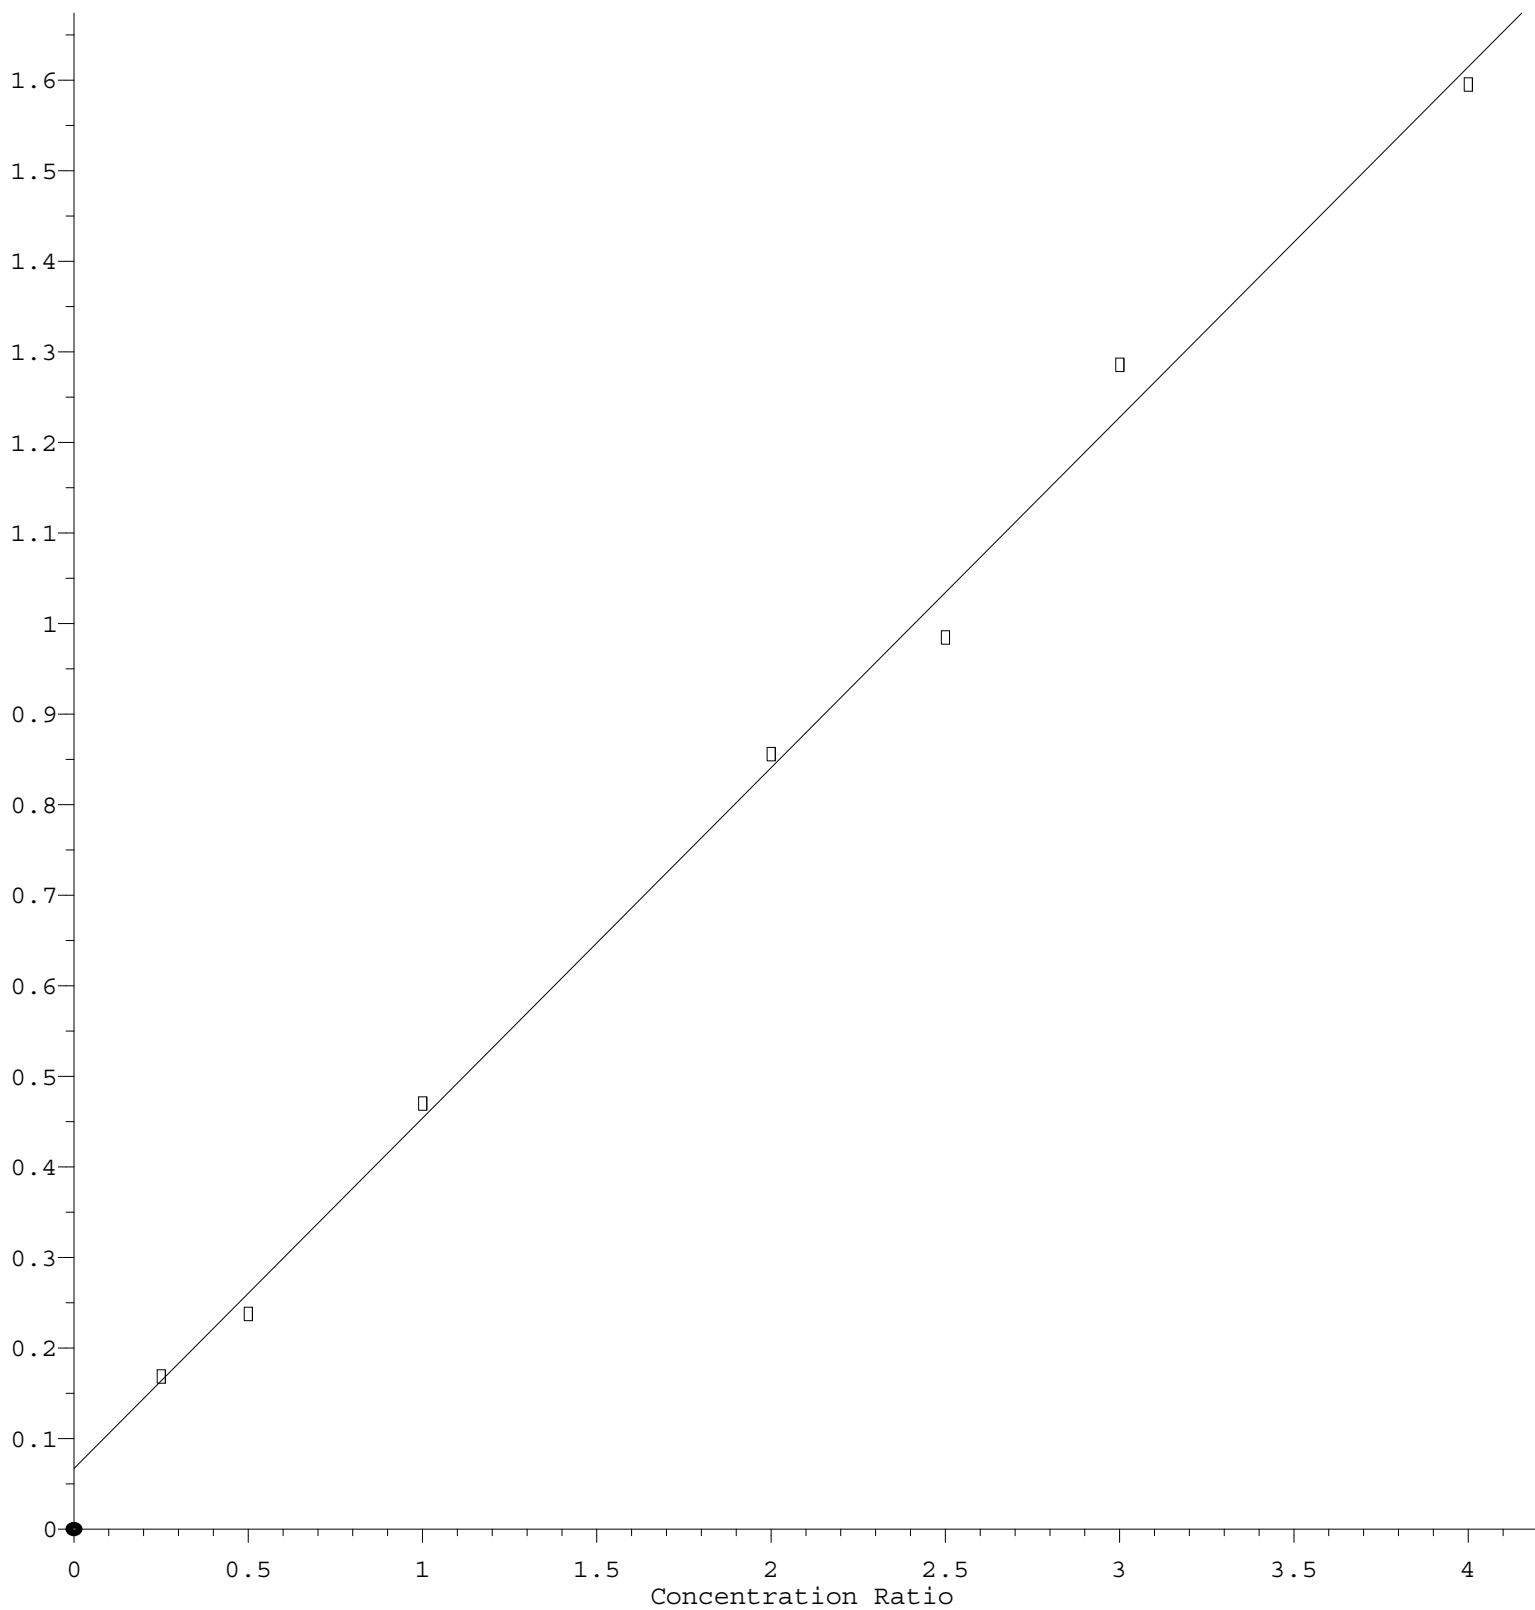

$$\text{Response} = 3.873\text{e-}001 * \text{Amt} + 6.658\text{e-}002$$


Coef of Det (r^2) = 0.995826 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP100821.M

Calibration Table Last Updated: Fri Oct 08 15:35:55 2021

4-Chloro-3-methylphenol

Response Ratio

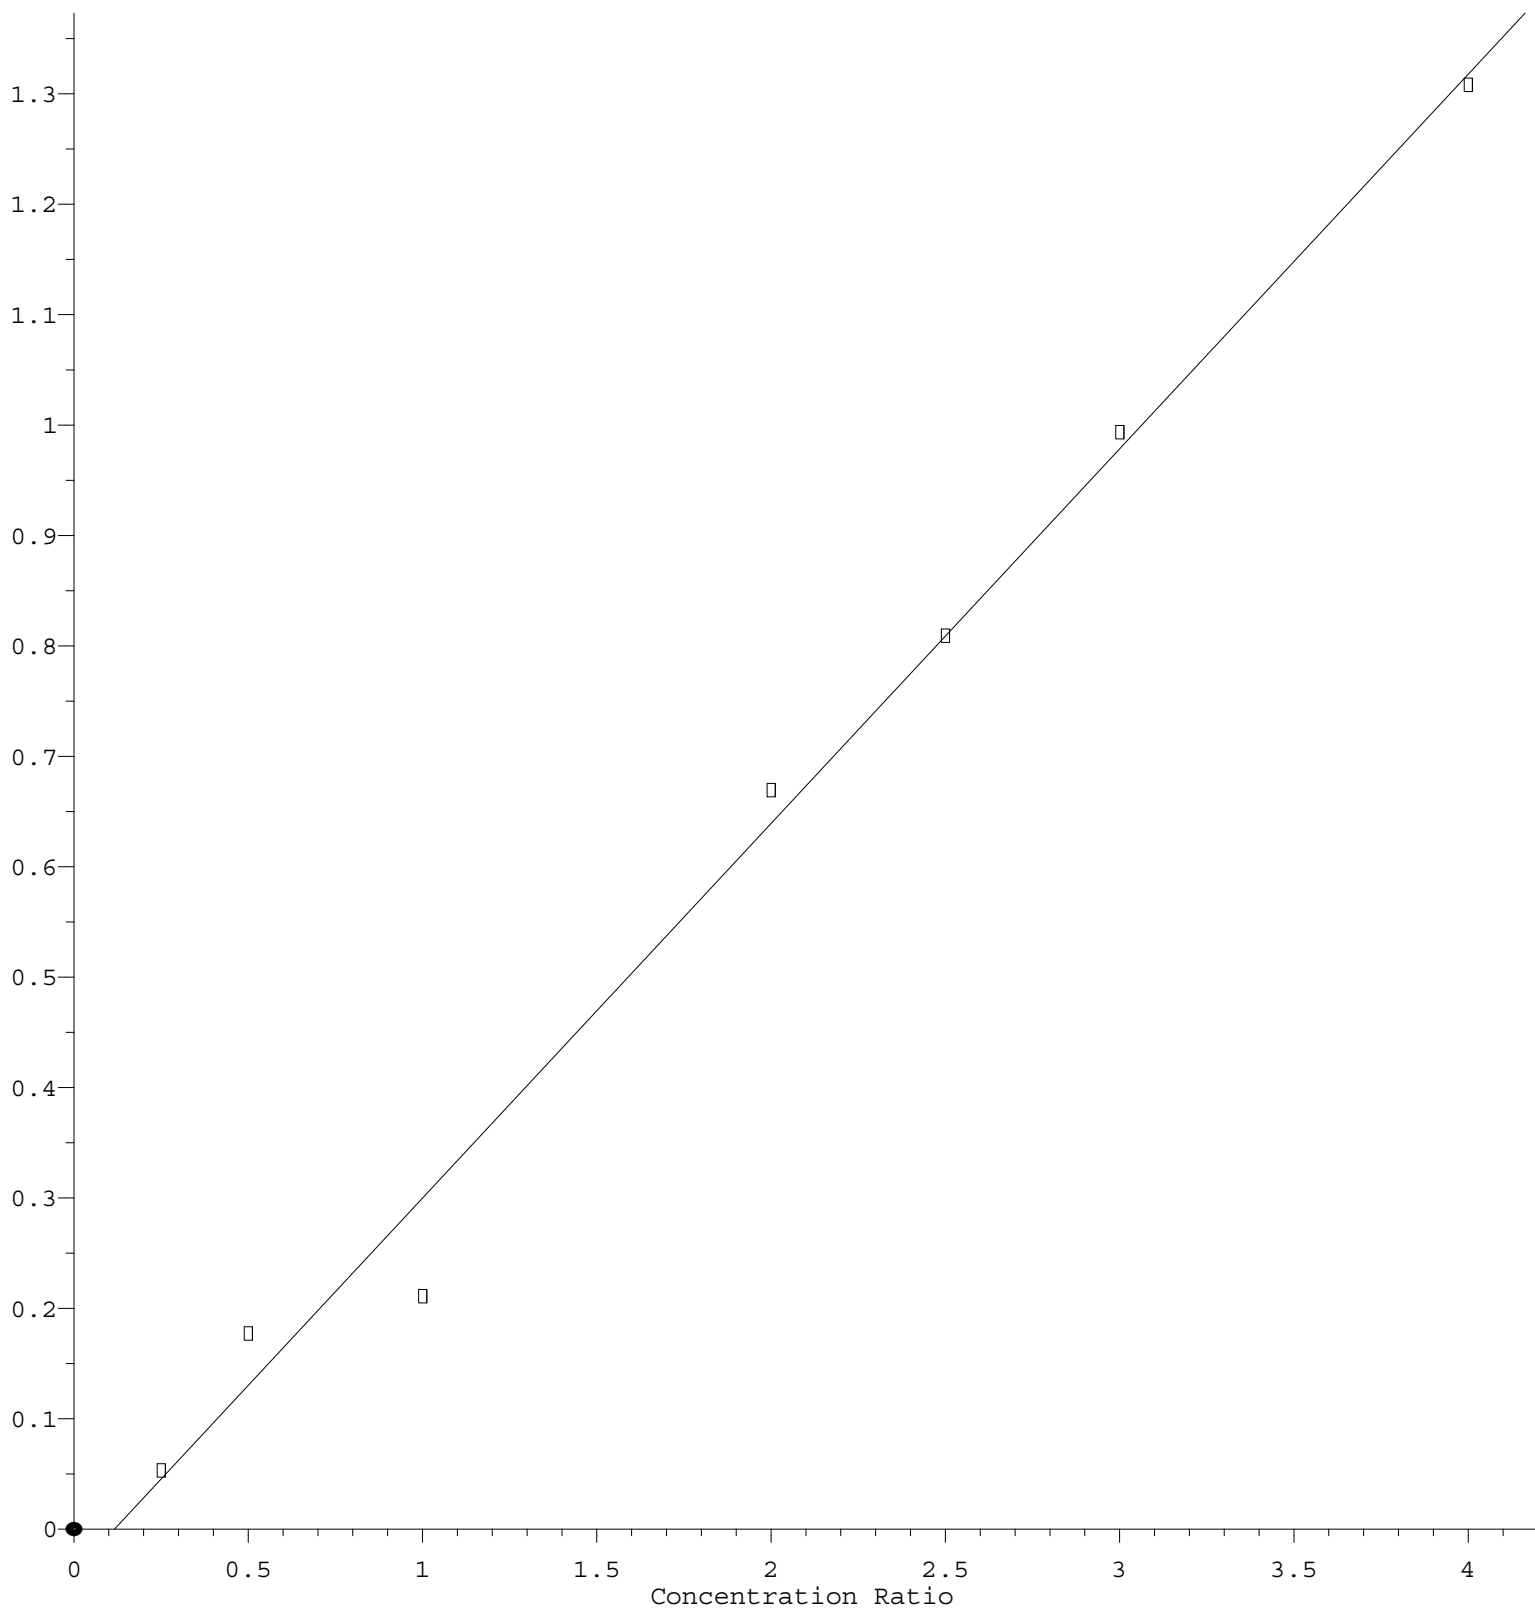


$$\text{Response} = 3.394\text{e-}001 * \text{Amt} - 3.932\text{e-}002$$

Coef of Det (r^2) = 0.991452 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP100821.M

Calibration Table Last Updated: Fri Oct 08 15:35:55 2021


Hexachlorocyclopentadiene

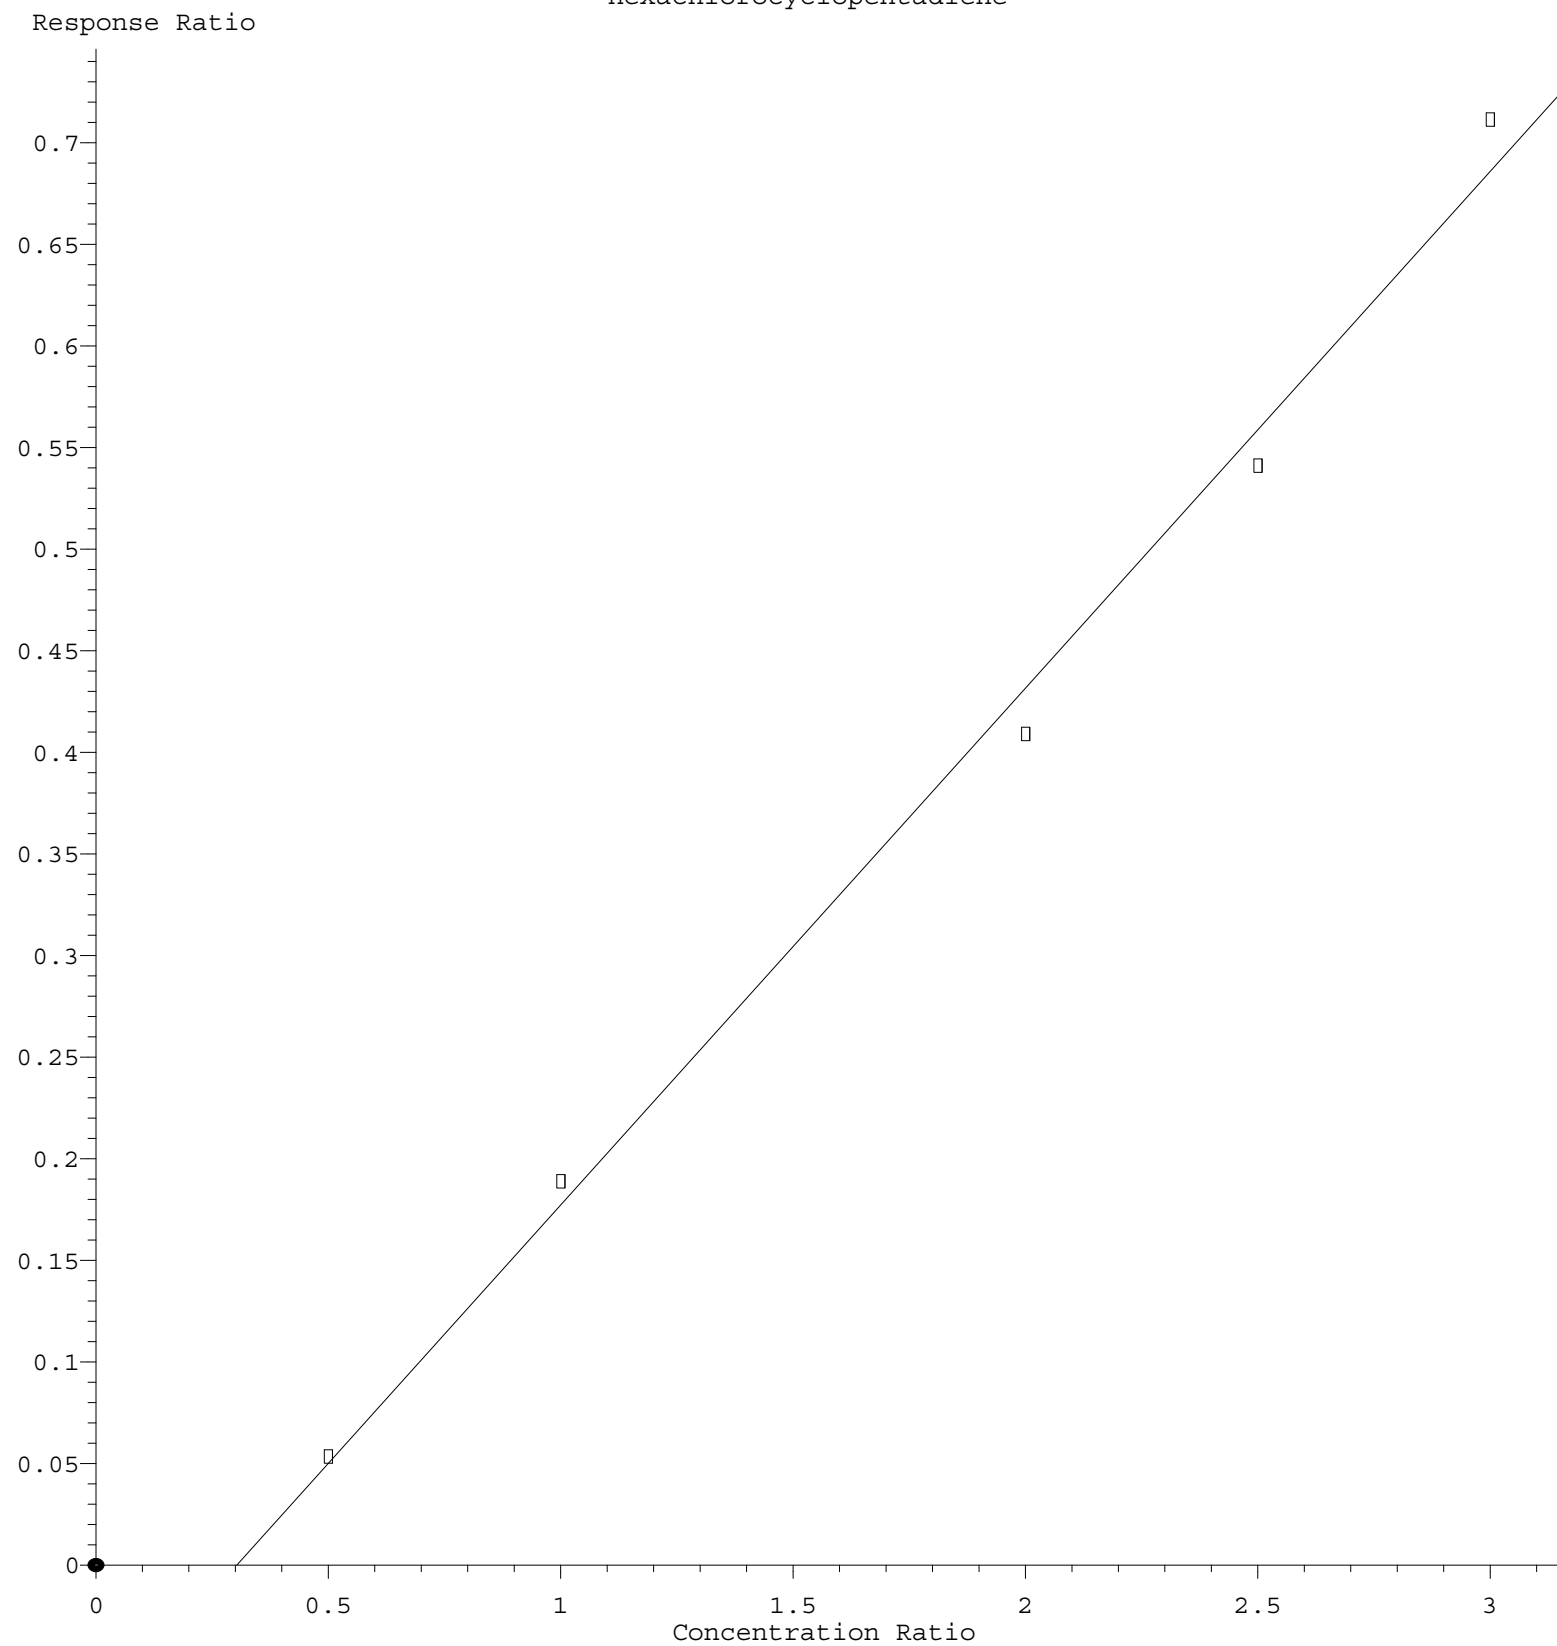

Response = $2.543 \times 10^{-1} \times \text{Amt} - 7.698 \times 10^{-2}$
Coef of Det (r^2) = 0.994223 Curve Fit: Linear
Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP100821.M
Calibration Table Last Updated: Fri Oct 08 15:35:55 2021

n-Nitrosodiphenylamine

Response Ratio

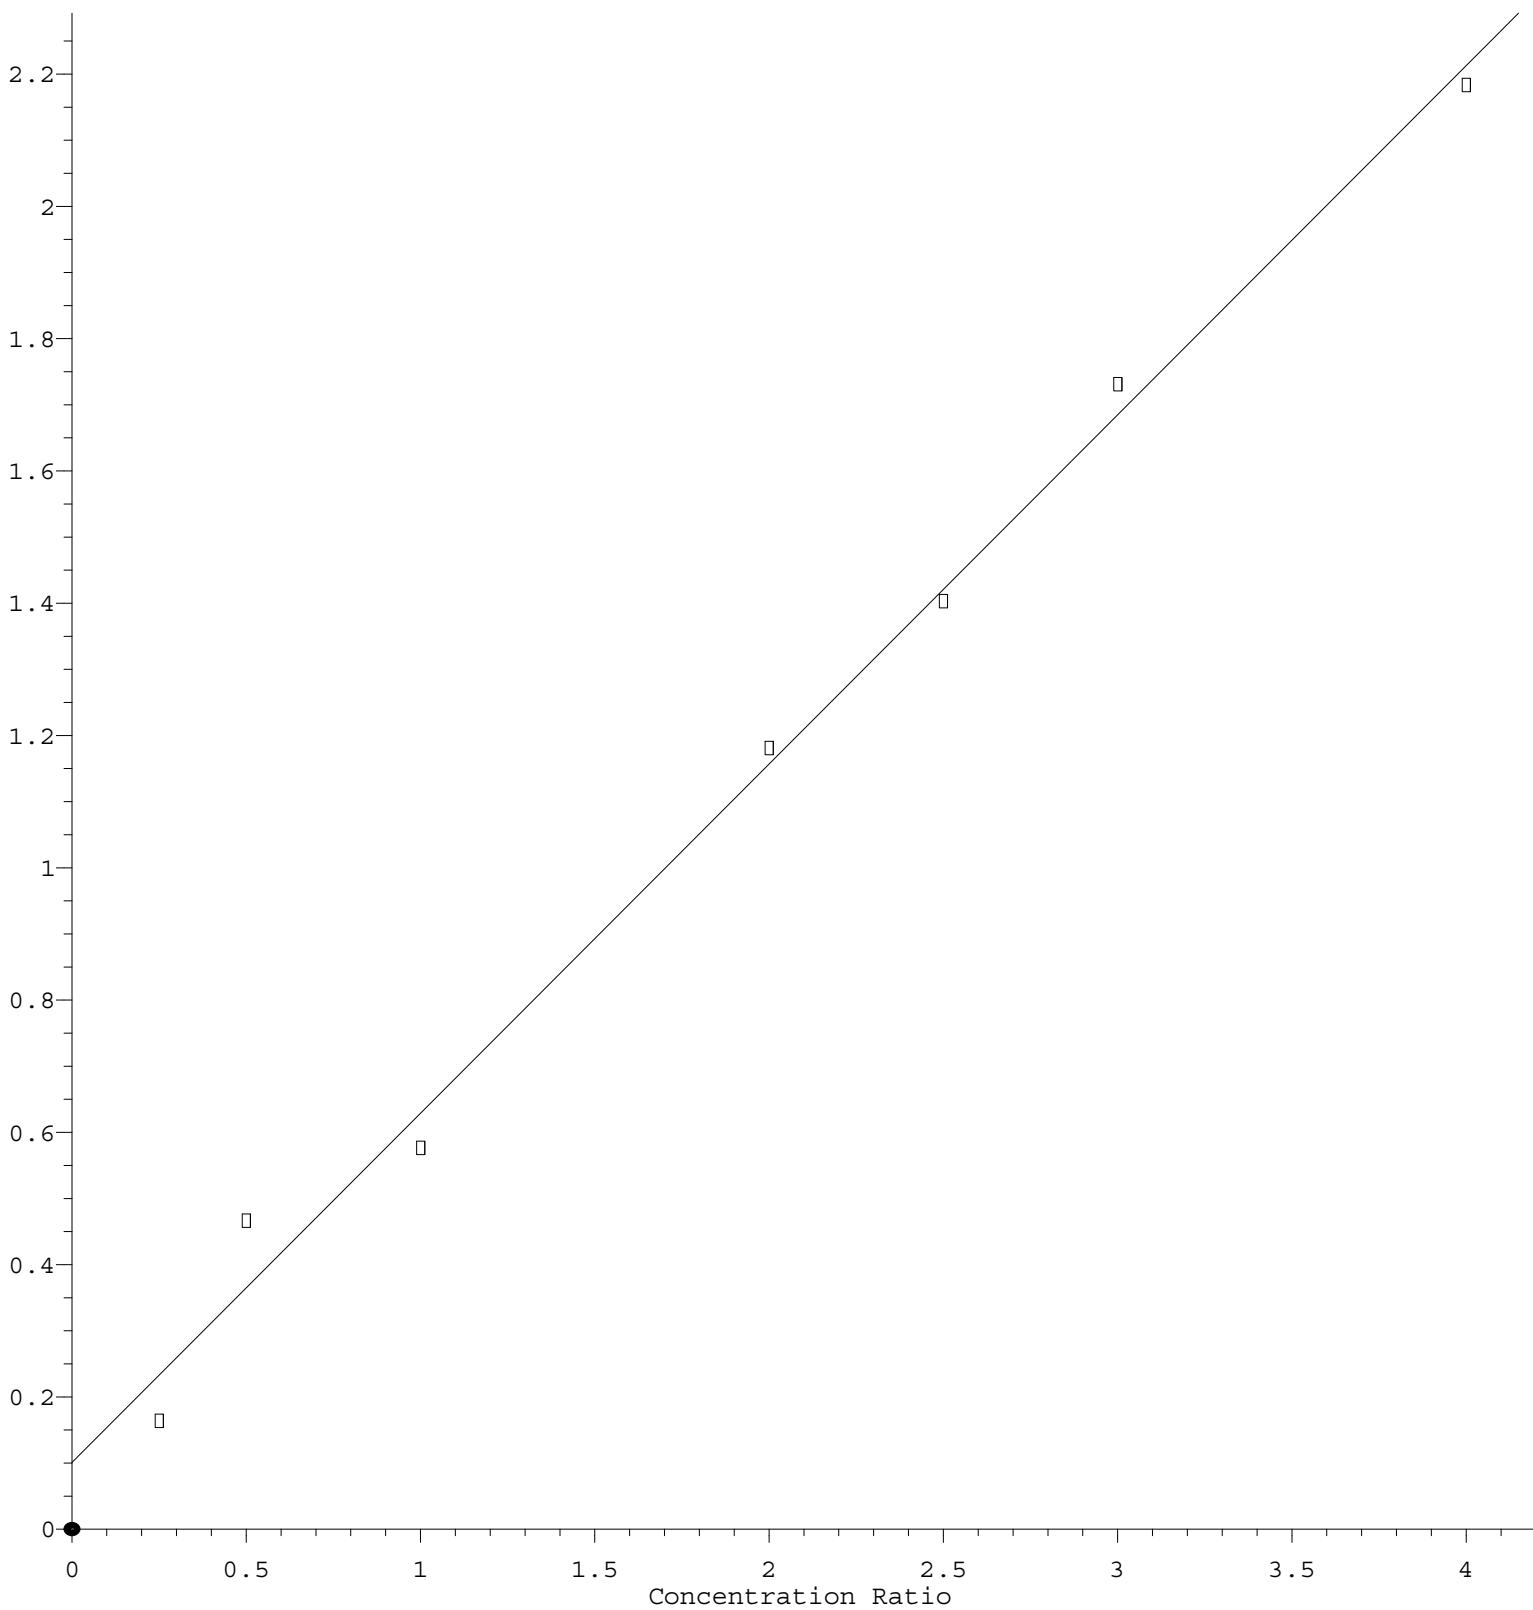

$$\text{Response} = 5.280\text{e-}001 * \text{Amt} + 1.013\text{e-}001$$


Coef of Det (r^2) = 0.993263 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP100821.M

Calibration Table Last Updated: Fri Oct 08 15:35:55 2021

Hexachlorobenzene

Response Ratio

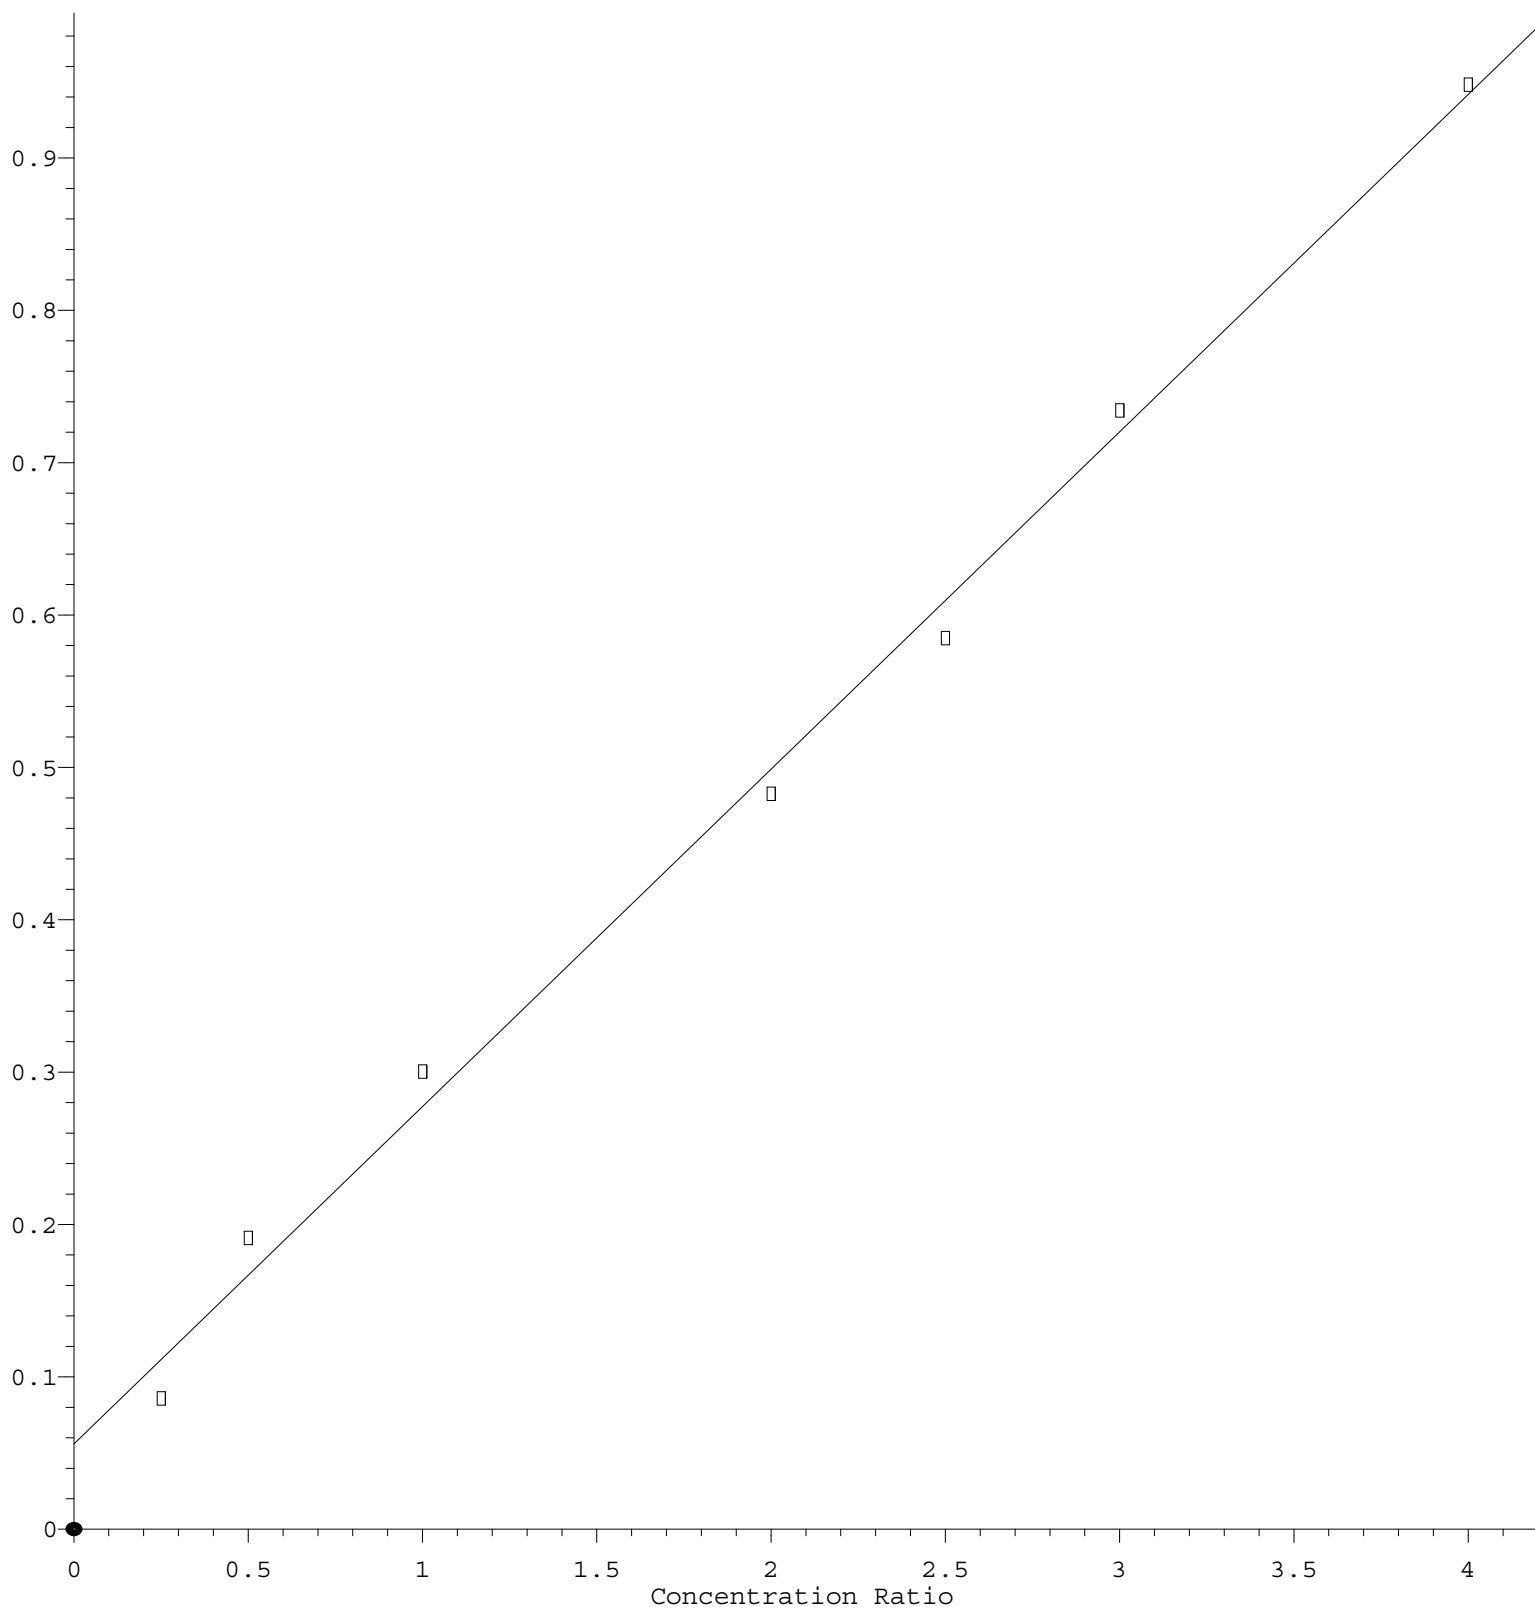


$$\text{Response} = 2.214\text{e-}001 * \text{Amt} + 5.621\text{e-}002$$

Coef of Det (r^2) = 0.994901 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP100821.M

Calibration Table Last Updated: Fri Oct 08 15:35:55 2021


Atrazine

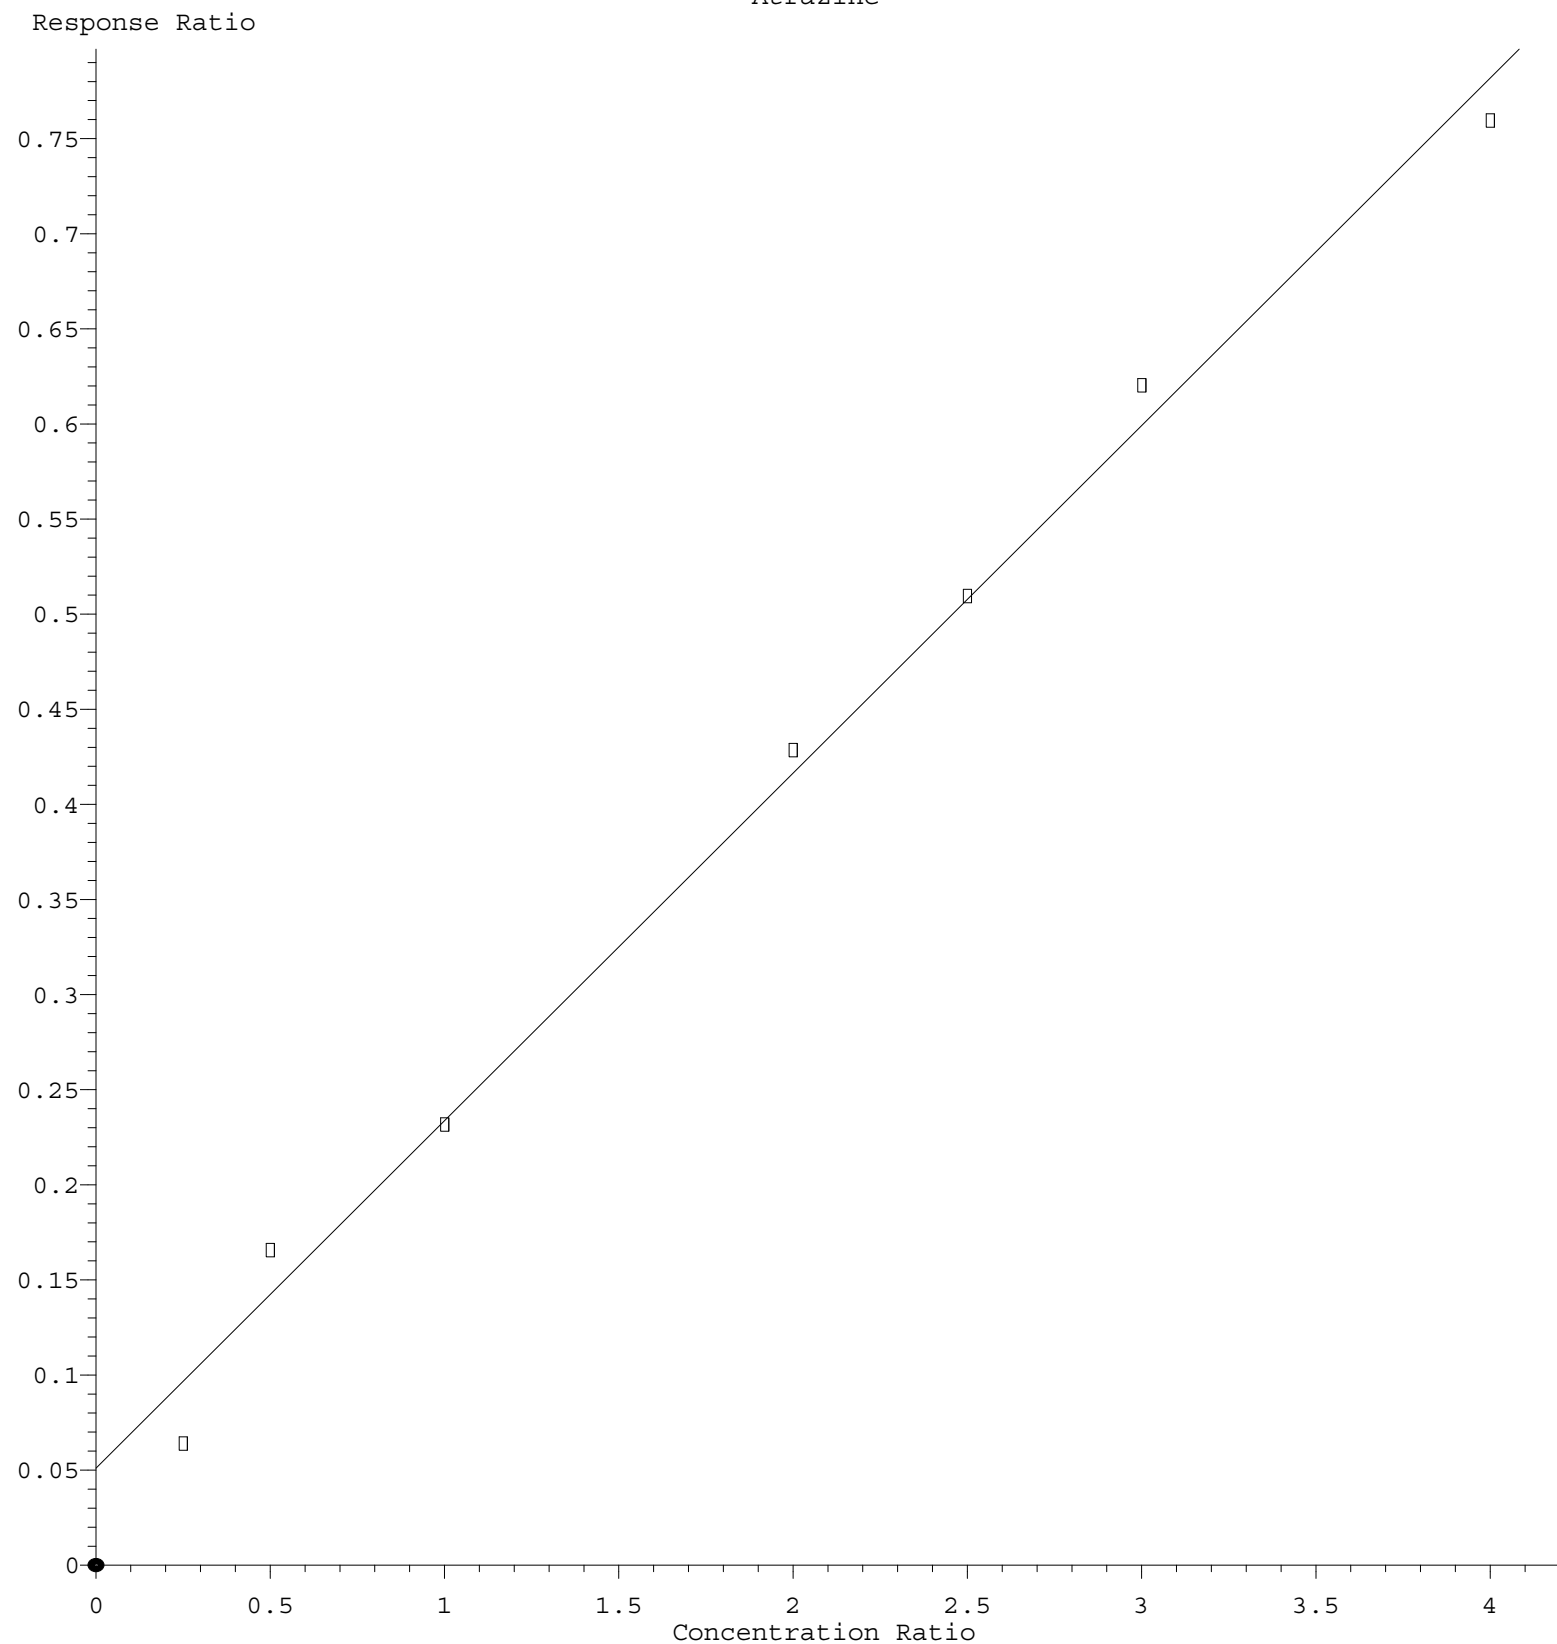

Response = 1.829e-001 * Amt + 5.084e-002
 Coef of Det (r^2) = 0.992986 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP100821.M
 Calibration Table Last Updated: Fri Oct 08 15:35:55 2021

Benzo (b) fluoranthene

Response Ratio

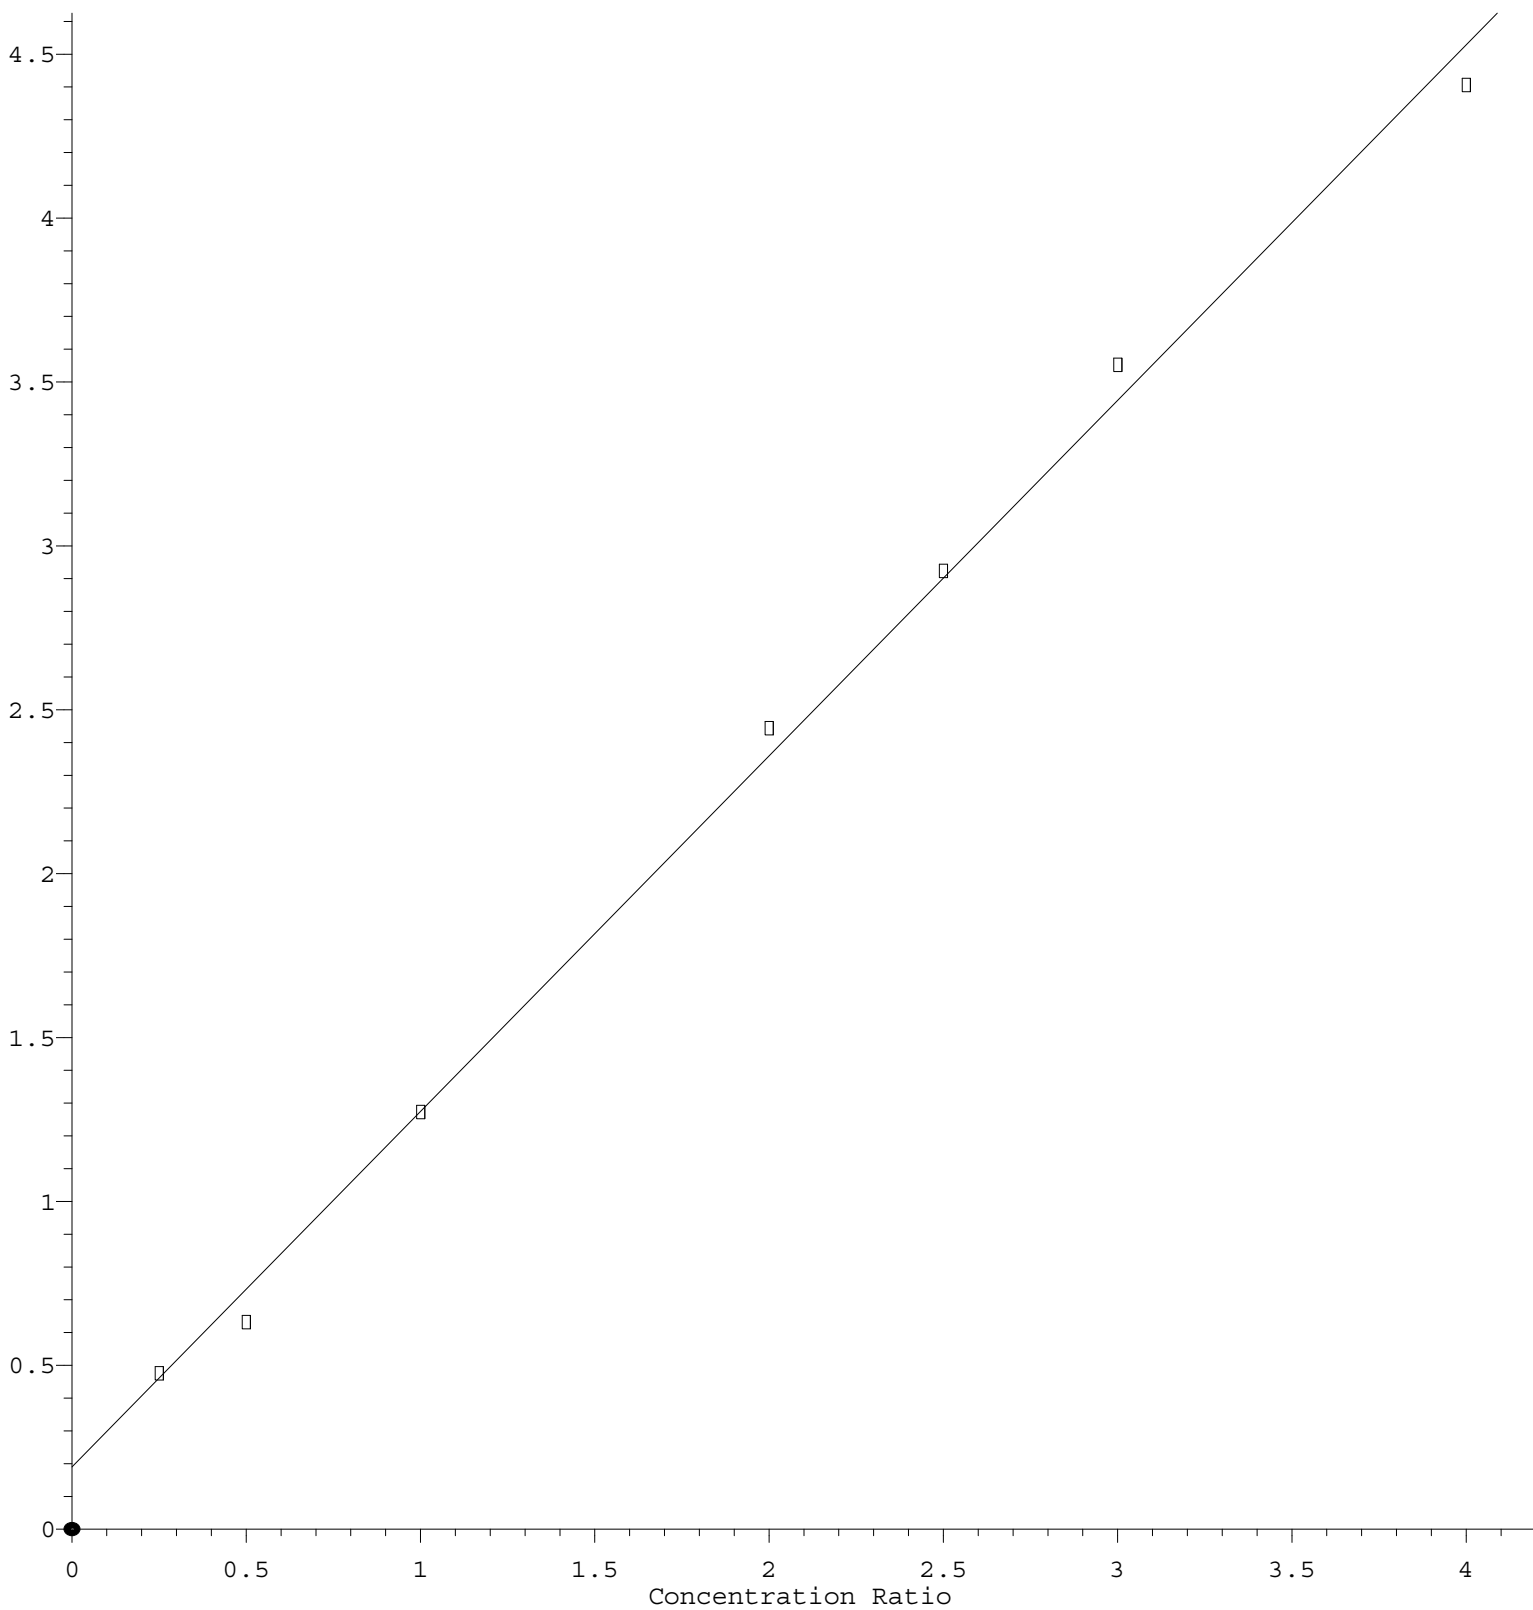

$$\text{Response} = 1.085\text{e}+000 * \text{Amt} + 1.903\text{e}-001$$


Coef of Det (r^2) = 0.996707 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP100821.M

Calibration Table Last Updated: Fri Oct 08 15:35:55 2021

Benzo (k) fluoranthene

Response Ratio

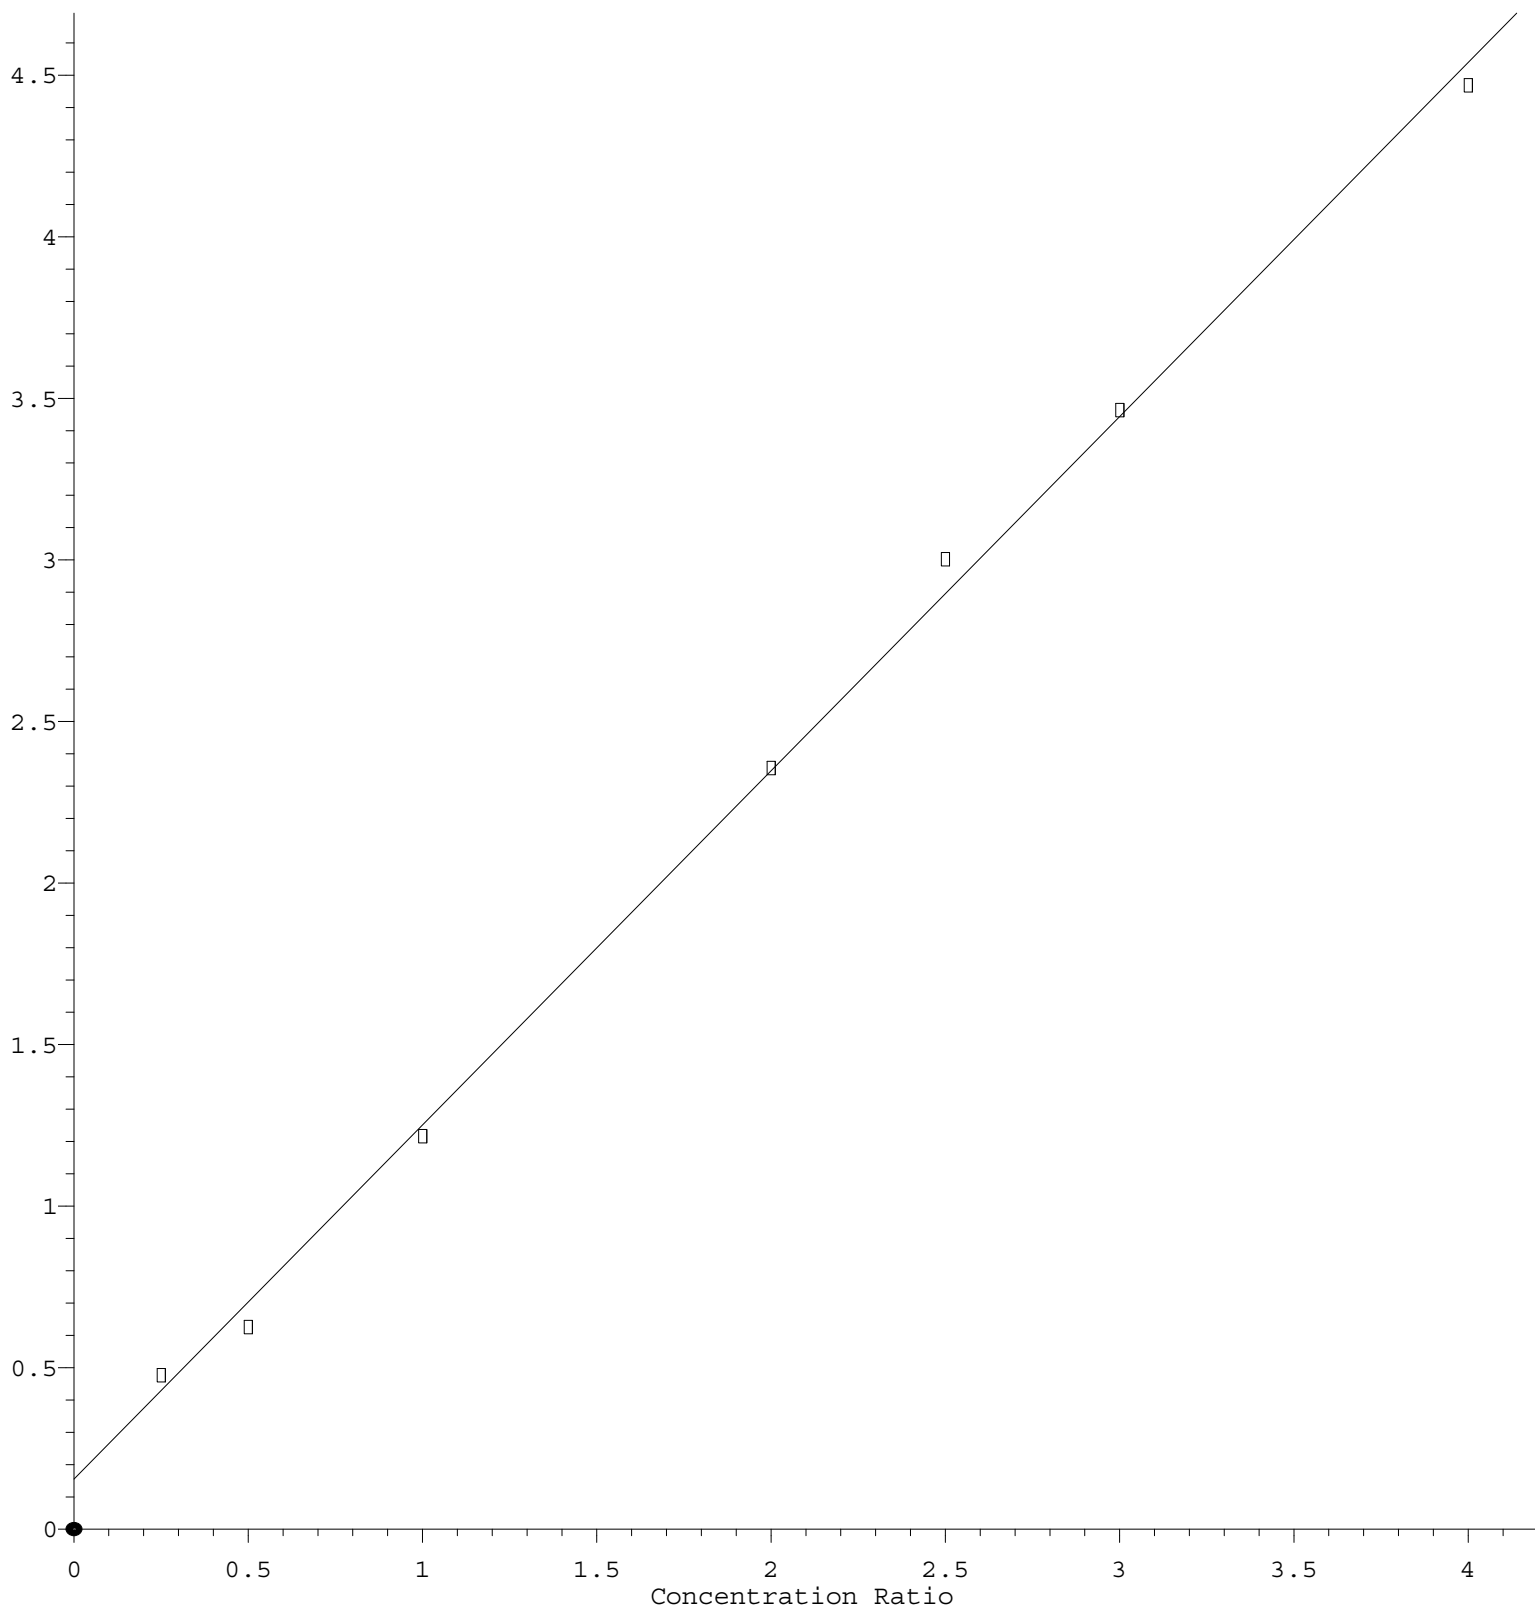

$$\text{Response} = 1.096\text{e}+000 * \text{Amt} + 1.549\text{e}-001$$

Coef of Det (r^2) = 0.998099 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP100821.M

Calibration Table Last Updated: Fri Oct 08 15:35:55 2021