
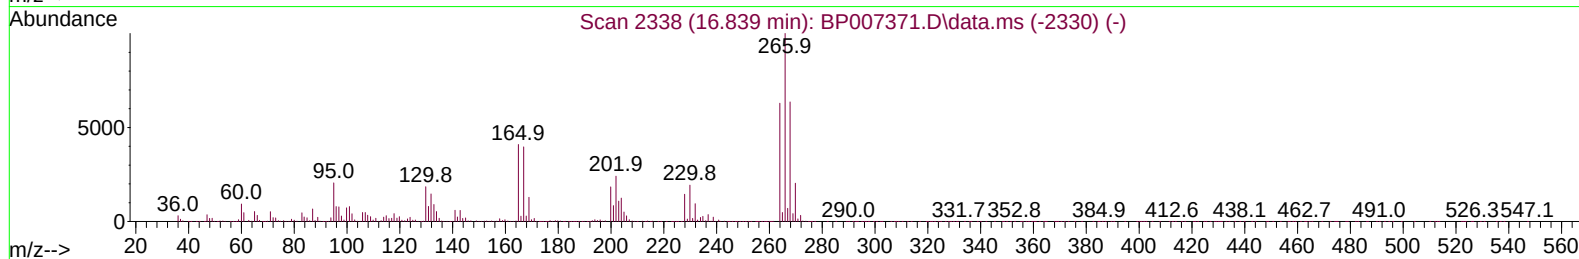
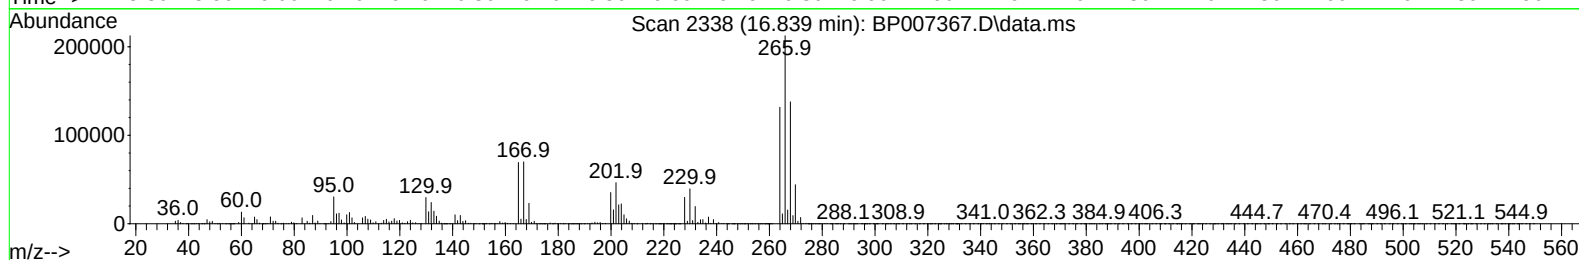


Quant Time: Oct 08 18:24:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 08 15:35:55 2021
Response via : Initial Calibration

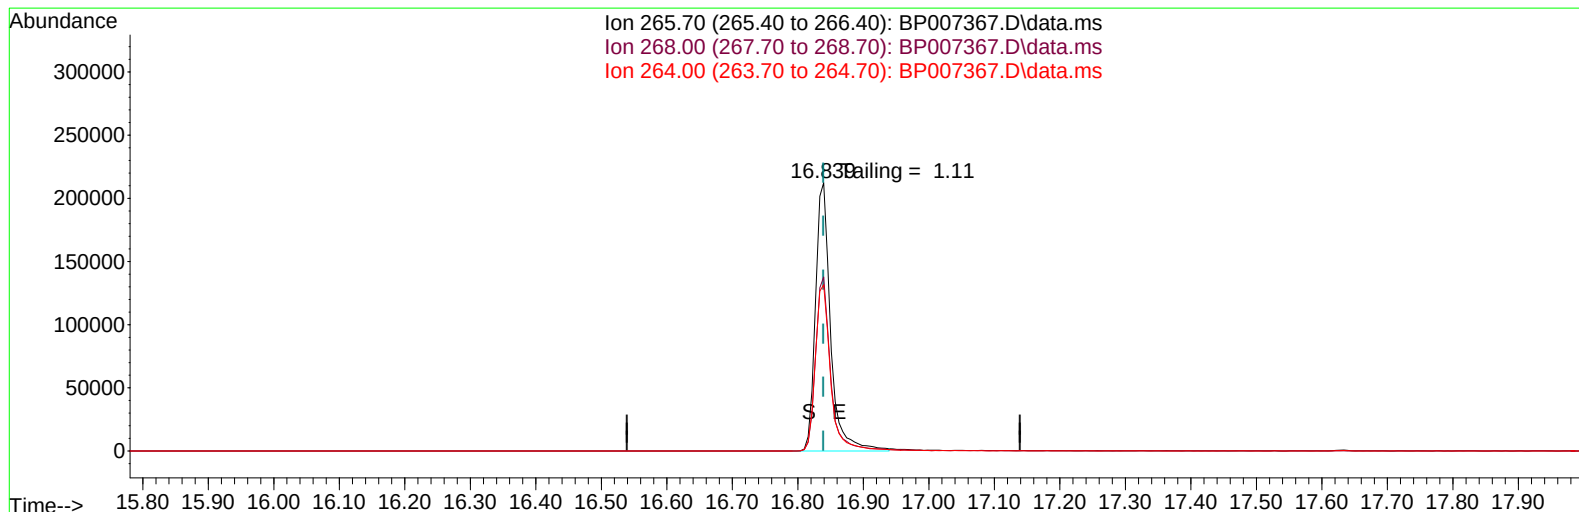

TIC: BP007367.D\data.ms

16.839min (+ 0.000) 847992.47 ng

response **343773**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	64.50	64.87
--------	-------	-------

264.00	62.90	61.95
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100821\
 Data File : BP007367.D
 Acq On : 08 Oct 2021 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 18:24:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 15:35:55 2021
 Response via : Initial Calibration

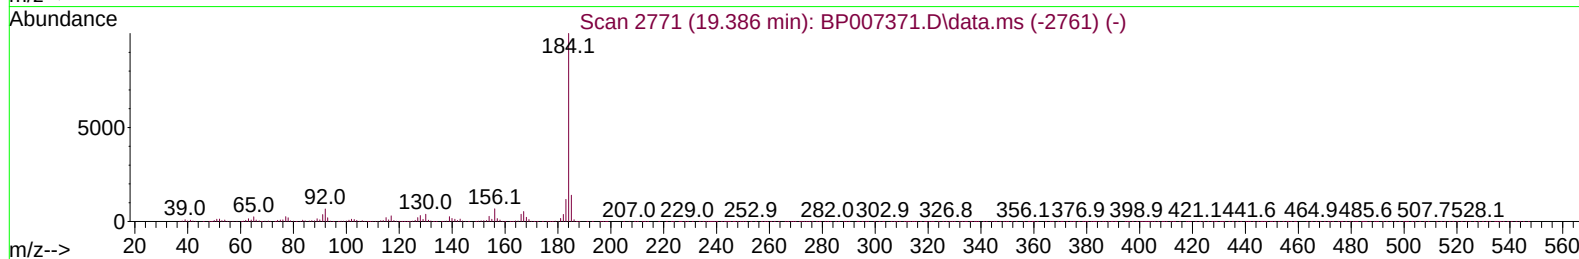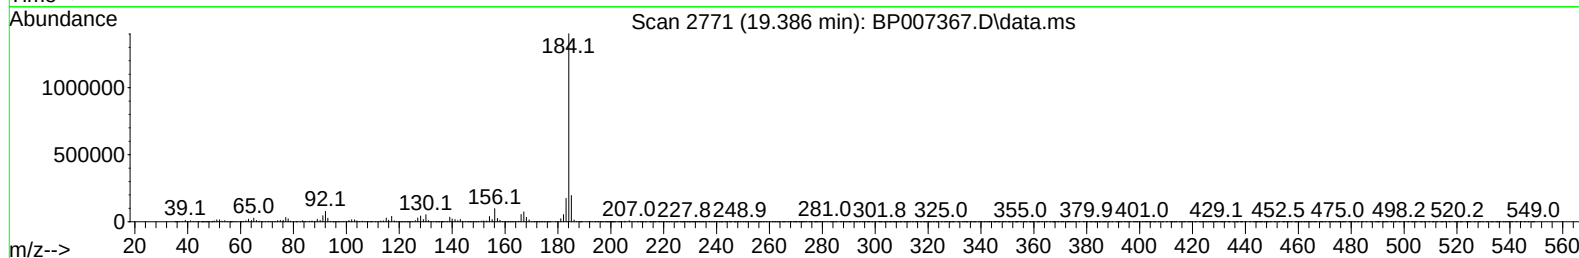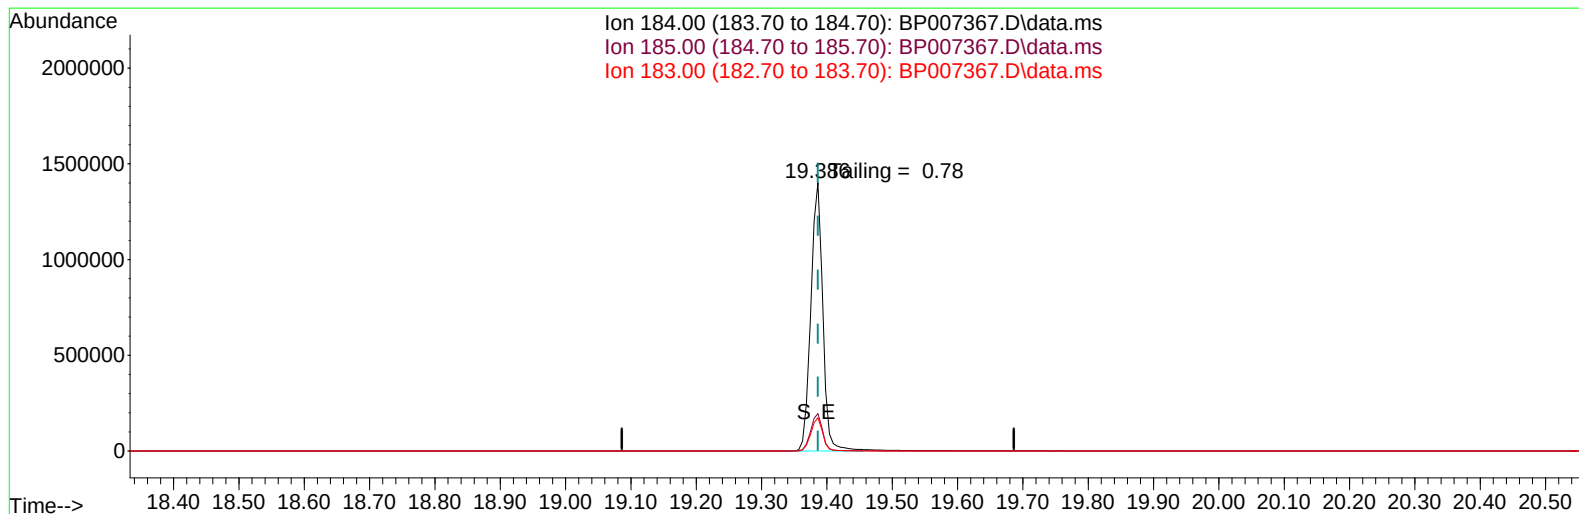

TIC: BP007367.D\data.ms

(77) Benzidine**19.386min (+ 0.000) 286525.59 ng****response 1804507**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.97
183.00	11.90	12.41
0.00	0.00	0.00