
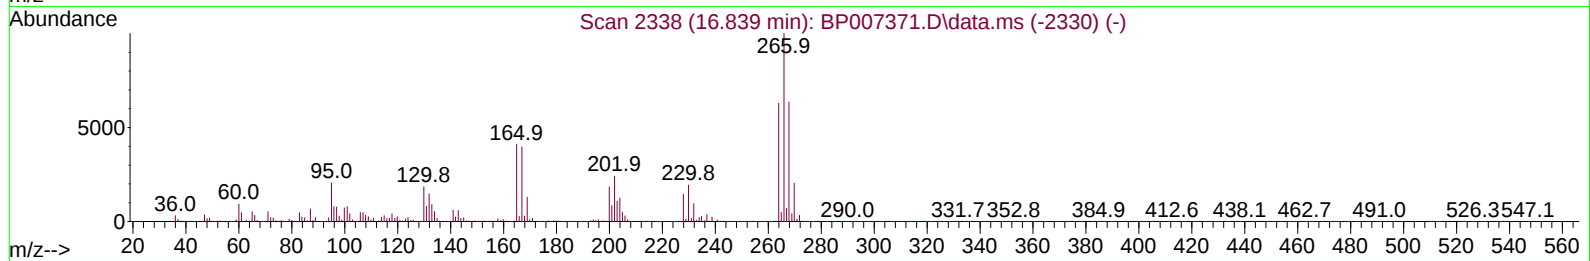
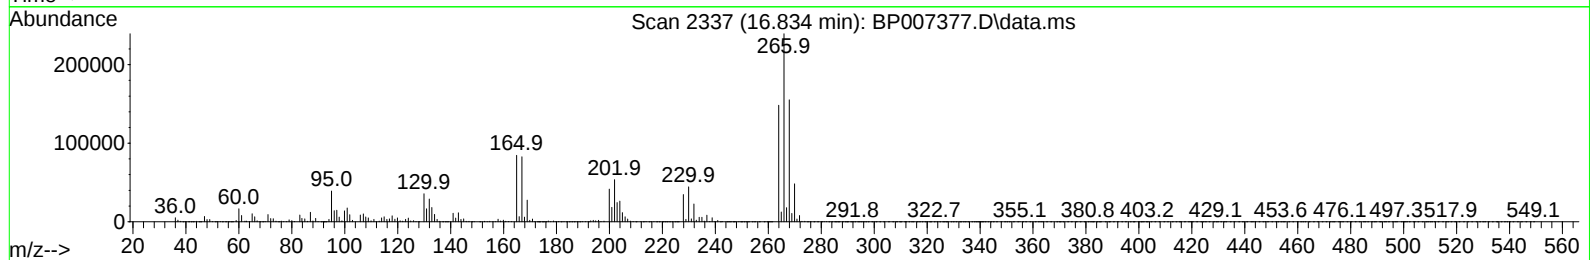


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100821\
 Data File : BP007377.D
 Acq On : 08 Oct 2021 16:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 18:24:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 15:35:55 2021
 Response via : Initial Calibration

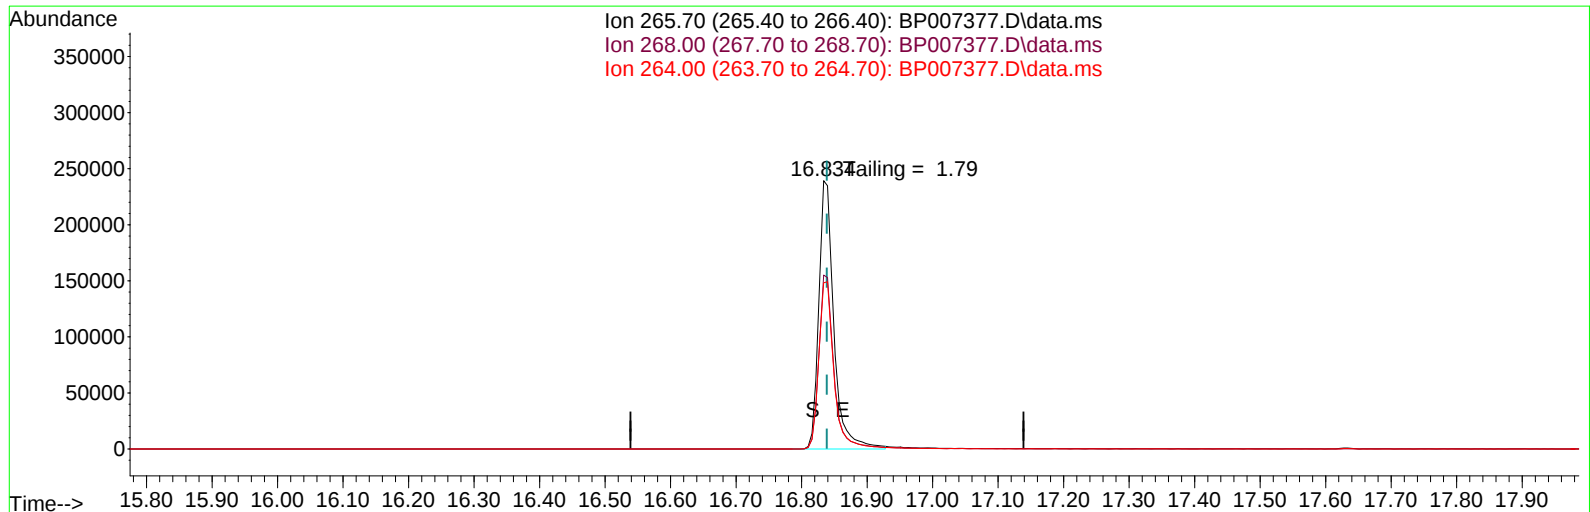

TIC: BP007377.D\data.ms

(70) Pentachlorophenol (C)




16.834min (-0.005) 776393.54 ng

response 387381

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.84
264.00	62.90	61.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100821\
 Data File : BP007377.D
 Acq On : 08 Oct 2021 16:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 18:24:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 15:35:55 2021
 Response via : Initial Calibration

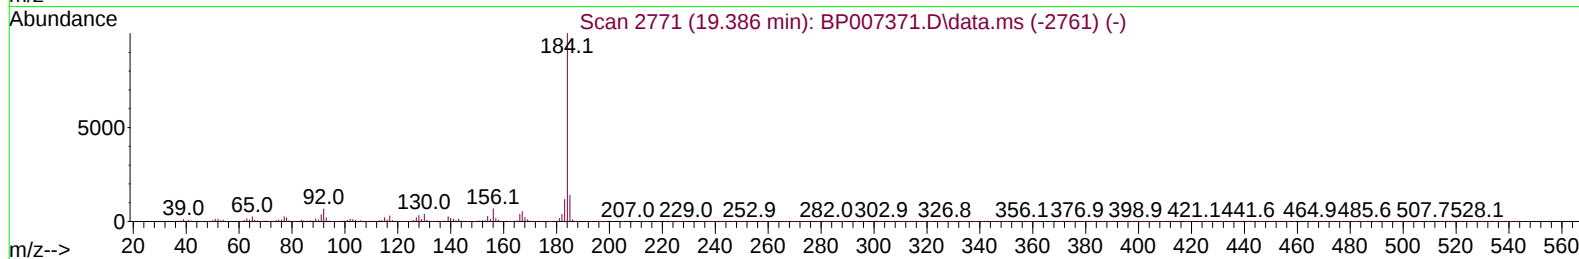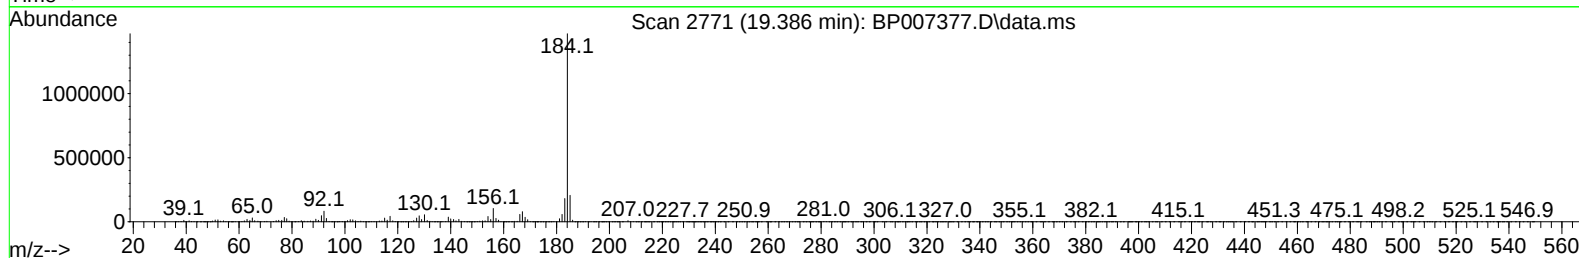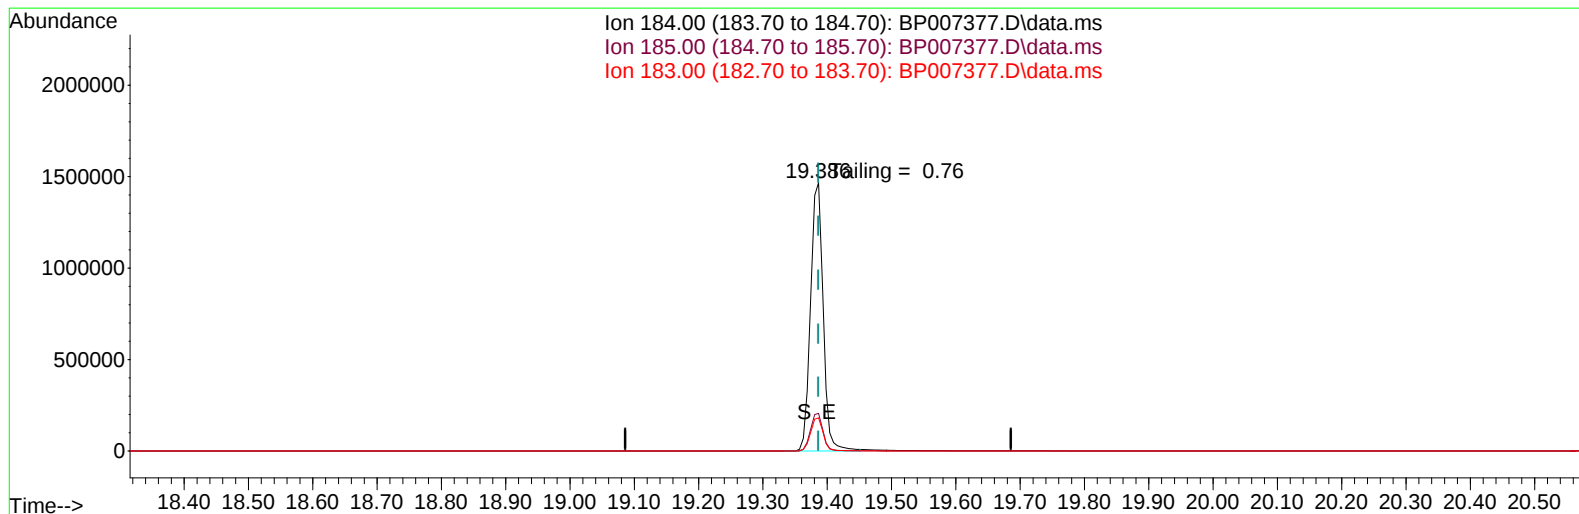

TIC: BP007377.D\data.ms

(77) Benzidine**19.386min (+ 0.000) 2508528.06 ng****response 2038508**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.01
183.00	11.90	12.38
0.00	0.00	0.00