

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100821\
 Data File : BP007379.D
 Acq On : 08 Oct 2021 18:08
 Operator : CG/JU
 Sample : PB139656BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139656BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007379.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.358	379	386	408	rBV	3205765	4717102	56.35%	12.208%
2	6.963	652	659	683	rBV	2439886	4106824	49.06%	10.629%
3	7.781	791	798	813	rBV	601589	972073	11.61%	2.516%
4	8.946	988	996	1021	rBV	1055548	1786488	21.34%	4.623%
5	10.575	1263	1273	1291	rBV	440791	806469	9.63%	2.087%
6	13.045	1685	1693	1709	rBV	3279378	5050454	60.33%	13.071%
7	14.422	1920	1927	1944	rBV	781813	1198675	14.32%	3.102%
8	15.922	2174	2182	2204	rBV	4240567	6290066	75.14%	16.279%
9	17.175	2389	2395	2411	rBV	967757	1509207	18.03%	3.906%
10	19.745	2826	2832	2840	rBV	6740156	8370812	100.00%	21.664%
11	21.268	3086	3091	3100	rBV	1356308	1750852	20.92%	4.531%
12	23.621	3485	3491	3503	rVB2	829965	1695196	20.25%	4.387%
13	28.939	4388	4395	4399	rBV3	131733	385193	4.60%	0.997%




Sum of corrected areas: 38639411

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100821\
Data File : BP007379.D
Acq On : 08 Oct 2021 18:08
Operator : CG/JU
Sample : PB139656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139656BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

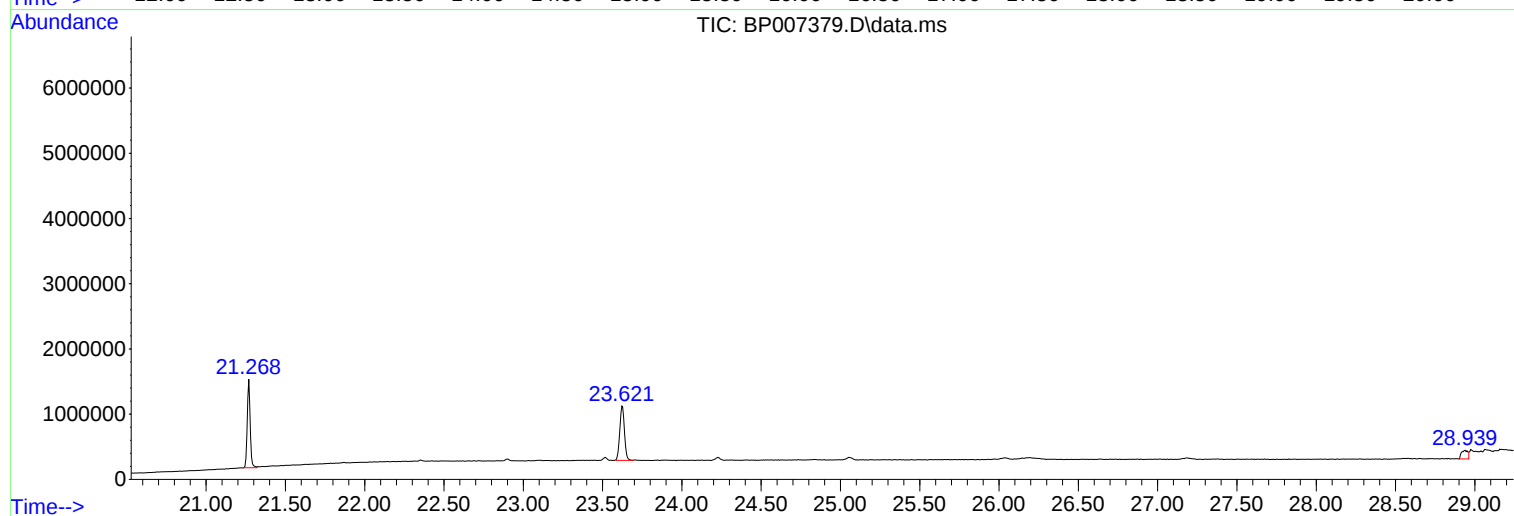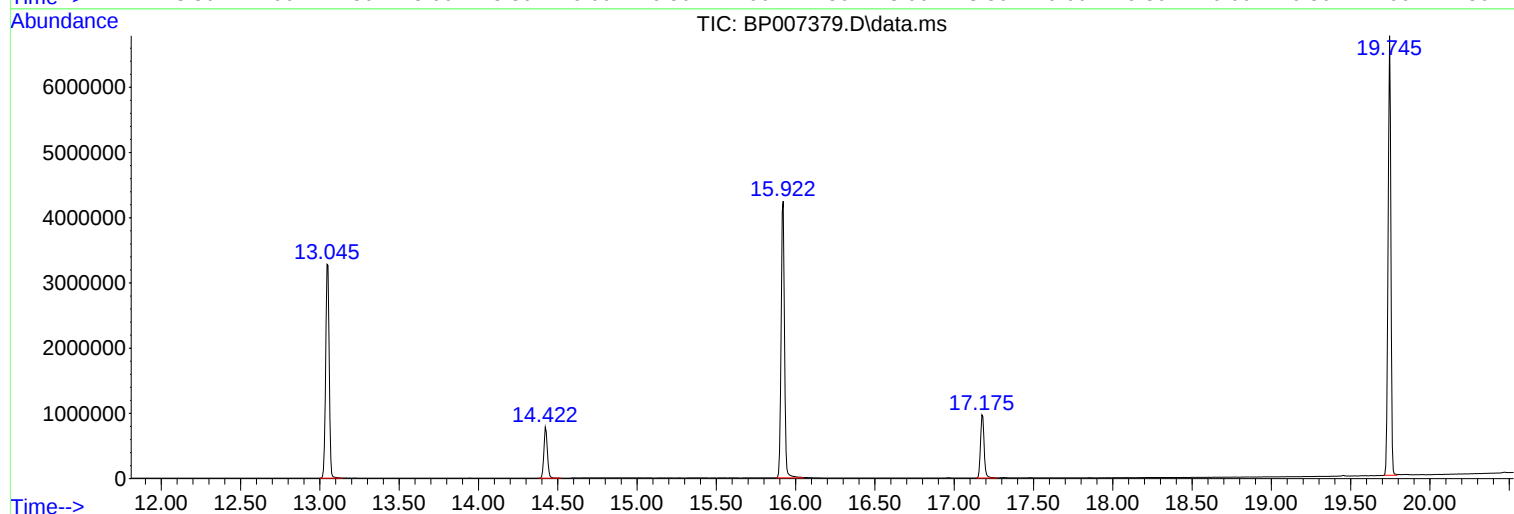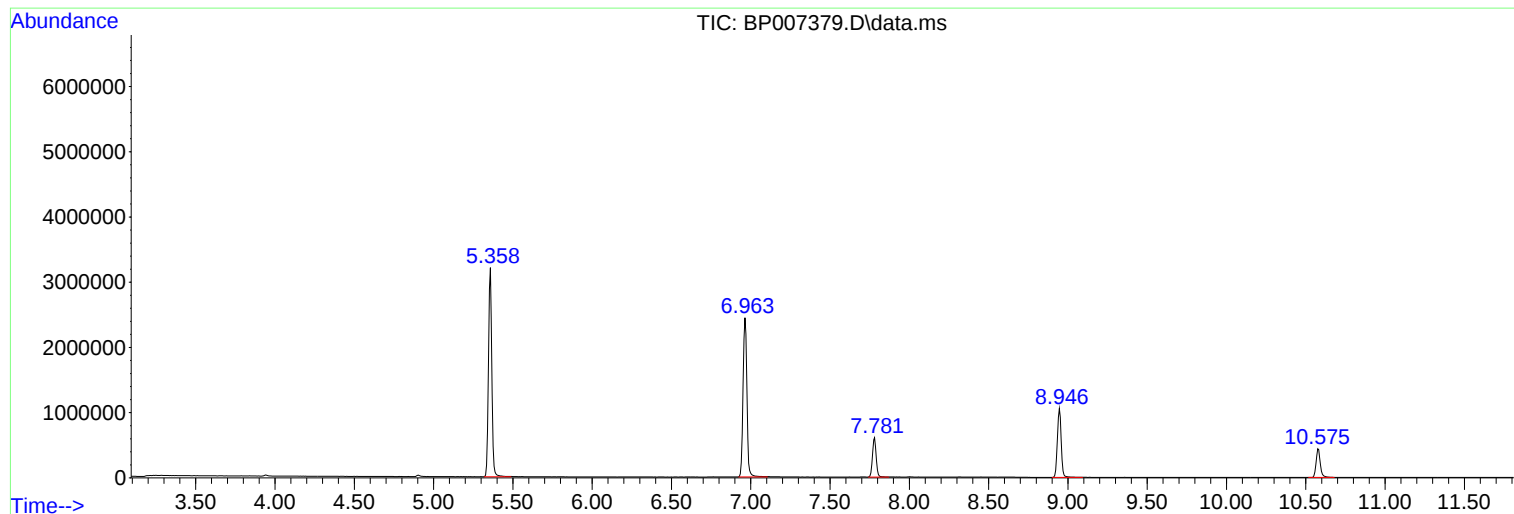

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100821\
Data File : BP007379.D
Acq On : 08 Oct 2021 18:08
Operator : CG/JU
Sample : PB139656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1






Instrument :
BNA_P
ClientSampleId :
PB139656BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclotrisiloxane, hexamethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
28.939	4.54 ng	385193	Perylene-d12			23.621
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Cyclotrisiloxane, hexamethyl-		222	C6H18O3Si3	000541-05-9	72
2	Methyltris(trimethylsiloxy)silane		310	C10H30O3Si4	017928-28-8	64
3	2,4,6-Cycloheptatrien-1-one, 3,5...		250	C13H22O5Si2	1000161-21-8	59
4	4-tert-Octylphenol, TMS derivative		278	C17H30O5Si	078721-87-6	53
5	Tris(tert-butyldimethylsilyloxy)...		468	C18H45AsO3Si3	1000366-57-5	50

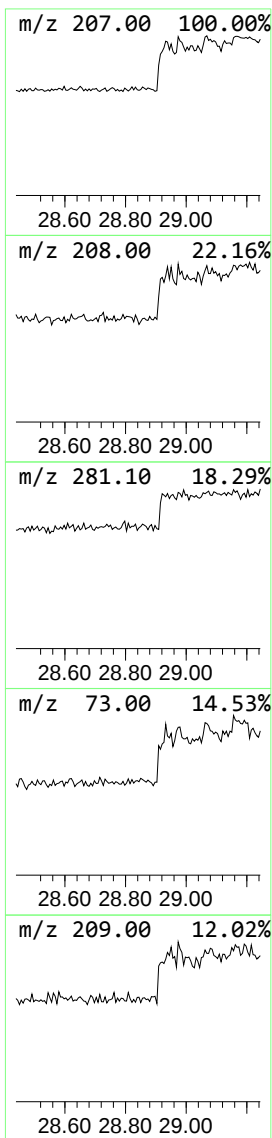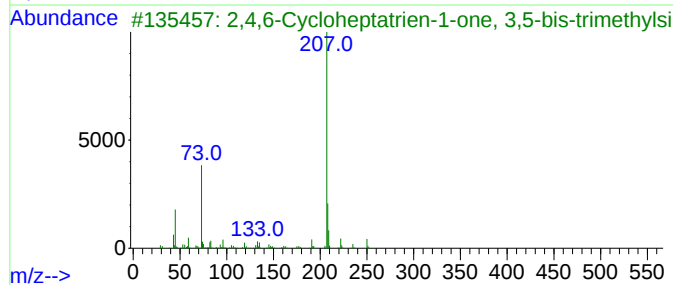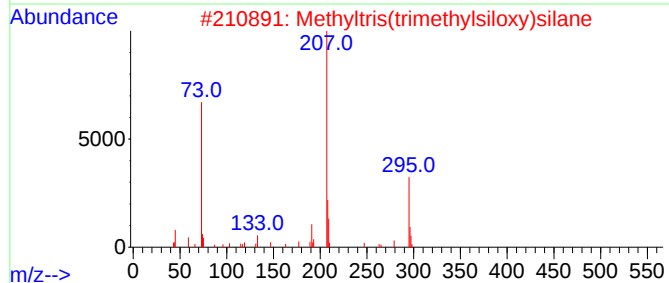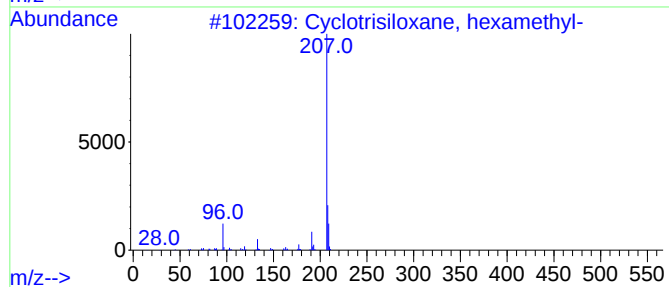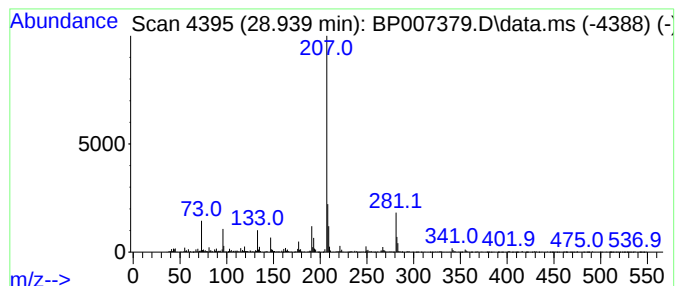

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100821\
Data File : BP007379.D
Acq On : 08 Oct 2021 18:08
Operator : CG/JU
Sample : PB139656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139656BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclotrisiloxan...	28.939	4.5	ng	385193	6	23.621	1695200	20.0