
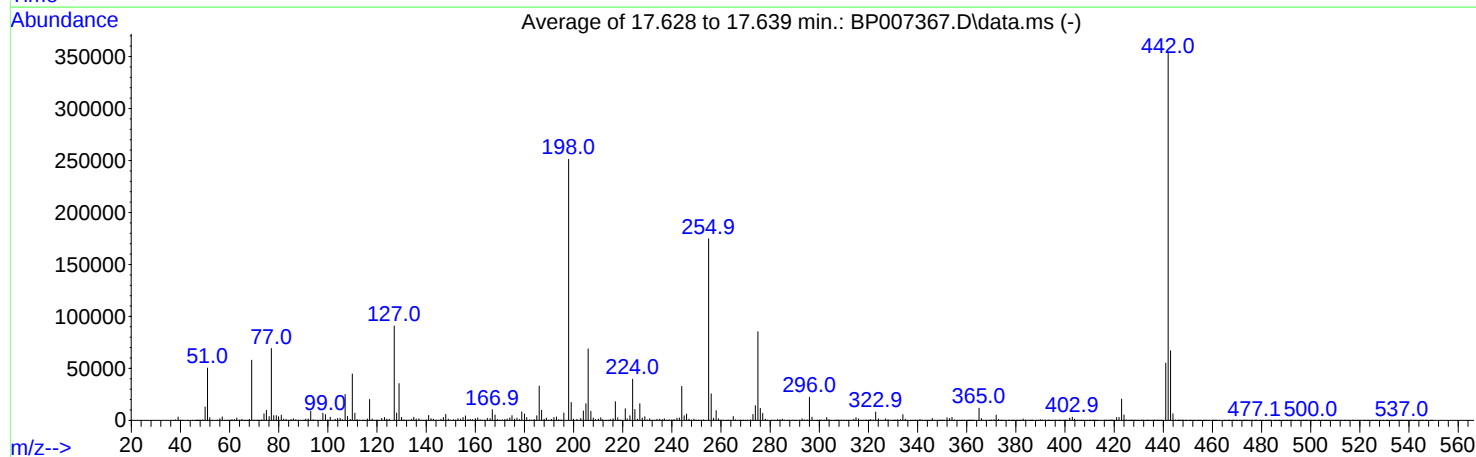


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100821\
 Data File : BP007367.D
 Acq On : 08 Oct 2021 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 08 15:35:55 2021

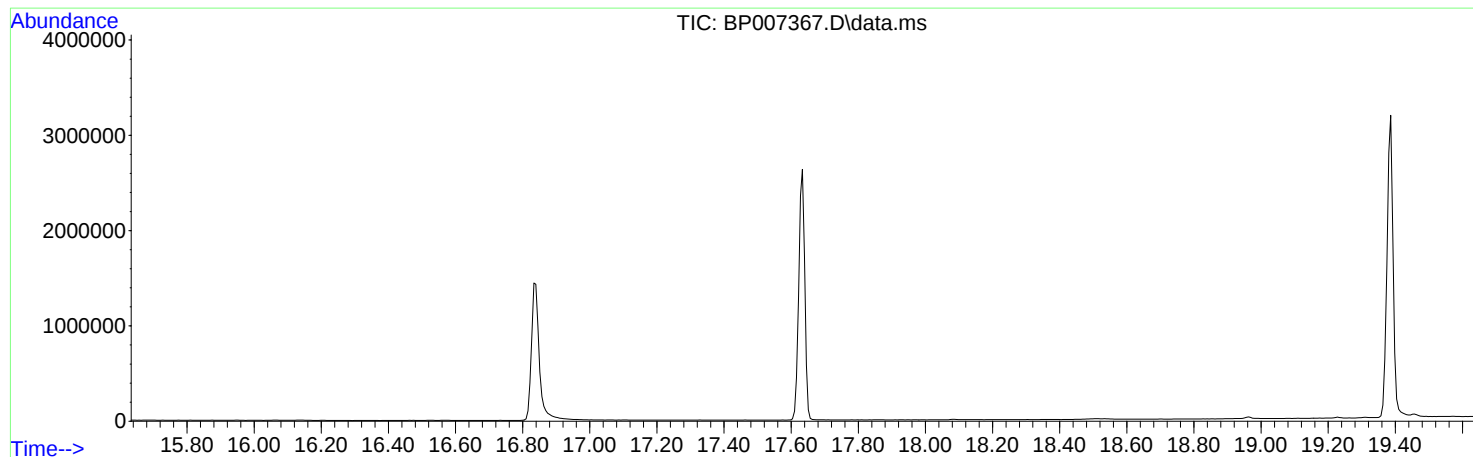




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.1	50385	PASS
68	69	0.00	2	2.0	1145	PASS
69	198	0.00	100	23.0	57845	PASS
70	69	0.00	2	0.6	324	PASS
127	198	10	80	36.2	90832	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	251236	PASS
199	198	5	9	6.9	17300	PASS
275	198	10	60	34.0	85296	PASS
365	198	1	100	4.7	11723	PASS
441	198	0.01	100	21.9	55096	PASS
442	442	100	100	100.0	353920	PASS
443	442	15	24	18.9	67046	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100821\
 Data File : BP007367.D
 Acq On : 08 Oct 2021 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Oct 08 18:24:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP100821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 08 15:35:55 2021
 Response via : Initial Calibration

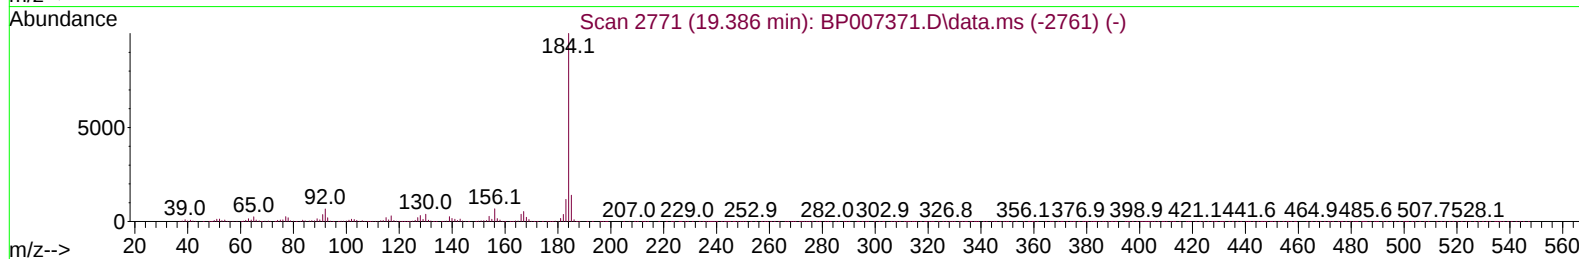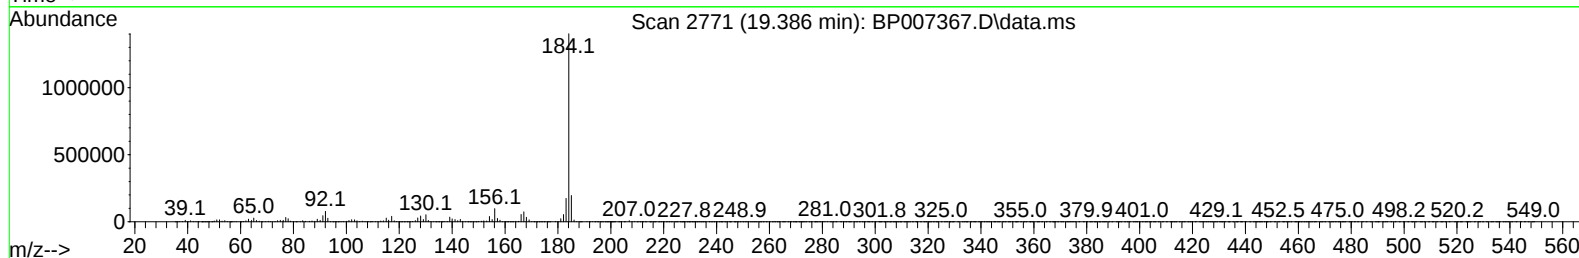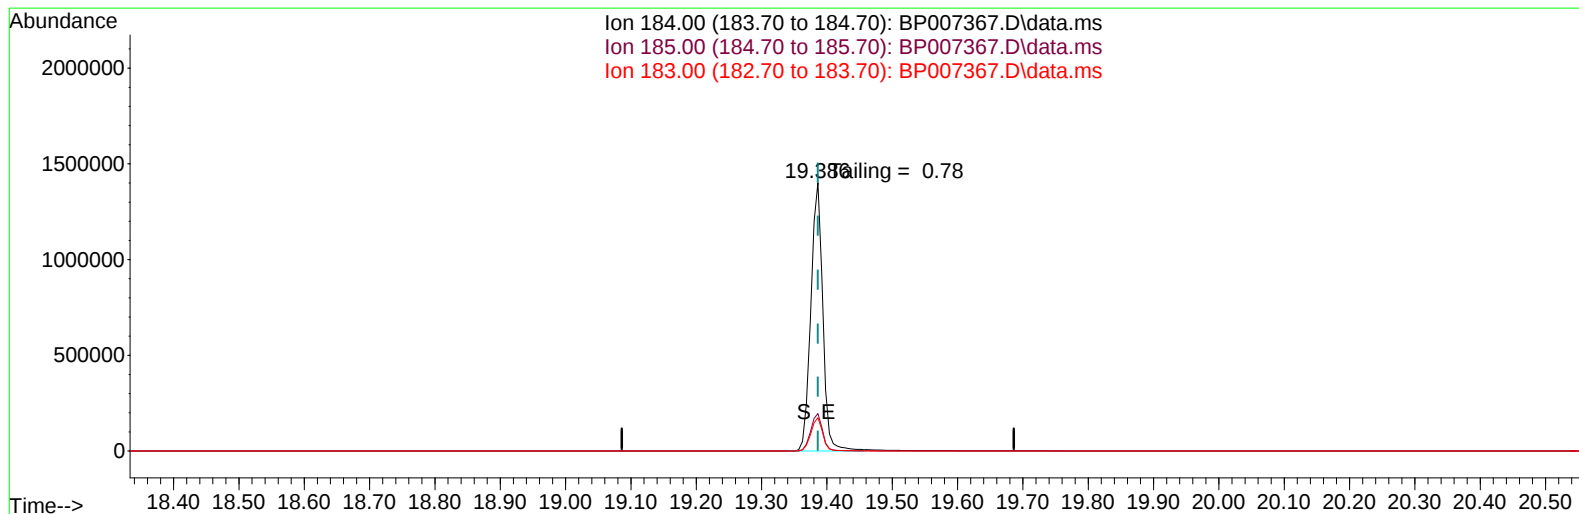

TIC: BP007367.D\data.ms

(77) Benzidine

19.386min (+ 0.000) 286525.59 ng

response 1804507

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.97
183.00	11.90	12.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/8/2021	BNA_P	BP007367.D
Compound Name	Response	Retention Time
DDT	1024250	20.58
DDD	6678	20.15
DDE	935	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7613	1031863	0.74

Instrument :
BNA_P
ClientSampleId :
DFTPP