
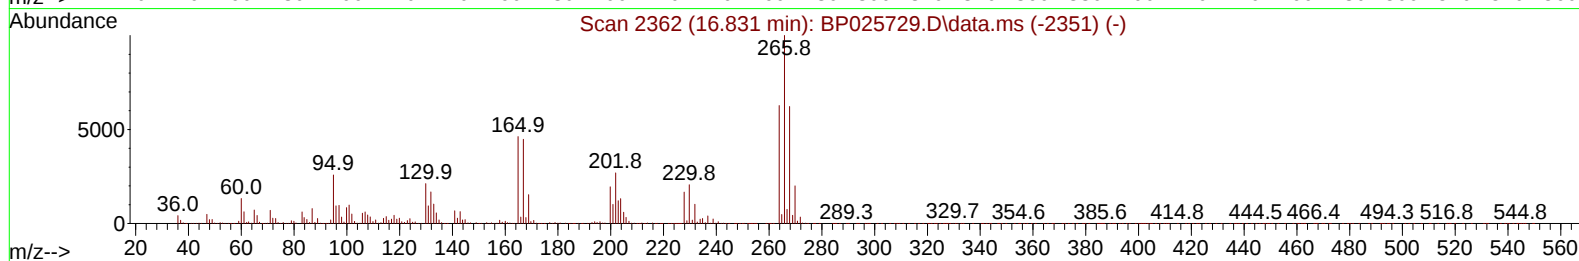
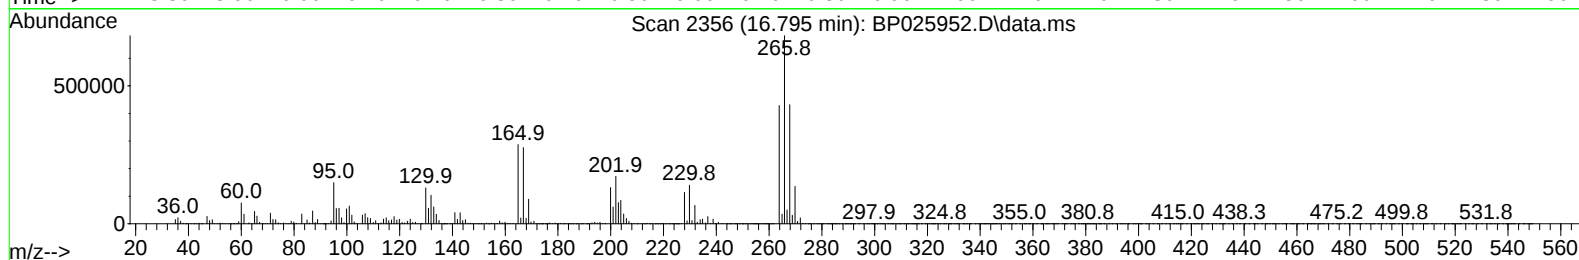


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100825\
Data File : BP025952.D
Acq On : 08 Oct 2025 14:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 15:52:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 19:16:54 2025
Response via : Initial Calibration

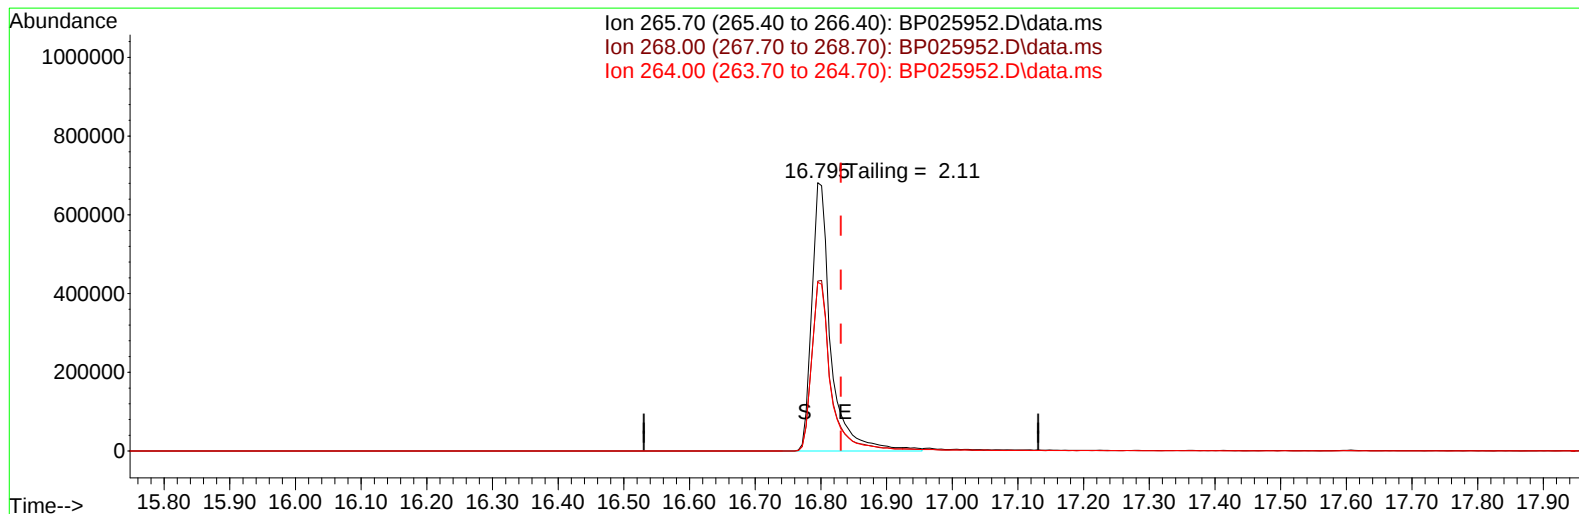

TIC: BP025952.D\data.ms

(70) Pentachlorophenol (C)




16.795min (-0.035) 248115.37 ng

response 1372230

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.33
264.00	62.70	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100825\
Data File : BP025952.D
Acq On : 08 Oct 2025 14:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 15:52:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 19:16:54 2025
Response via : Initial Calibration

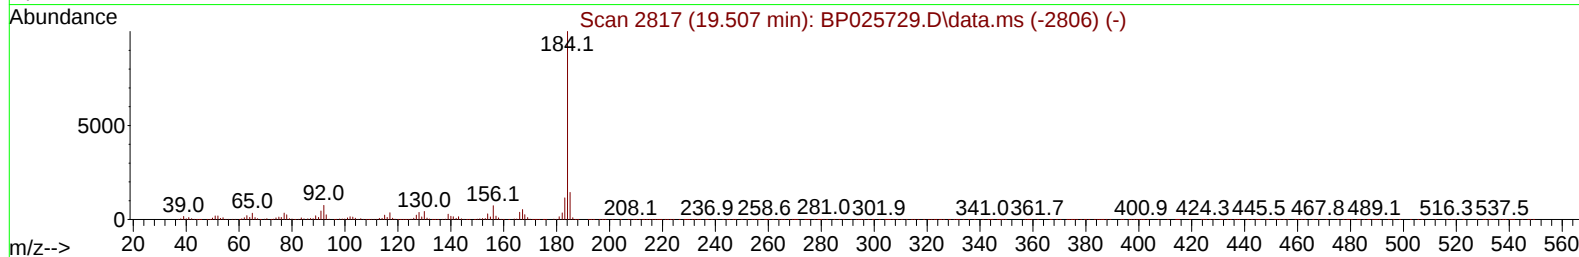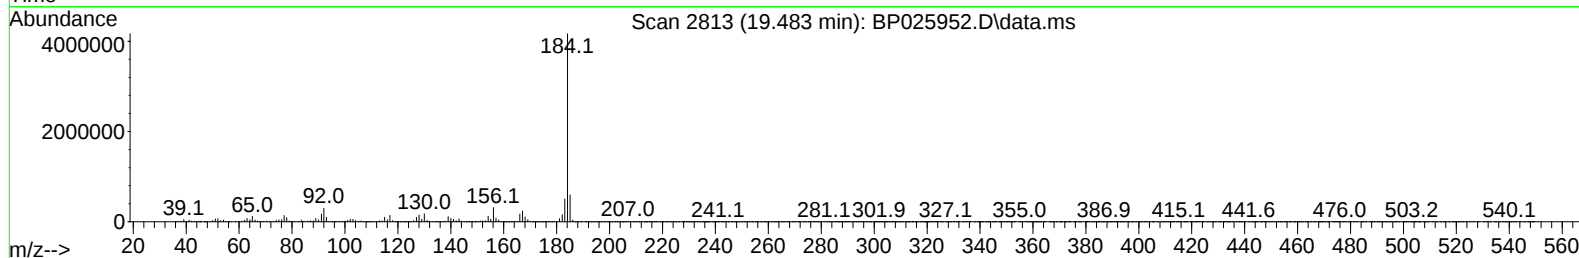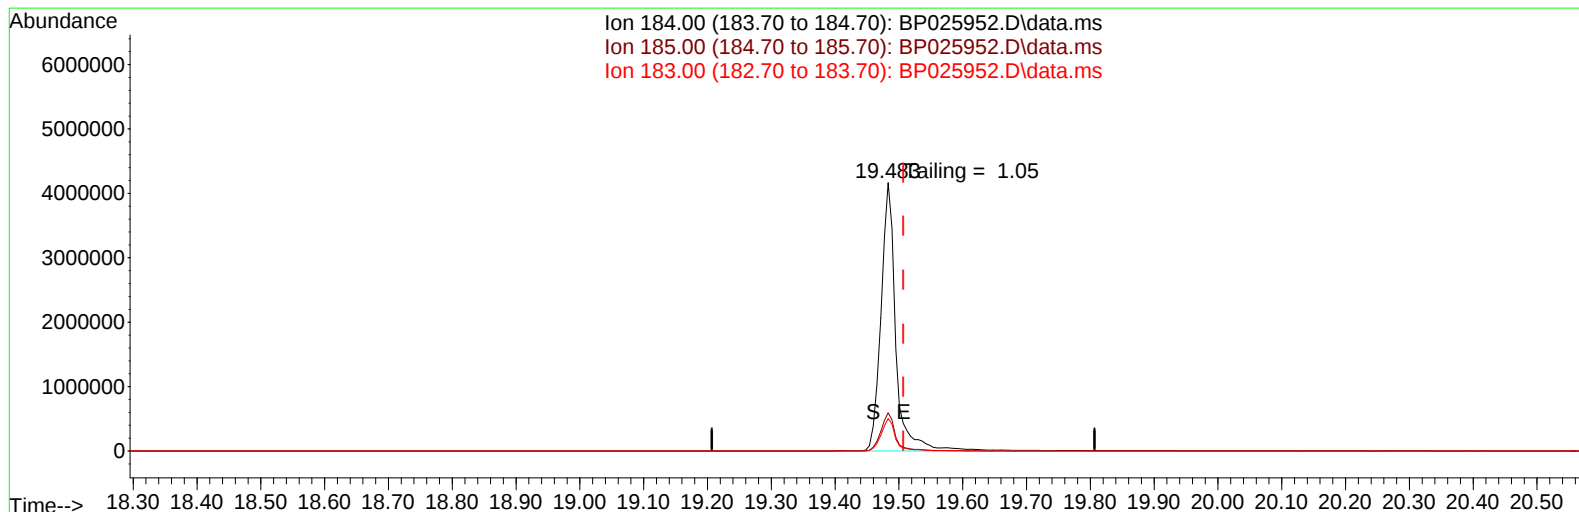

TIC: BP025952.D\data.ms

(77) Benzidine**19.483min (-0.024) 103203.29 ng****response 6590713**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.28
183.00	11.50	12.10
0.00	0.00	0.00