

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022286.D
 Acq On : 09 Oct 2024 12:15
 Operator : RC/JU
 Sample : P4162-21
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4EJ6

Quant Time: Oct 09 12:44:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.704	152	140886	20.000	ng/u1	0.00
20) Naphthalene-d8	10.469	136	537827	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.322	164	420414	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.110	188	1014412	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1014277	20.000	ng/u1	0.00
88) Perylene-d12	24.845	264	1215046	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	8956	2.470	ng/uL	0.00
4) Pyridine-d5	3.640	84	118286	11.885	ng/u1	0.00
7) Phenol-d5	6.893	99	174125	14.682	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.045	67	106555	15.287	ng/u1	0.00
11) 2-Chlorophenol-d4	7.245	132	134235	15.952	ng/u1	0.00
15) 4-Methylphenol-d8	8.404	113	149042	15.748	ng/u1	0.00
21) Nitrobenzene-d5	8.845	128	67010	16.204	ng/u1	0.00
24) 2-Nitrophenol-d4	9.557	143	81766	17.078	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.098	165	169537	16.661	ng/u1	0.00
31) 4-Chloroaniline-d4	10.598	131	187001	15.553	ng/u1	0.00
46) Dimethylphthalate-d6	13.716	166	638190	19.106	ng/u1	0.00
49) Acenaphthylene-d8	14.004	160	669906	18.882	ng/u1	0.00
54) 4-Nitrophenol-d4	14.545	143	76228	13.603	ng/u1	0.02
60) Fluorene-d10	15.327	176	576929	19.913	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.445	200	88917	13.328	ng/u1	0.00
73) Anthracene-d10	17.216	188	953621	19.984	ng/u1	0.00
81) Pyrene-d10	19.598	212	1166830	21.754	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.615	264	1339255	20.639	ng/u1	0.02
Target Compounds						
					Qvalue	
82) Pyrene	19.621	202	68493	1.036	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022286.D
Acq On : 09 Oct 2024 12:15
Operator : RC/JU
Sample : P4162-21
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4EJ6

Quant Time: Oct 09 12:44:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 08 02:14:47 2024
Response via : Initial Calibration

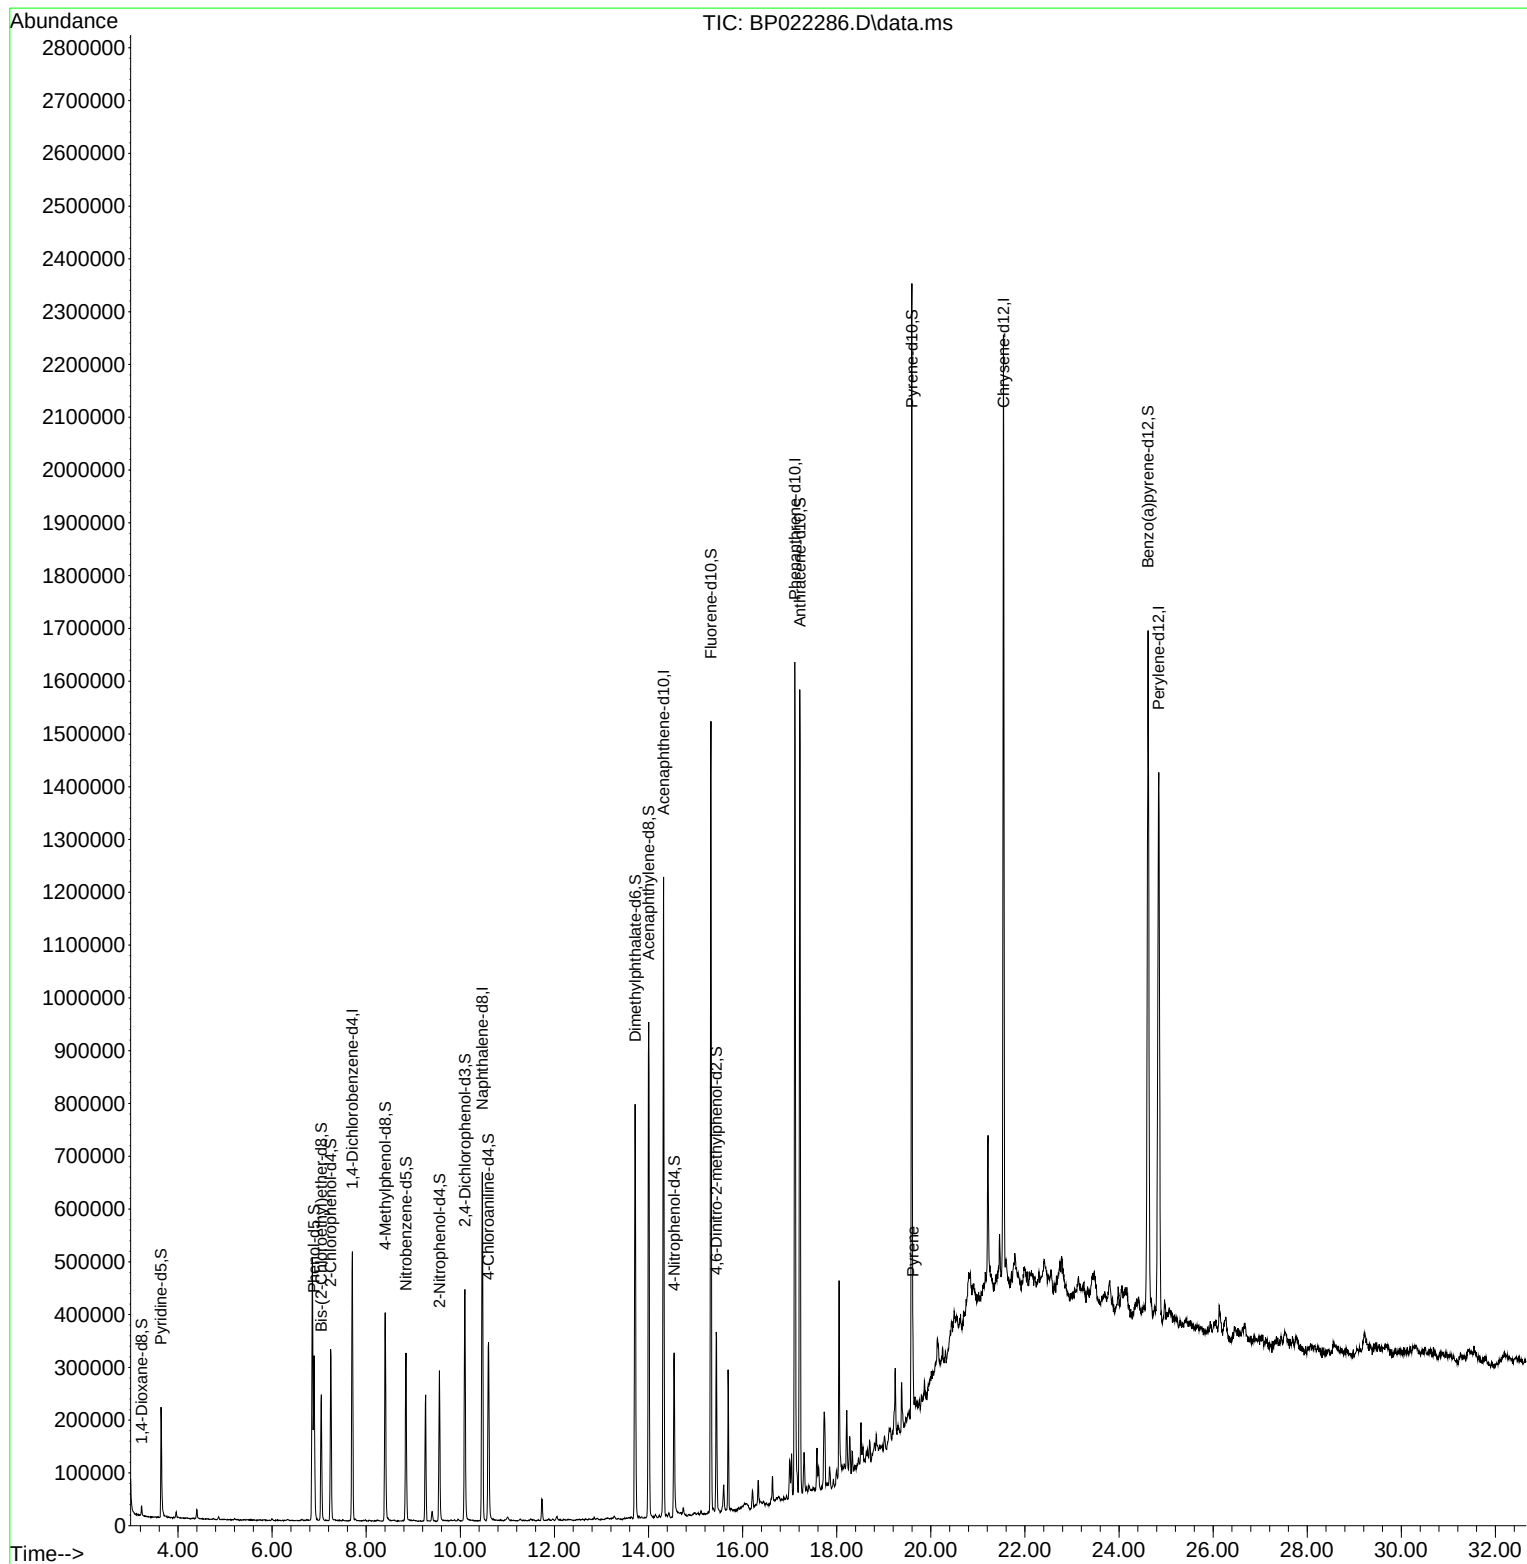

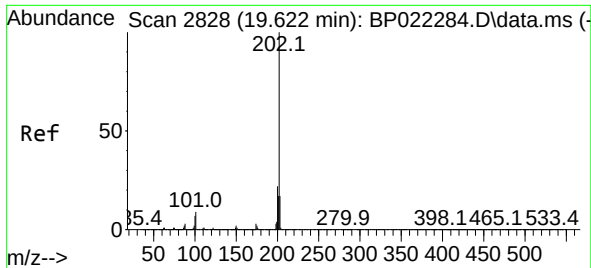

#82
 Pyrene
 Concen: 1.036 ng/ul
 RT: 19.621 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP022286.D
 Acq: 09 Oct 2024 12:15

Instrument :
 BNA_P
 ClientSampleId :
 A4EJ6

Tgt Ion:202 Resp: 68493
 Ion Ratio Lower Upper
 202 100
 101 7.4 6.7 10.1
 100 7.3 5.8 8.6

