

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022306.D
 Acq On : 10 Oct 2024 02:35
 Operator : RC/JU
 Sample : P4207-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY051

Quant Time: Oct 10 03:06:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	140803	20.000	ng/u1	0.00
20) Naphthalene-d8	10.463	136	521911	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.310	164	399900	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.116	188	964162	20.000	ng/u1	0.00
79) Chrysene-d12	21.551	240	1049066	20.000	ng/u1	0.01
88) Perylene-d12	24.839	264	1212608	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	12392	3.420	ng/uL	0.00
4) Pyridine-d5	3.646	84	34852	3.504	ng/u1	0.01
7) Phenol-d5	6.899	99	92365	7.793	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.046	67	159947	22.961	ng/u1	0.00
11) 2-Chlorophenol-d4	7.252	132	197107	23.437	ng/u1	0.00
15) 4-Methylphenol-d8	8.404	113	162727	17.204	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	102330	25.500	ng/u1	0.00
24) 2-Nitrophenol-d4	9.557	143	125120	26.931	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	250074	25.325	ng/u1	0.00
31) 4-Chloroaniline-d4	10.599	131	173076	14.833	ng/u1	0.00
46) Dimethylphthalate-d6	13.722	166	819408	25.789	ng/u1	0.00
49) Acenaphthylene-d8	14.004	160	837632	24.821	ng/u1	0.00
54) 4-Nitrophenol-d4	14.539	143	36922	6.927	ng/u1	0.01
60) Fluorene-d10	15.316	176	692948	25.144	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	130656	20.604	ng/u1	0.01
73) Anthracene-d10	17.222	188	1270184	28.004	ng/u1	0.00
81) Pyrene-d10	19.598	212	1674813	30.190	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.621	264	1852681	28.609	ng/u1	0.02


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.264	88	12734	3.269	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022306.D
Acq On : 10 Oct 2024 02:35
Operator : RC/JU
Sample : P4207-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY051


Quant Time: Oct 10 03:06:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 08 02:14:47 2024
Response via : Initial Calibration

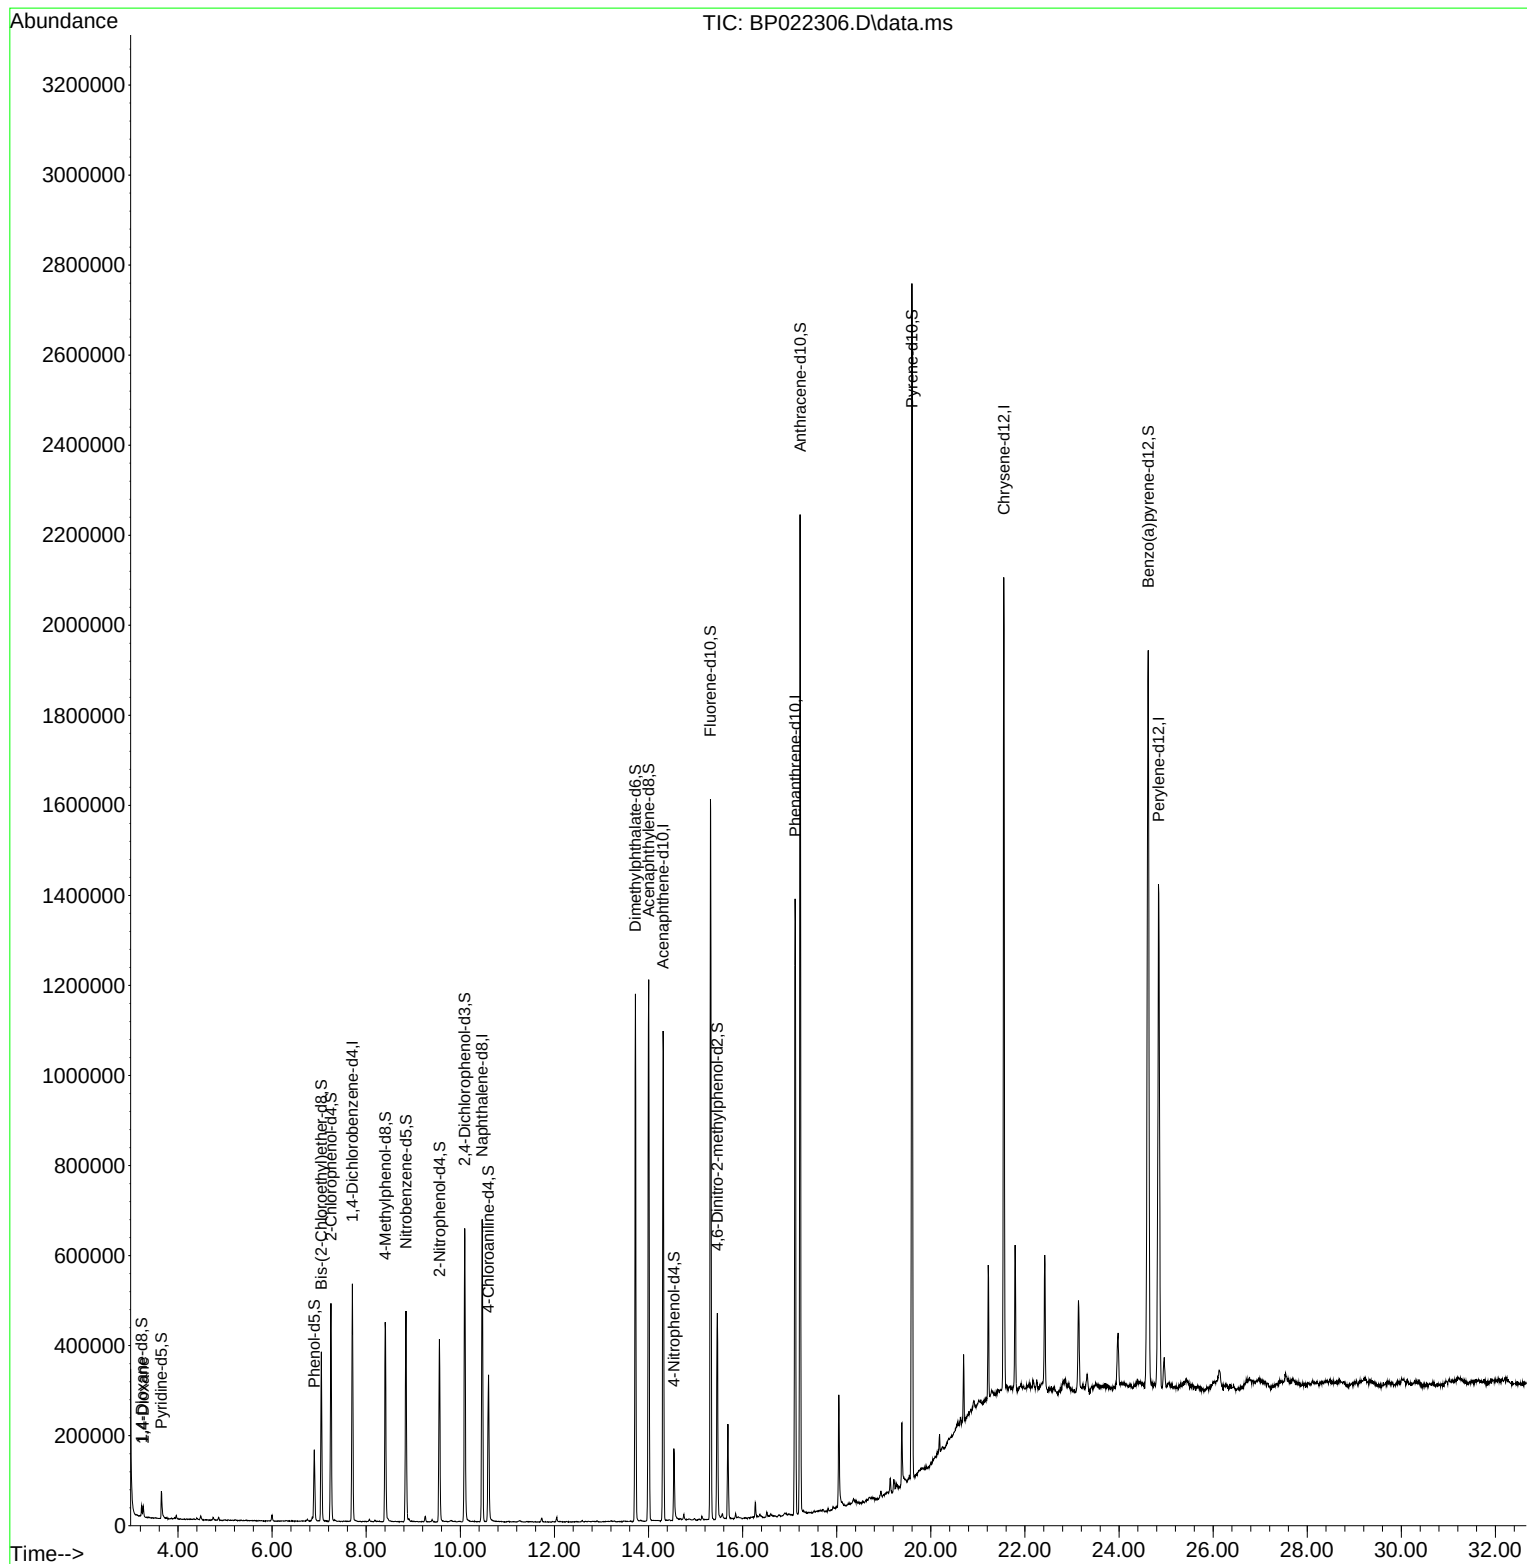

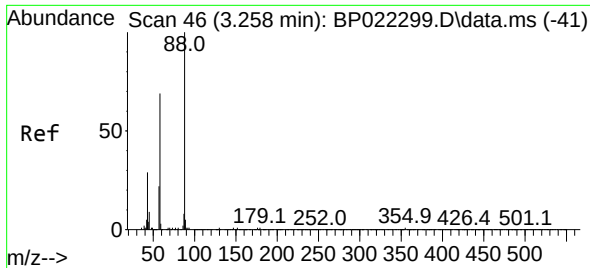

#2
 1,4-Dioxane
 Concen: 3.269 ng/uL
 RT: 3.264 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: BP022306.D
 Acq: 10 Oct 2024 02:35

Instrument :
 BNA_P
 ClientSampleId :
 EY051

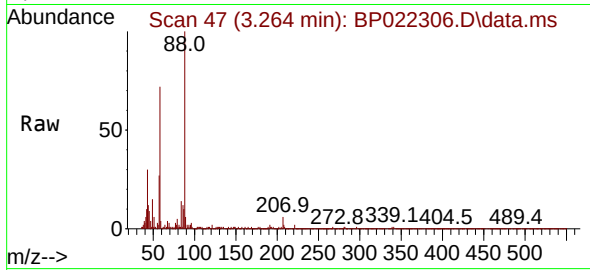

Tgt Ion: 88 Resp: 12734

Ion	Ratio	Lower	Upper
88	100		
43	30.0	22.3	33.5
58	72.2	54.7	82.1

