

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022308.D
 Acq On : 10 Oct 2024 03:57
 Operator : RC/JU
 Sample : P4207-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY052

Quant Time: Oct 10 04:34:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	118133	20.000	ng/u1	0.00
20) Naphthalene-d8	10.463	136	465486	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.316	164	374263	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.116	188	948209	20.000	ng/u1	0.00
79) Chrysene-d12	21.551	240	949902	20.000	ng/u1	0.01
88) Perylene-d12	24.857	264	1107076	20.000	ng/u1	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	9402	3.093	ng/uL	0.00
4) Pyridine-d5	3.646	84	42590	5.103	ng/u1	0.01
7) Phenol-d5	6.899	99	58697	5.903	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.046	67	122664	20.988	ng/u1	0.00
11) 2-Chlorophenol-d4	7.252	132	144071	20.418	ng/u1	0.00
15) 4-Methylphenol-d8	8.410	113	114000	14.365	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	79614	22.244	ng/u1	0.00
24) 2-Nitrophenol-d4	9.557	143	98657	23.809	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	198897	22.584	ng/u1	0.00
31) 4-Chloroaniline-d4	10.604	131	187070	17.976	ng/u1	0.01
46) Dimethylphthalate-d6	13.716	166	759741	25.550	ng/u1	0.00
49) Acenaphthylene-d8	14.004	160	737273	23.344	ng/u1	0.00
54) 4-Nitrophenol-d4	14.540	143	31846	6.384	ng/u1	0.01
60) Fluorene-d10	15.328	176	656901	25.469	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.451	200	135716	21.763	ng/u1	0.00
73) Anthracene-d10	17.210	188	1282239	28.746	ng/u1	0.00
81) Pyrene-d10	19.598	212	1643652	32.721	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.633	264	1769099	29.922	ng/u1	0.04
Target Compounds						
2) 1,4-Dioxane	3.258	88	6415	1.963	ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022308.D
Acq On : 10 Oct 2024 03:57
Operator : RC/JU
Sample : P4207-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY052


Quant Time: Oct 10 04:34:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 08 02:14:47 2024
Response via : Initial Calibration

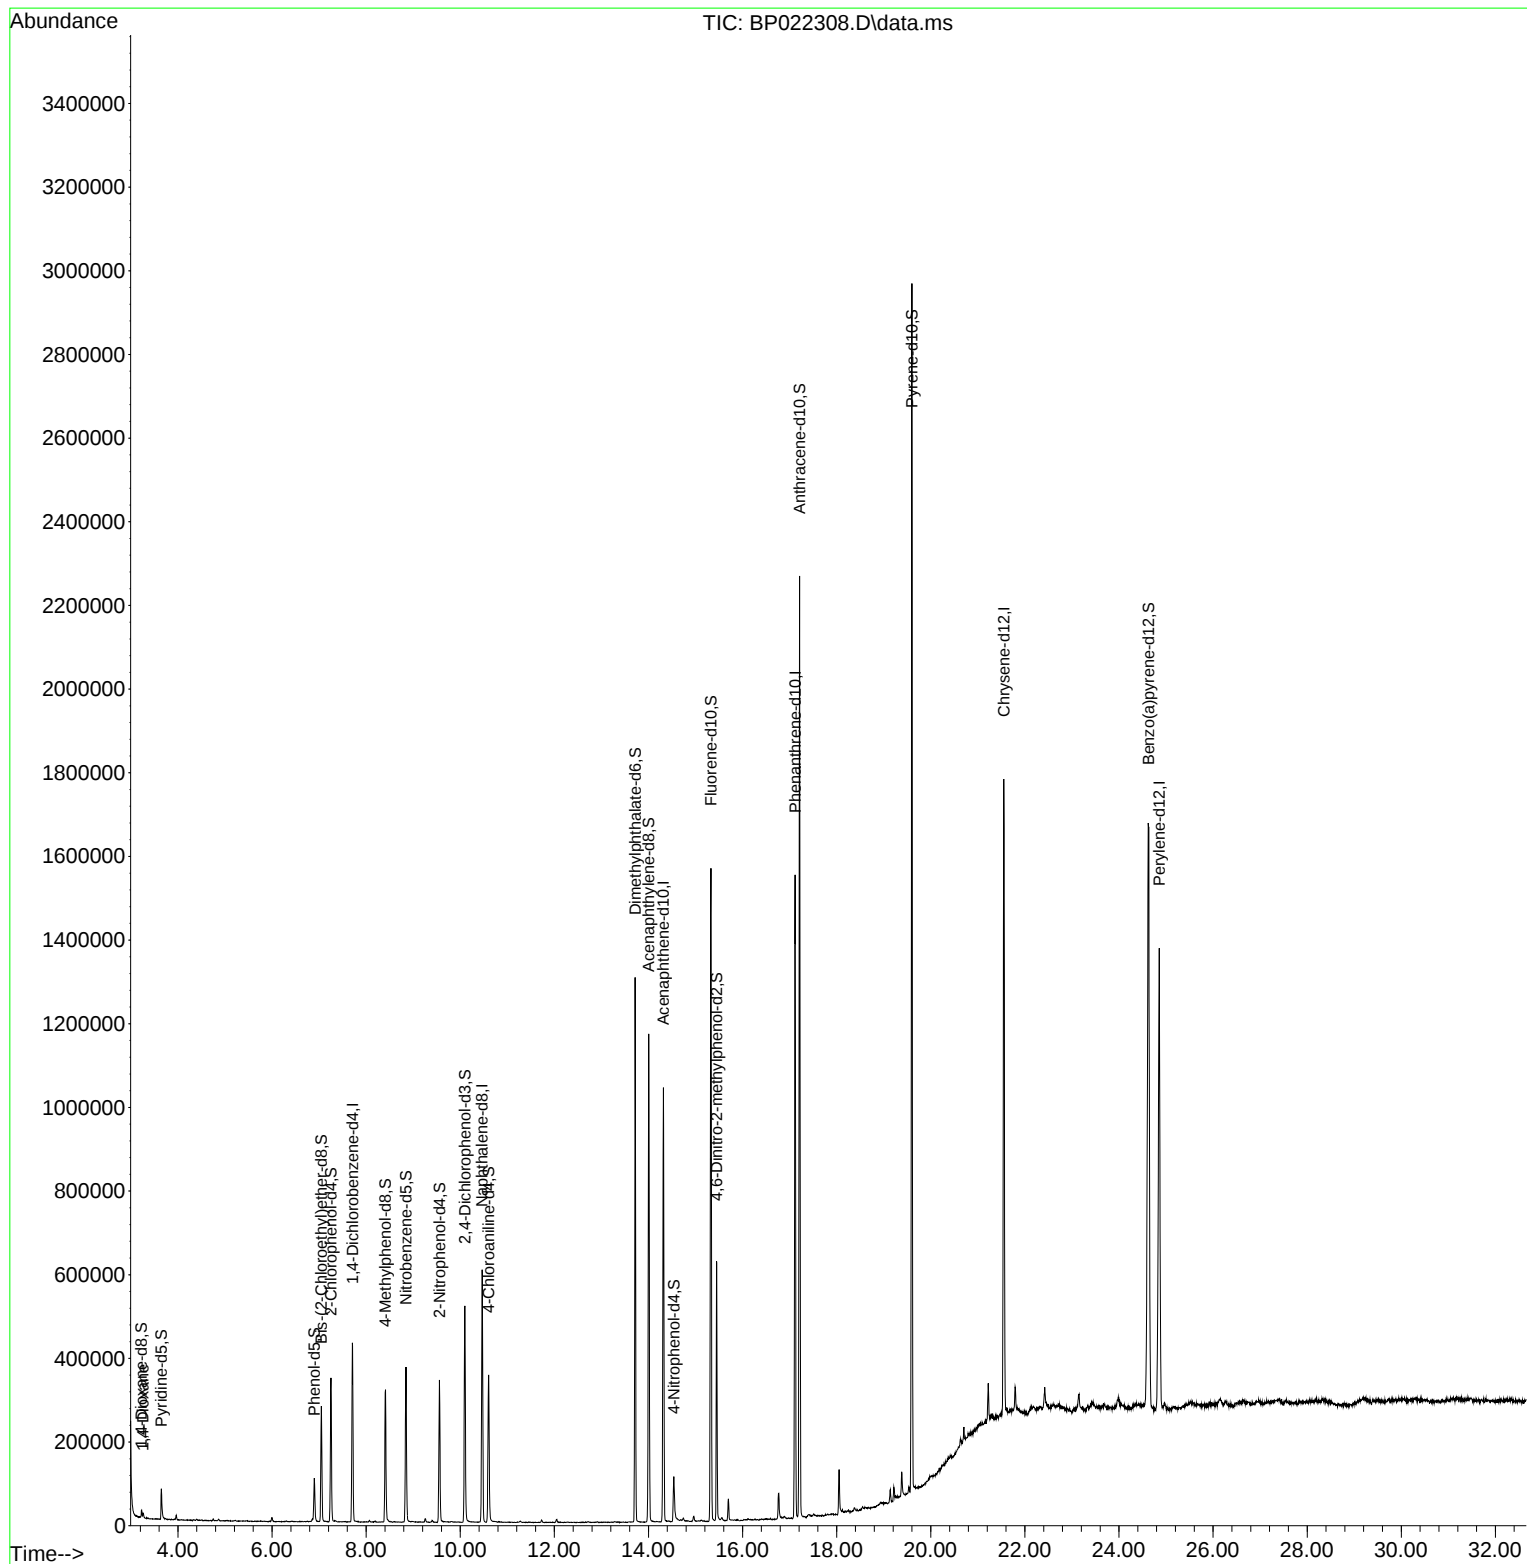

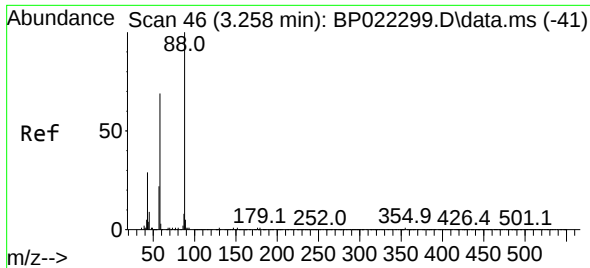

#2
 1,4-Dioxane
 Concen: 1.963 ng/uL
 RT: 3.258 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP022308.D
 Acq: 10 Oct 2024 03:57

Instrument :
 BNA_P
 ClientSampleId :
 EY052

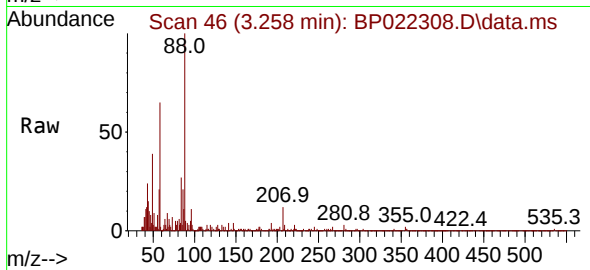

Tgt Ion: 88 Resp: 6415

Ion	Ratio	Lower	Upper
88	100		
43	23.8	22.3	33.5
58	64.6	54.7	82.1

