

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022312.D
 Acq On : 10 Oct 2024 06:41
 Operator : RC/JU
 Sample : P4207-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY062

Quant Time: Oct 10 07:16:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	127265	20.000	ng/u1	0.00
20) Naphthalene-d8	10.463	136	479009	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.316	164	365868	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.104	188	897598	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	985077	20.000	ng/u1	0.00
88) Perylene-d12	24.827	264	1110789	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	11954	3.650	ng/uL	0.00
4) Pyridine-d5	3.646	84	77501	8.620	ng/u1	0.01
7) Phenol-d5	6.899	99	108105	10.091	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.046	67	182595	29.000	ng/u1	0.00
11) 2-Chlorophenol-d4	7.246	132	222963	29.332	ng/u1	0.00
15) 4-Methylphenol-d8	8.410	113	184552	21.587	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	117490	31.900	ng/u1	0.00
24) 2-Nitrophenol-d4	9.557	143	148461	34.817	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	284636	31.407	ng/u1	0.00
31) 4-Chloroaniline-d4	10.599	131	280182	26.164	ng/u1	0.00
46) Dimethylphthalate-d6	13.716	166	902325	31.041	ng/u1	0.00
49) Acenaphthylene-d8	14.010	160	956440	30.978	ng/u1	0.01
54) 4-Nitrophenol-d4	14.551	143	42573	8.730	ng/u1	0.02
60) Fluorene-d10	15.322	176	798373	31.664	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	167346	28.348	ng/u1	0.00
73) Anthracene-d10	17.222	188	1457358	34.514	ng/u1	0.00
81) Pyrene-d10	19.586	212	1952204	37.476	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.604	264	2101235	35.421	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.264	88	18524	5.261	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022312.D
Acq On : 10 Oct 2024 06:41
Operator : RC/JU
Sample : P4207-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY062

Quant Time: Oct 10 07:16:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 08 02:14:47 2024
Response via : Initial Calibration

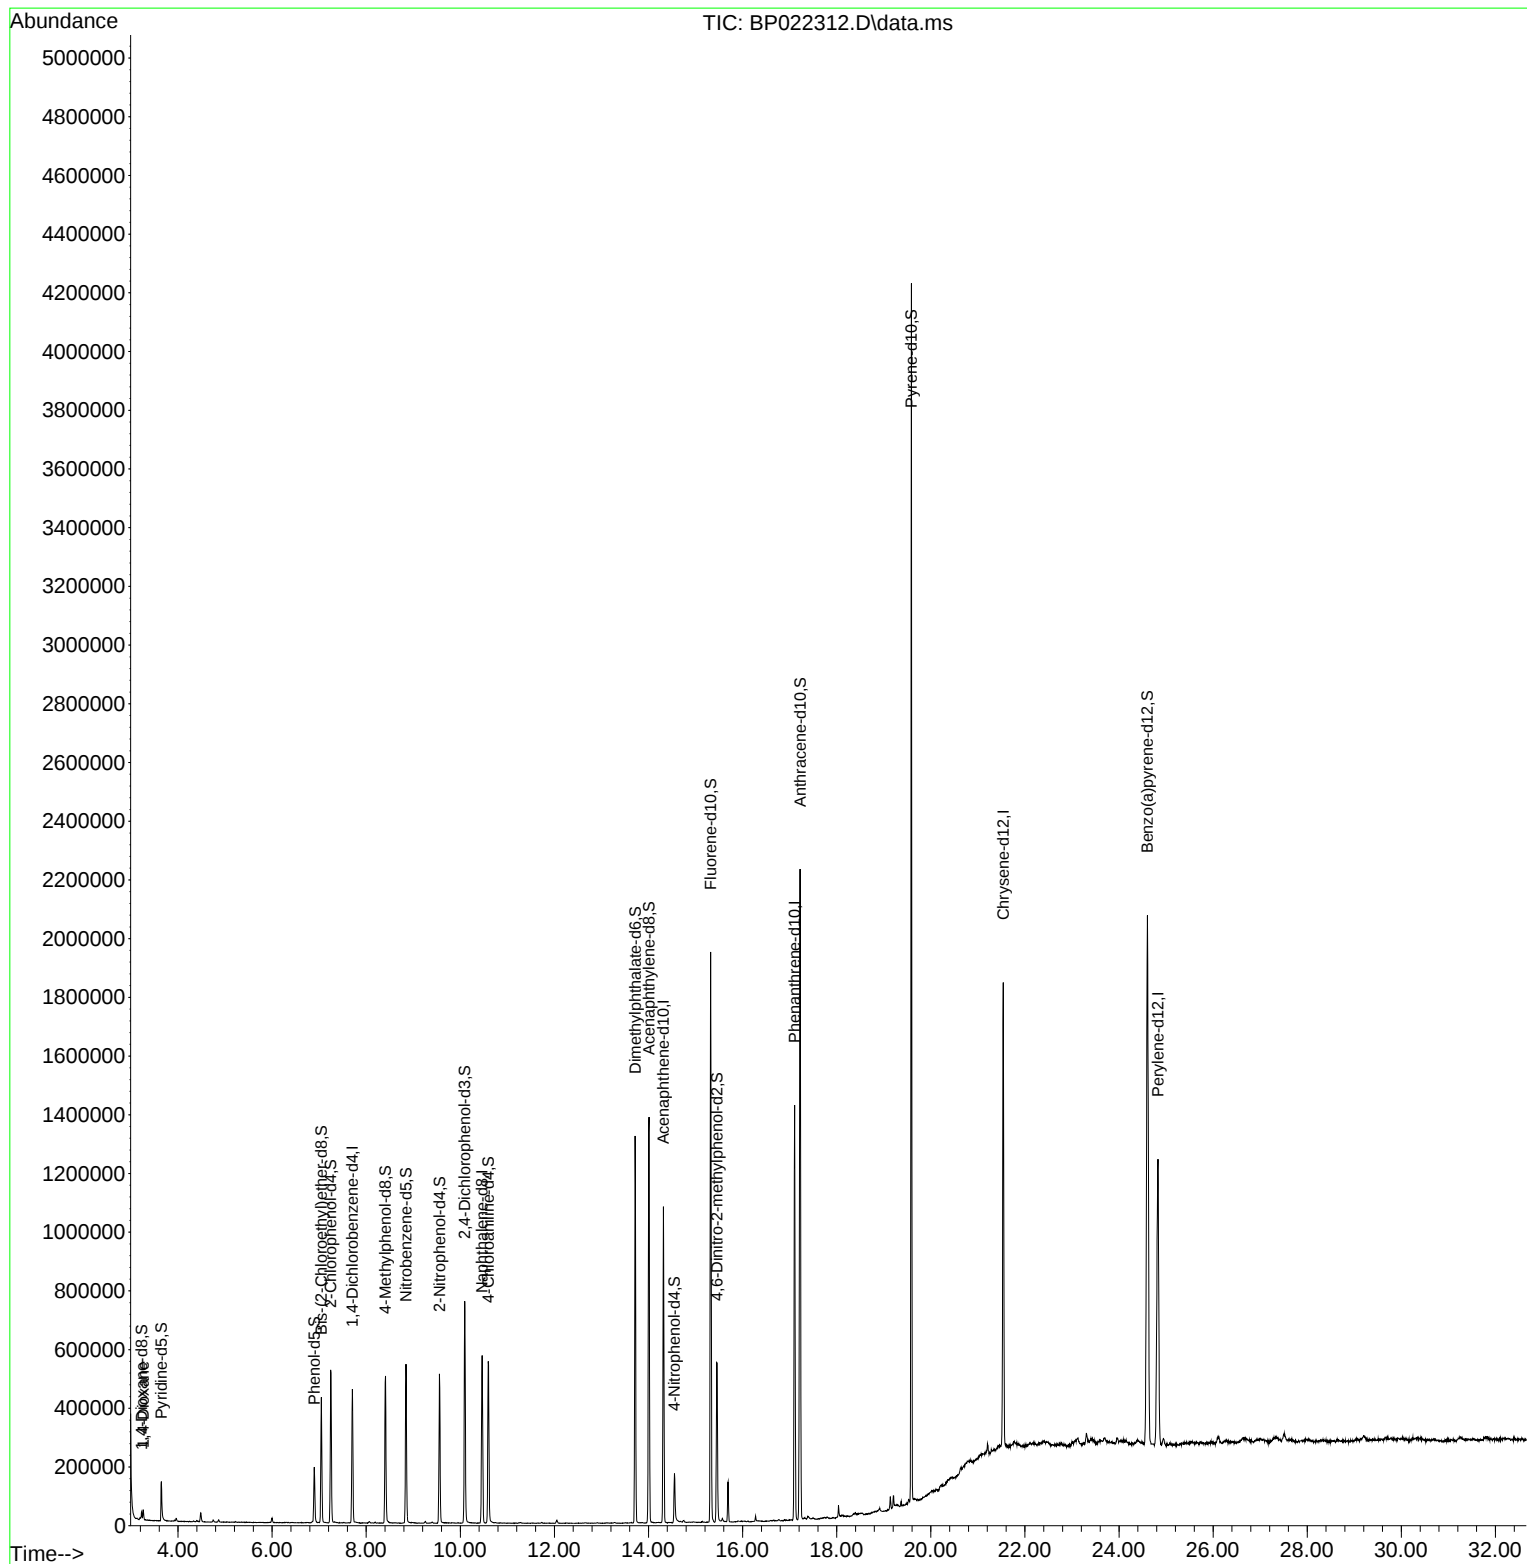

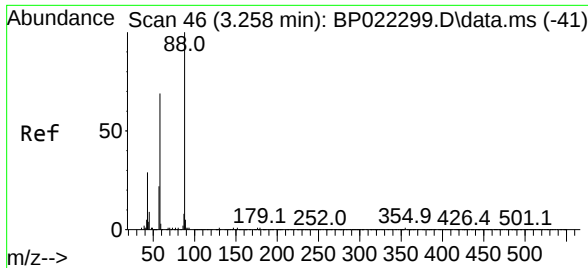

#2
1,4-Dioxane
Concen: 5.261 ng/uL
RT: 3.264 min Scan# 41
Delta R.T. 0.006 min
Lab File: BP022312.D
Acq: 10 Oct 2024 06:41

Instrument :
BNA_P
ClientSampleId :
EY062

Tgt Ion:	88	Resp:	18524
Ion	Ratio	Lower	Upper
88	100		
43	25.9	22.3	33.5
58	59.3	54.7	82.1

