

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022318.D
 Acq On : 10 Oct 2024 11:27
 Operator : RC/JU
 Sample : P4207-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY063

Quant Time: Oct 10 12:04:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 08 02:14:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	113409	20.000	ng/u1	0.00
20) Naphthalene-d8	10.457	136	454820	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.310	164	374900	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.116	188	939755	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1031343	20.000	ng/u1	0.00
88) Perylene-d12	24.839	264	1173997	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	9811	3.362	ng/uL	0.00
4) Pyridine-d5	3.646	84	66092	8.249	ng/u1	0.01
7) Phenol-d5	6.893	99	83315	8.727	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.046	67	152920	27.254	ng/u1	0.00
11) 2-Chlorophenol-d4	7.252	132	181651	26.816	ng/u1	0.00
15) 4-Methylphenol-d8	8.410	113	150640	19.773	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	101020	28.887	ng/u1	0.00
24) 2-Nitrophenol-d4	9.557	143	124116	30.655	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	242413	28.171	ng/u1	0.00
31) 4-Chloroaniline-d4	10.604	131	241690	23.770	ng/u1	0.01
46) Dimethylphthalate-d6	13.734	166	849905	28.533	ng/u1	0.02
49) Acenaphthylene-d8	14.010	160	883238	27.918	ng/u1	0.01
54) 4-Nitrophenol-d4	14.534	143	39122	7.829	ng/u1	0.00
60) Fluorene-d10	15.322	176	766923	29.684	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	168874	27.323	ng/u1	0.01
73) Anthracene-d10	17.216	188	1488241	33.664	ng/u1	0.00
81) Pyrene-d10	19.598	212	1887060	34.600	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.604	264	2111615	33.679	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.258	88	13700	4.366	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022318.D
Acq On : 10 Oct 2024 11:27
Operator : RC/JU
Sample : P4207-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY063


Quant Time: Oct 10 12:04:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 08 02:14:47 2024
Response via : Initial Calibration

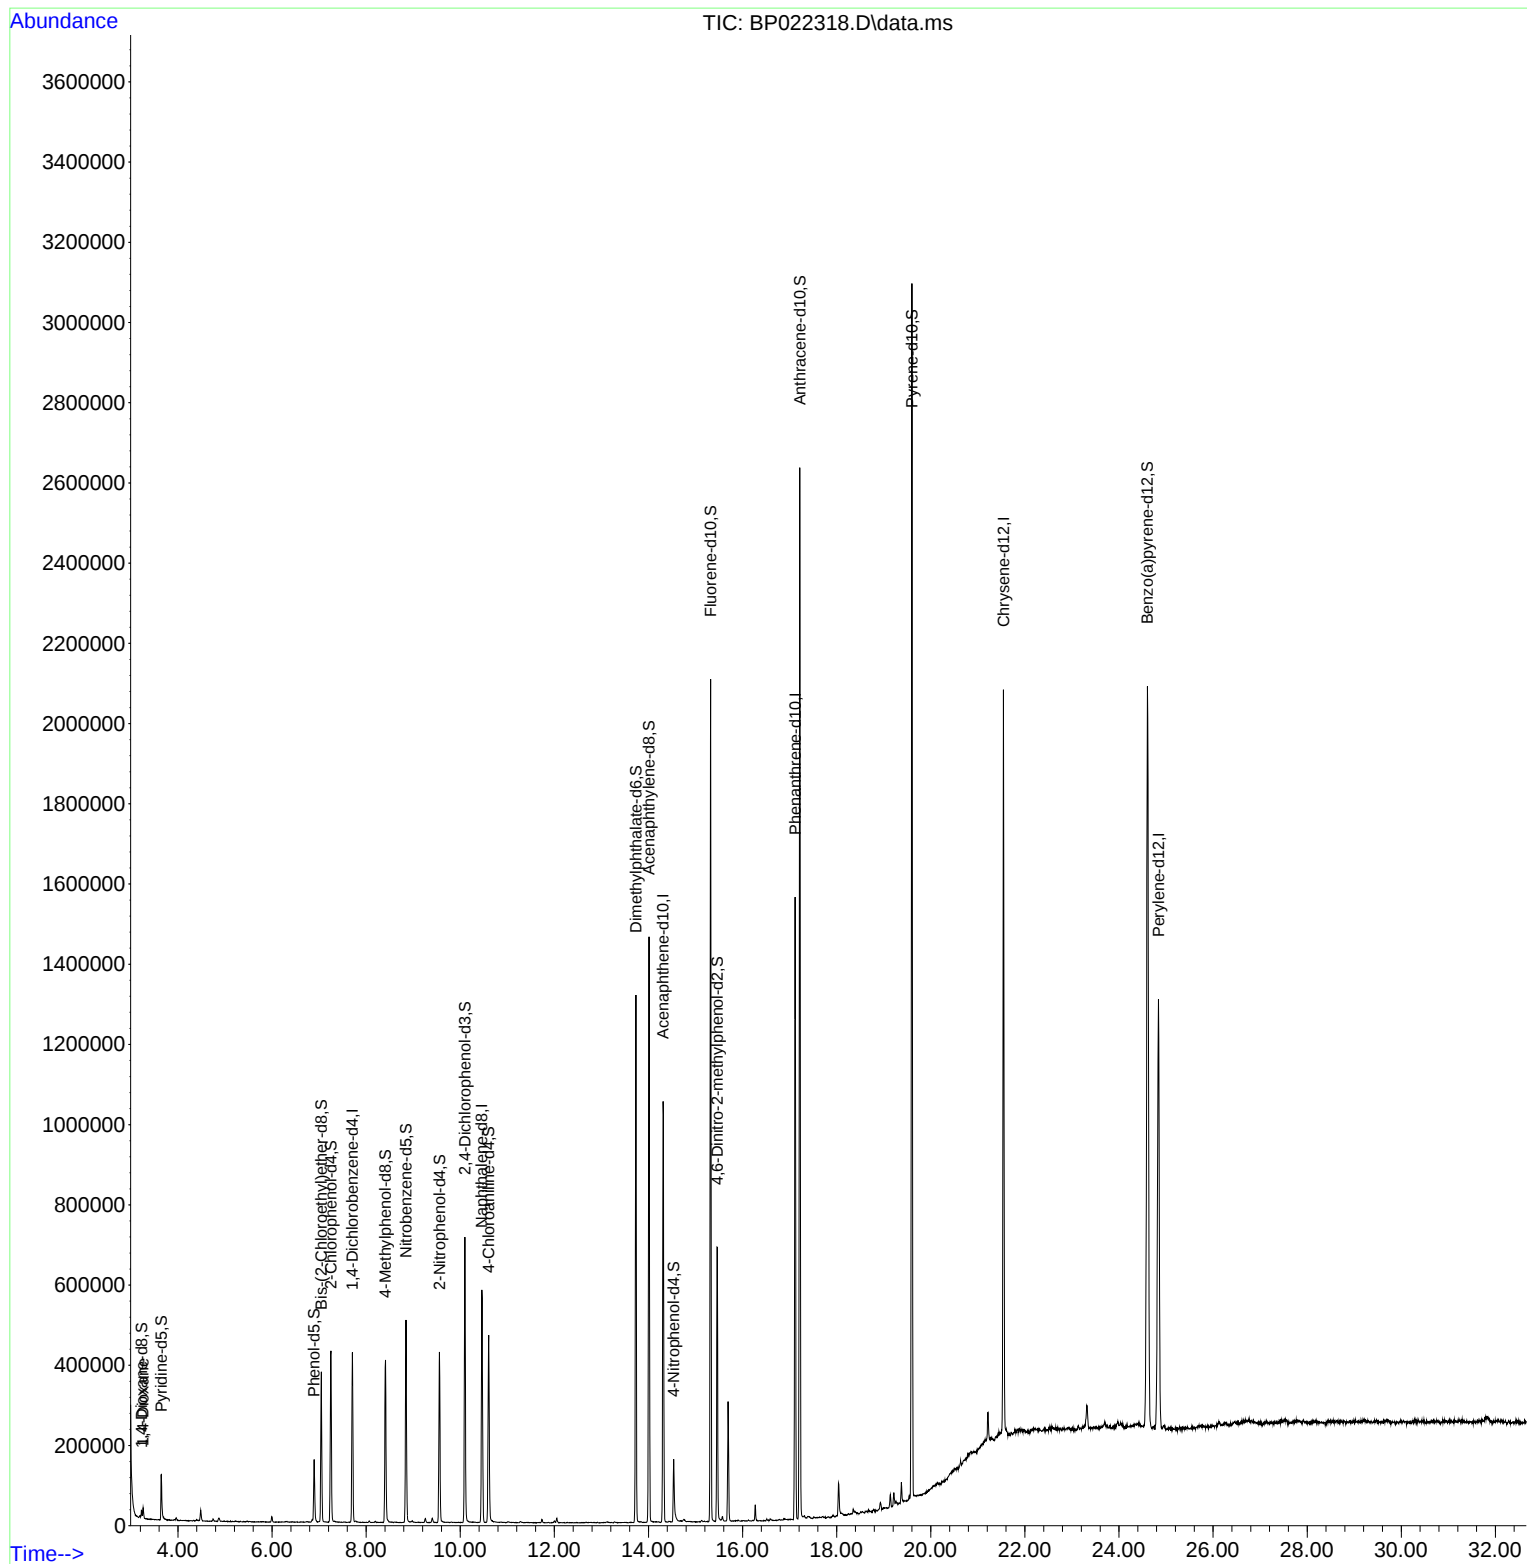

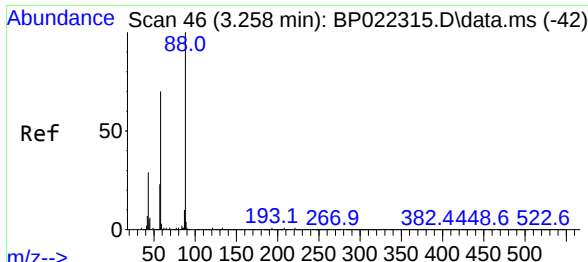

#2
1,4-Dioxane
Concen: 4.366 ng/uL
RT: 3.258 min Scan# 40
Delta R.T. -0.000 min
Lab File: BP022318.D
Acq: 10 Oct 2024 11:27

Instrument :
BNA_P
ClientSampleId :
EY063

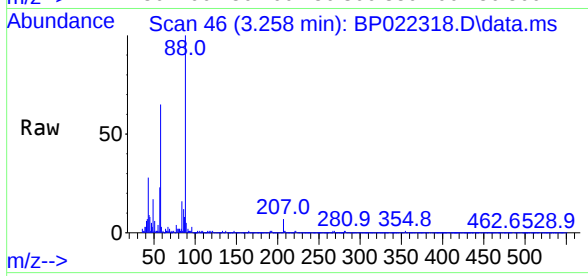

Tgt Ion: 88 Resp: 13700

Ion	Ratio	Lower	Upper
88	100		
43	27.6	22.3	33.5
58	65.1	54.7	82.1

