

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022300.D
 Acq On : 09 Oct 2024 22:30
 Operator : RC/JU
 Sample : PB163726BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK726

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	49	rVB	30560	44573	1.17%	0.117%
2	3.646	107	112	128	rBV	370268	582323	15.28%	1.529%
3	3.964	162	166	170	rBV2	6044	8768	0.23%	0.023%
4	4.399	236	240	244	rBV2	5551	9364	0.25%	0.025%
5	6.858	652	658	661	rBV	111179	179833	4.72%	0.472%
6	6.899	661	665	680	rVV	519149	831164	21.81%	2.182%
7	7.046	684	690	701	rVB	382473	605395	15.89%	1.589%
8	7.252	717	725	735	rBV	527146	841730	22.09%	2.210%
9	7.710	795	803	813	rBV	489135	801840	21.04%	2.105%
10	8.410	914	922	933	rBV	639815	1064095	27.92%	2.793%
11	8.846	989	996	1011	rBV	491329	823950	21.62%	2.163%
12	9.257	1059	1066	1074	rVB	42848	64474	1.69%	0.169%
13	9.557	1109	1117	1128	rBV	455701	740651	19.44%	1.944%
14	10.099	1201	1209	1224	rBV	694381	1200440	31.50%	3.151%
15	10.463	1263	1271	1282	rBV	692100	1143589	30.01%	3.002%
16	10.599	1287	1294	1306	rBV	608313	1069426	28.06%	2.807%
17	11.734	1480	1487	1491	rBV3	8505	14386	0.38%	0.038%
18	12.051	1536	1541	1548	rBV2	11430	20814	0.55%	0.055%
19	13.722	1817	1825	1834	rBV	1165196	1759976	46.18%	4.620%
20	14.004	1864	1873	1888	rBV	1527991	2086254	54.75%	5.477%
21	14.316	1919	1926	1935	rBV	1227140	1721216	45.17%	4.519%
22	14.539	1958	1964	1975	rBV	510107	886994	23.28%	2.329%
23	14.681	1986	1988	1993	rVB6	2758	3854	0.10%	0.010%
24	15.322	2091	2097	2106	rBV	2085580	2717148	71.30%	7.133%
25	15.451	2112	2119	2126	rBV	462997	656299	17.22%	1.723%
26	15.575	2135	2140	2144	rVB4	9902	14185	0.37%	0.037%
27	16.592	2311	2313	2319	rBV7	3058	4334	0.11%	0.011%
28	16.904	2361	2366	2368	rBV6	4267	7763	0.20%	0.020%
29	17.110	2395	2401	2408	rBV	1661395	2319634	60.87%	6.090%
30	17.216	2412	2419	2429	rVV	2029036	3161505	82.96%	8.300%
31	17.381	2443	2447	2458	rBV	27878	61353	1.61%	0.161%
32	19.139	2743	2746	2750	rBV2	37987	52614	1.38%	0.138%
33	19.210	2755	2758	2762	rVB	28029	41197	1.08%	0.108%
34	19.586	2817	2822	2831	rVB	2668715	3810837	100.00%	10.004%
35	21.545	3149	3155	3173	rVB2	1436065	2694360	70.70%	7.073%
36	24.615	3668	3677	3686	rVB	1356398	3512022	92.16%	9.220%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022300.D
Acq On : 09 Oct 2024 22:30
Operator : RC/JU
Sample : PB163726BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK726

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Title : SVOA CALIBRATION

37	24.839	3707	3715	3726	rVB	914680	2533985	66.49%	6.652%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 38092345

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022300.D
Acq On : 09 Oct 2024 22:30
Operator : RC/JU
Sample : PB163726BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

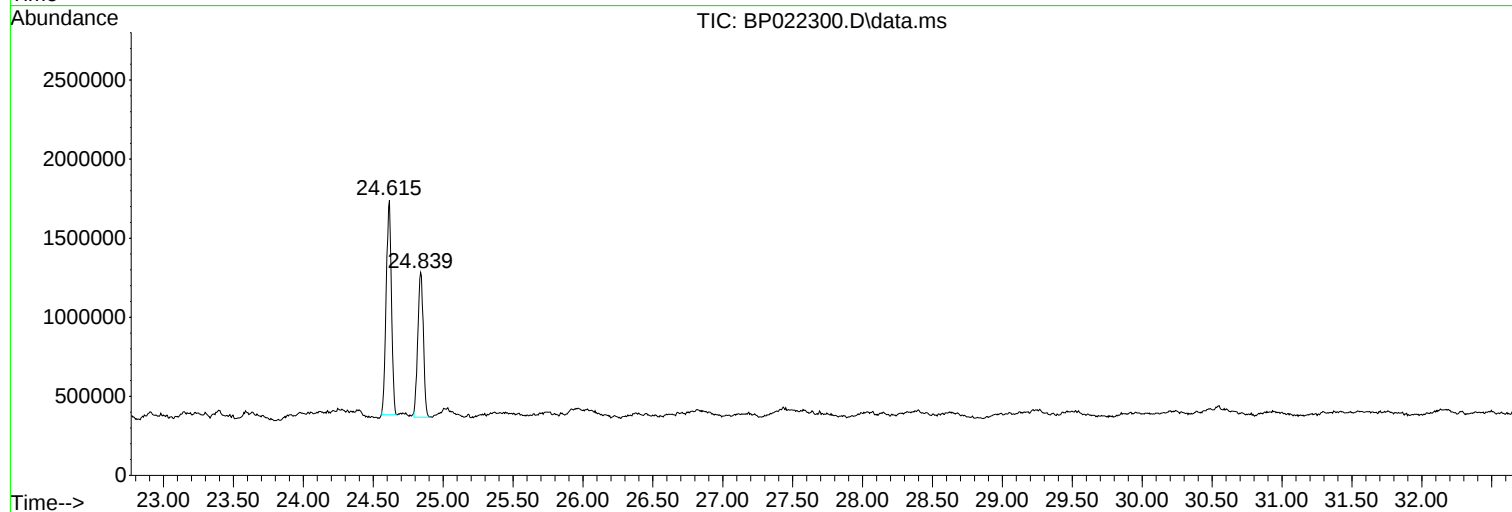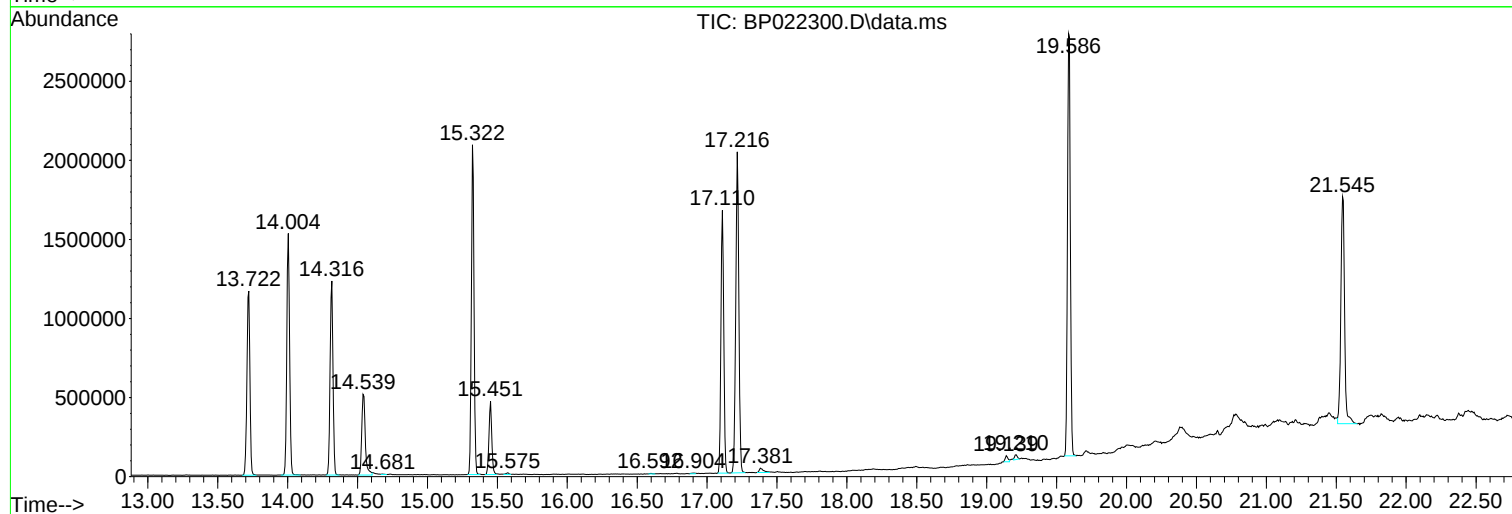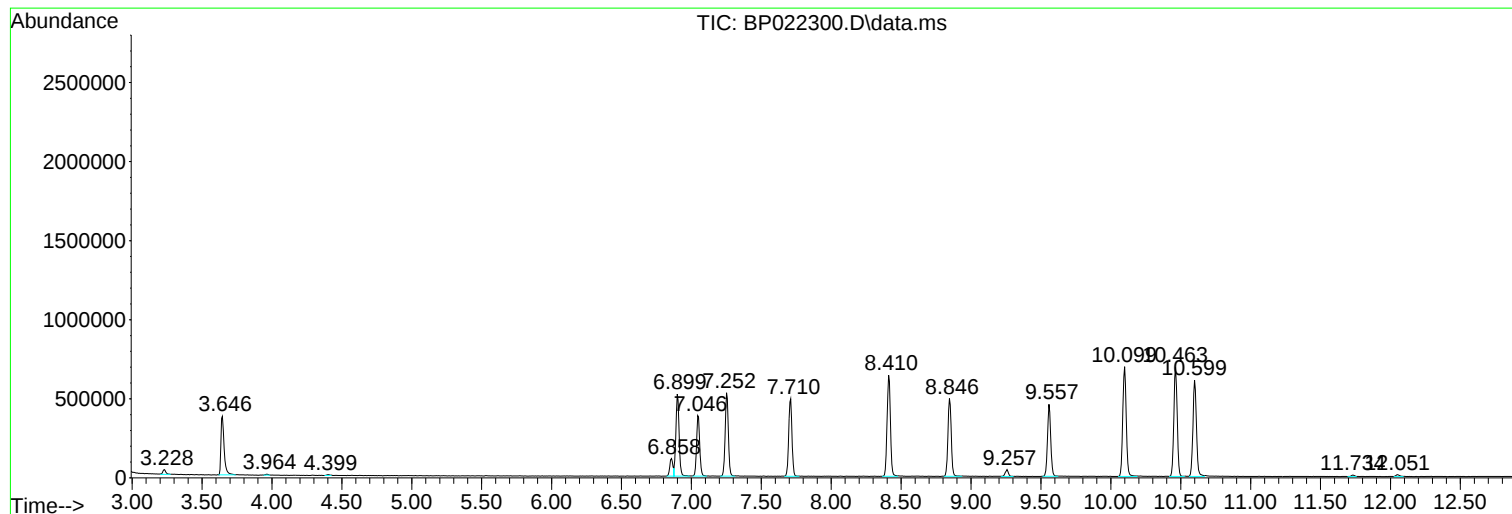

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022300.D
Acq On : 09 Oct 2024 22:30
Operator : RC/JU
Sample : PB163726BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022300.D
Acq On : 09 Oct 2024 22:30
Operator : RC/JU
Sample : PB163726BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------