

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022303.D
 Acq On : 10 Oct 2024 00:33
 Operator : RC/JU
 Sample : P4207-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY069

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.229	37	41	46	rVB	21430	26243	0.63%	0.068%
2	3.646	108	112	125	rBV	65239	107388	2.56%	0.277%
3	3.964	161	166	171	rVB2	21386	30805	0.74%	0.079%
4	4.405	238	241	249	rVB4	3945	8063	0.19%	0.021%
5	4.746	294	299	304	rBV5	7046	11701	0.28%	0.030%
6	4.864	315	319	324	rBV	6828	10074	0.24%	0.026%
7	5.999	507	512	520	rVB3	14571	24693	0.59%	0.064%
8	6.852	653	657	659	rBV	8725	11474	0.27%	0.030%
9	6.899	659	665	676	rVB	176965	287269	6.86%	0.740%
10	7.046	683	690	699	rBV	408575	652333	15.57%	1.681%
11	7.111	699	701	706	rVB6	3652	4477	0.11%	0.012%
12	7.252	717	725	735	rBV	502815	821966	19.62%	2.118%
13	7.711	794	803	810	rBV	544691	845947	20.20%	2.180%
14	8.069	859	864	869	rVB7	7930	11194	0.27%	0.029%
15	8.193	879	885	888	rVB8	3709	6424	0.15%	0.017%
16	8.405	914	921	936	rBV	462976	806716	19.26%	2.079%
17	8.846	988	996	1006	rBV	527487	912734	21.79%	2.352%
18	9.258	1059	1066	1071	rBV2	12389	22129	0.53%	0.057%
19	9.399	1086	1090	1096	rVB7	3642	7209	0.17%	0.019%
20	9.558	1108	1117	1130	rBV	448671	830288	19.82%	2.140%
21	9.740	1142	1148	1156	rBV2	17424	37867	0.90%	0.098%
22	10.093	1199	1208	1220	rBV	729976	1290294	30.81%	3.325%
23	10.463	1258	1271	1282	rBV	680939	1222280	29.18%	3.150%
24	10.605	1287	1295	1310	rBV	482973	826418	19.73%	2.130%
25	11.234	1397	1402	1404	rBV6	4050	5391	0.13%	0.014%
26	11.269	1406	1408	1417	rVB10	4700	8339	0.20%	0.021%
27	11.728	1480	1486	1493	rBV3	8412	15775	0.38%	0.041%
28	12.052	1535	1541	1548	rVB	13219	22053	0.53%	0.057%
29	12.269	1571	1578	1583	rBV9	2364	5485	0.13%	0.014%
30	12.675	1642	1647	1650	rBV6	2435	4260	0.10%	0.011%
31	13.046	1705	1710	1712	rBV6	2315	4325	0.10%	0.011%
32	13.287	1745	1751	1753	rBV6	2978	5029	0.12%	0.013%
33	13.722	1818	1825	1835	rBV	1649172	1930199	46.08%	4.975%
34	14.010	1864	1874	1890	rBV2	1346539	2244990	53.60%	5.786%
35	14.316	1918	1926	1935	rBV	1105962	1871429	44.68%	4.823%
36	14.540	1957	1964	1979	rBV	129304	292846	6.99%	0.755%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022303.D
 Acq On : 10 Oct 2024 00:33
 Operator : RC/JU
 Sample : P4207-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY069

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	14.757	1995	2001	2007	rVB	6365	10468	0.25%	0.027%
38	15.122	2059	2063	2067	rBV2	6176	9143	0.22%	0.024%
39	15.322	2090	2097	2111	rBV	1930831	2939213	70.17%	7.575%
40	15.457	2114	2120	2129	rBV	673994	845092	20.18%	2.178%
41	15.563	2134	2138	2143	rVB2	13601	20568	0.49%	0.053%
42	15.704	2156	2162	2168	rBV	37140	55052	1.31%	0.142%
43	16.122	2228	2233	2235	rBV5	5600	8685	0.21%	0.022%
44	16.598	2311	2314	2318	rVB5	4918	6278	0.15%	0.016%
45	16.769	2335	2343	2345	rBV8	7555	15983	0.38%	0.041%
46	16.875	2358	2361	2363	rBV4	4237	6008	0.14%	0.015%
47	17.116	2396	2402	2409	rBV	1652687	2386984	56.99%	6.152%
48	17.210	2412	2418	2432	rVB2	2216017	3517391	83.98%	9.065%
49	17.392	2444	2449	2450	rBV2	13442	19231	0.46%	0.050%
50	17.510	2466	2469	2473	rBV5	7600	10873	0.26%	0.028%
51	17.787	2513	2516	2524	rBV8	10474	24583	0.59%	0.063%
52	18.051	2557	2561	2568	rBV3	37389	65978	1.58%	0.170%
53	18.975	2715	2718	2722	rBV4	19791	28503	0.68%	0.073%
54	19.134	2742	2745	2750	rVB3	33858	47492	1.13%	0.122%
55	19.216	2755	2759	2762	rBV	41401	56738	1.35%	0.146%
56	19.592	2817	2823	2831	rBV2	2969014	4188513	100.00%	10.795%
57	21.545	3149	3155	3162	rVB	1587816	2479782	59.20%	6.391%
58	24.616	3667	3677	3690	rVB	1653713	4186528	99.95%	10.790%
59	24.845	3707	3716	3726	rVB2	963692	2646610	63.19%	6.821%




Sum of corrected areas: 38801803

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022303.D
Acq On : 10 Oct 2024 00:33
Operator : RC/JU
Sample : P4207-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY069

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

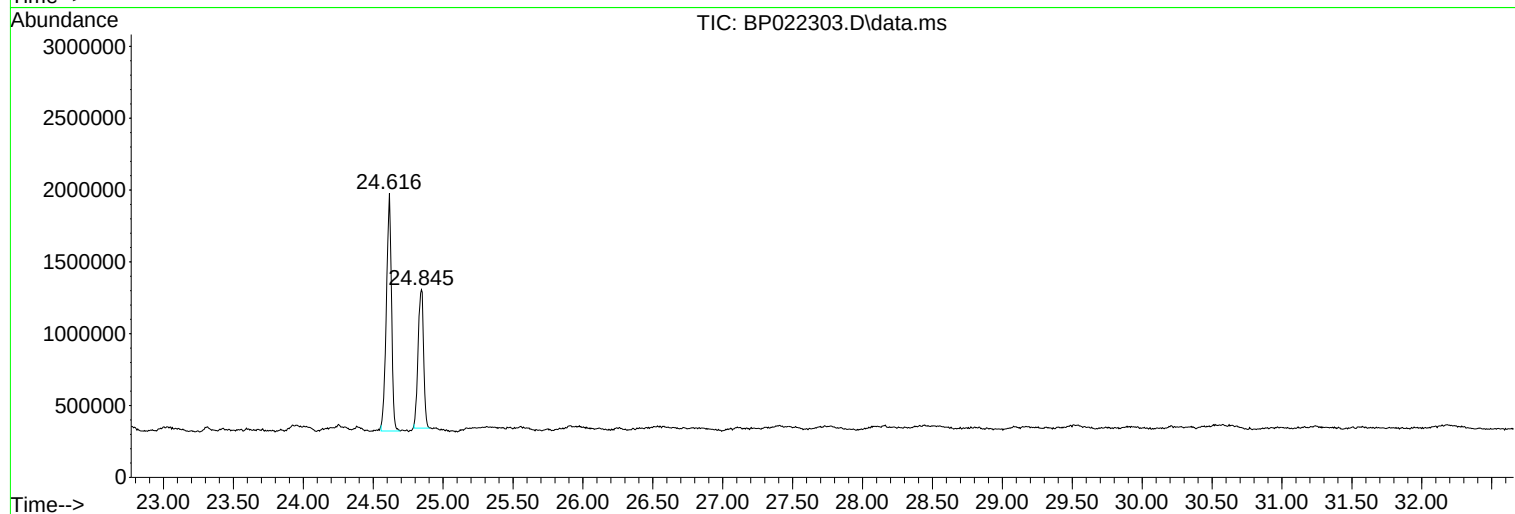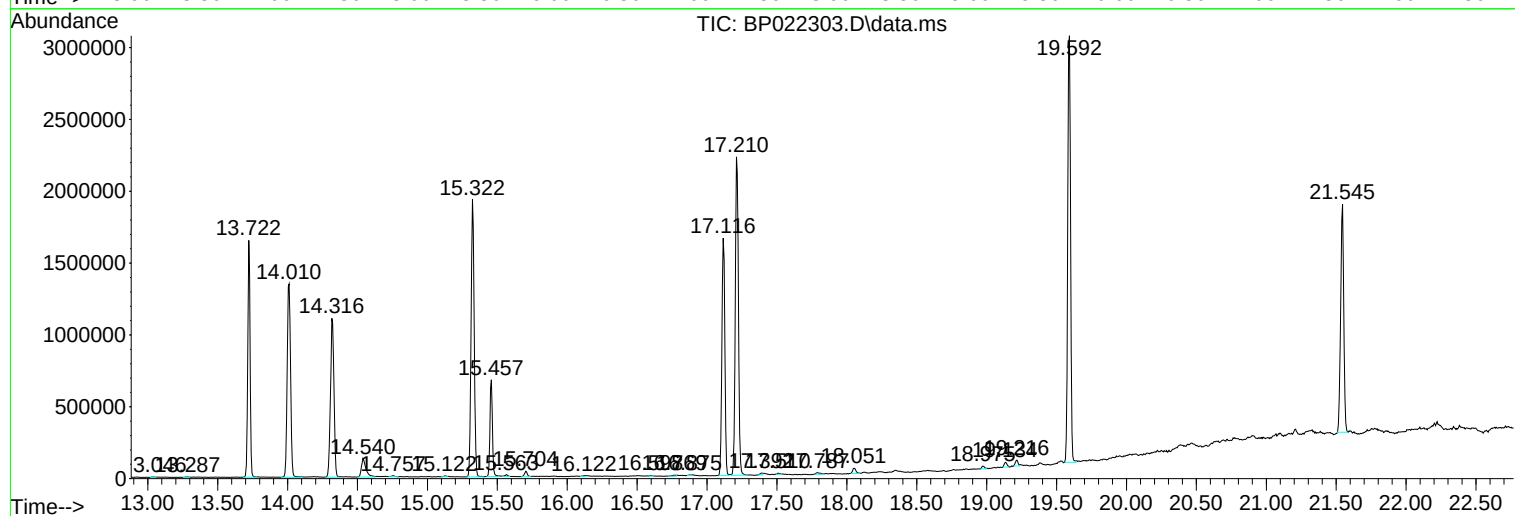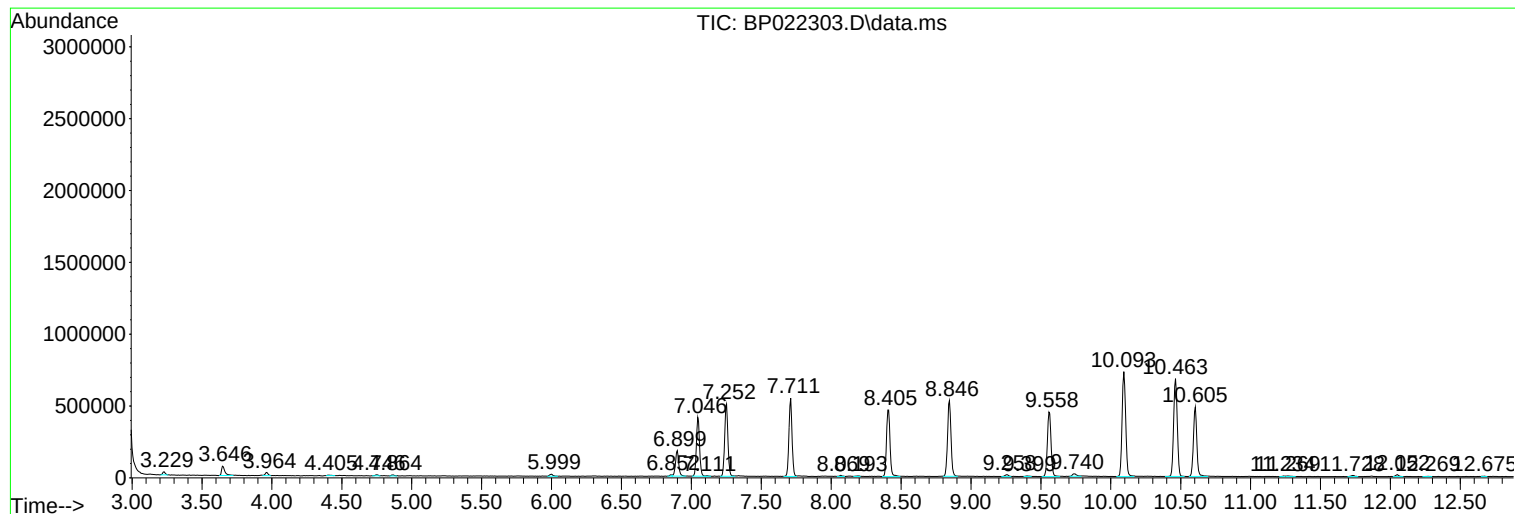

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022303.D
Acq On : 10 Oct 2024 00:33
Operator : RC/JU
Sample : P4207-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY069

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022303.D
Acq On : 10 Oct 2024 00:33
Operator : RC/JU
Sample : P4207-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY069

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc