

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022308.D
 Acq On : 10 Oct 2024 03:57
 Operator : RC/JU
 Sample : P4207-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	37	41	44	rBV	16831	21436	0.53%	0.063%
2	3.258	44	46	56	rVB	12416	18755	0.47%	0.055%
3	3.646	108	112	124	rBV	73461	118244	2.94%	0.347%
4	3.964	161	166	172	rVB	12006	18622	0.46%	0.055%
5	4.399	236	240	244	rVB5	3161	4966	0.12%	0.015%
6	4.752	296	300	303	rVB2	4093	4633	0.12%	0.014%
7	4.864	314	319	324	rVB5	4228	7569	0.19%	0.022%
8	5.993	508	511	517	rVB5	9142	14430	0.36%	0.042%
9	6.852	653	657	658	rBV	5558	5766	0.14%	0.017%
10	6.899	659	665	675	rVB	103692	177931	4.42%	0.522%
11	7.046	683	690	700	rBV	276234	445239	11.05%	1.307%
12	7.252	717	725	736	rBV	344451	566451	14.06%	1.662%
13	7.705	795	802	812	rBV	427950	713916	17.72%	2.095%
14	8.069	860	864	869	rVB7	4090	5849	0.15%	0.017%
15	8.187	880	884	888	rVB7	2651	4656	0.12%	0.014%
16	8.410	914	922	935	rBV	316285	533784	13.25%	1.567%
17	8.846	988	996	1006	rBV	370623	631538	15.68%	1.853%
18	9.257	1062	1066	1072	rVB3	8613	13812	0.34%	0.041%
19	9.399	1086	1090	1097	rVB7	4575	7577	0.19%	0.022%
20	9.557	1109	1117	1126	rBV	340838	573978	14.25%	1.685%
21	10.099	1201	1209	1219	rBV	517282	914032	22.69%	2.683%
22	10.463	1263	1271	1286	rVB	603992	1014028	25.18%	2.976%
23	10.599	1286	1294	1309	rBV	351452	677600	16.82%	1.989%
24	11.275	1402	1409	1416	rBV	3186	6757	0.17%	0.020%
25	11.728	1481	1486	1492	rVB3	6118	9047	0.22%	0.027%
26	12.051	1533	1541	1545	rBV3	8021	15511	0.39%	0.046%
27	12.716	1649	1654	1660	rBV10	2180	4208	0.10%	0.012%
28	12.916	1683	1688	1693	rVB9	2322	4429	0.11%	0.013%
29	13.716	1815	1824	1835	rBV	1302346	1620889	40.24%	4.757%
30	14.004	1862	1873	1887	rBV	1167109	1686934	41.88%	4.951%
31	14.316	1917	1926	1935	rBV	1038195	1604901	39.85%	4.710%
32	14.540	1957	1964	1975	rBV	107544	224210	5.57%	0.658%
33	14.687	1985	1989	1993	rBV7	2540	4580	0.11%	0.013%
34	14.740	1994	1998	2003	rVB8	7049	11588	0.29%	0.034%
35	14.963	2029	2036	2041	rBV5	12630	24713	0.61%	0.073%
36	15.328	2087	2098	2111	rBV	1562150	2412691	59.90%	7.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
 Data File : BP022308.D
 Acq On : 10 Oct 2024 03:57
 Operator : RC/JU
 Sample : P4207-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EY052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
 Title : SVOA CALIBRATION

37	15.445	2111	2118	2132	rVV	620480	815609	20.25%	2.394%
38	15.563	2133	2138	2144	rVB4	6969	15353	0.38%	0.045%
39	15.698	2155	2161	2168	rBV	52216	78009	1.94%	0.229%
40	15.898	2192	2195	2200	rVB7	3078	4869	0.12%	0.014%
41	16.257	2253	2256	2261	rBV6	2710	4468	0.11%	0.013%
42	16.504	2293	2298	2302	rVB8	2547	4121	0.10%	0.012%
43	16.769	2334	2343	2351	rBV	62469	117946	2.93%	0.346%
44	17.116	2393	2402	2411	rBV	1539082	2226138	55.27%	6.533%
45	17.210	2412	2418	2431	rVB	2250455	3151920	78.25%	9.251%
46	17.510	2466	2469	2473	rBV5	3999	5597	0.14%	0.016%
47	18.051	2555	2561	2570	rBV2	108520	185466	4.60%	0.544%
48	19.139	2741	2746	2750	rBV2	31857	46624	1.16%	0.137%
49	19.216	2755	2759	2763	rBV2	35068	58585	1.45%	0.172%
50	19.380	2783	2787	2795	rBV4	58678	101113	2.51%	0.297%
51	19.598	2817	2824	2831	rBV	2889798	4027765	100.00%	11.821%
52	21.551	3150	3156	3163	rBV2	1513636	2462756	61.14%	7.228%
53	24.621	3669	3678	3692	rVB	1398582	4025916	99.95%	11.816%
54	24.857	3709	3718	3728	rVB	1099248	2615289	64.93%	7.676%




Sum of corrected areas: 34072814

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022308.D
Acq On : 10 Oct 2024 03:57
Operator : RC/JU
Sample : P4207-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY052

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

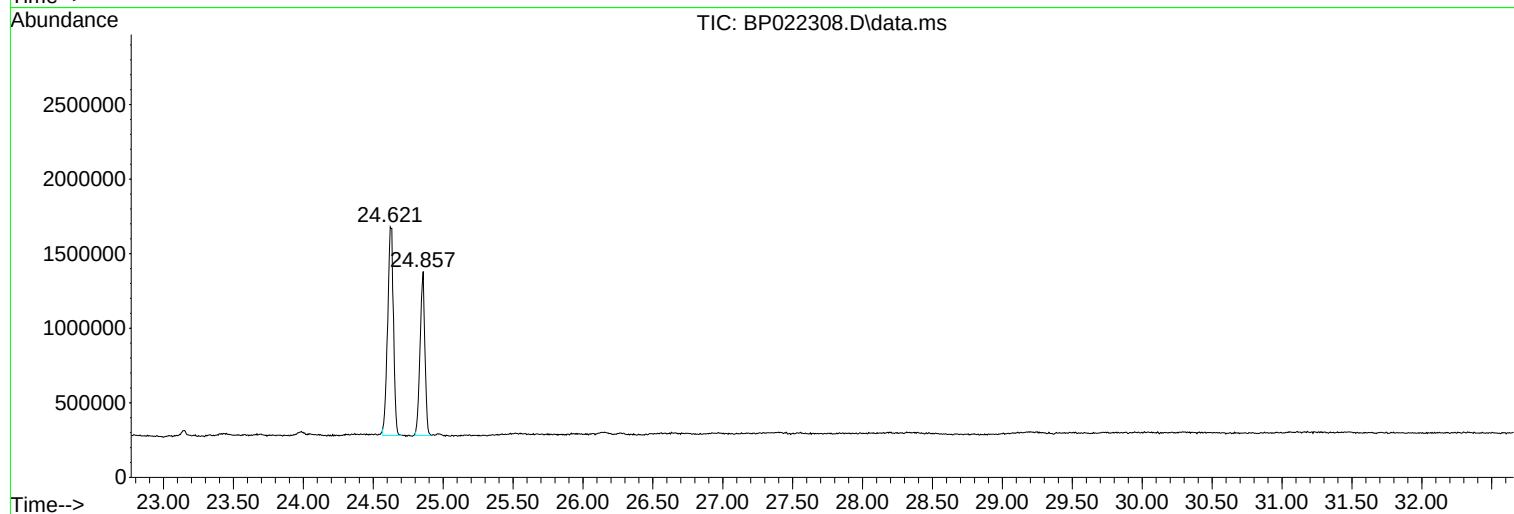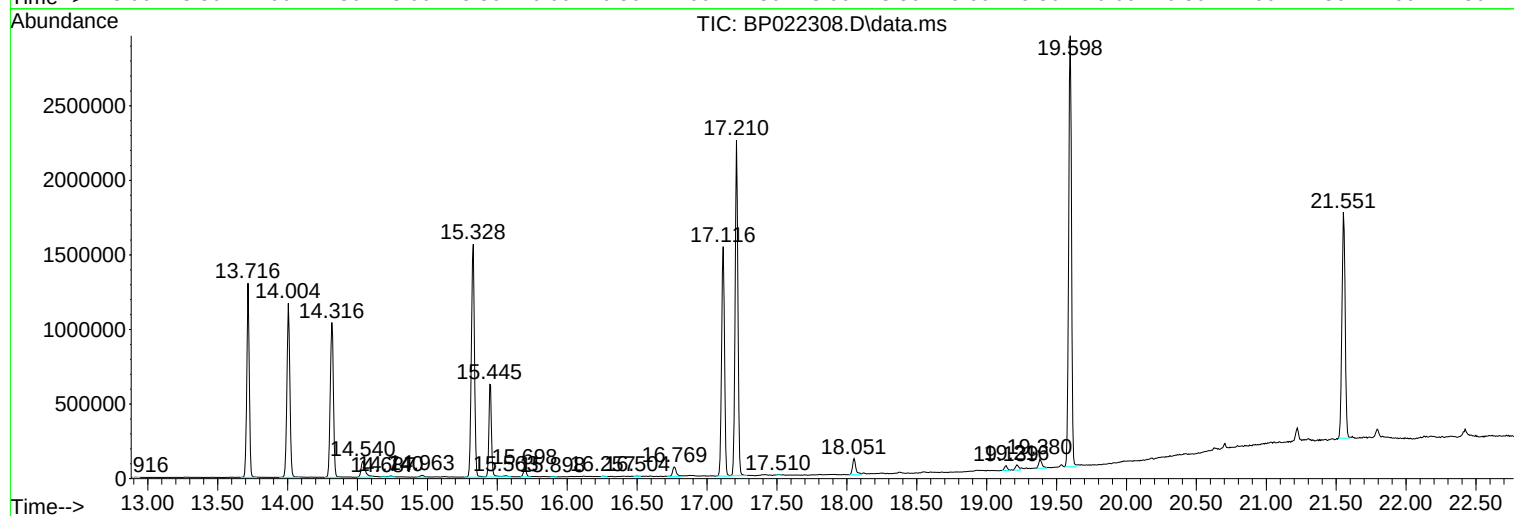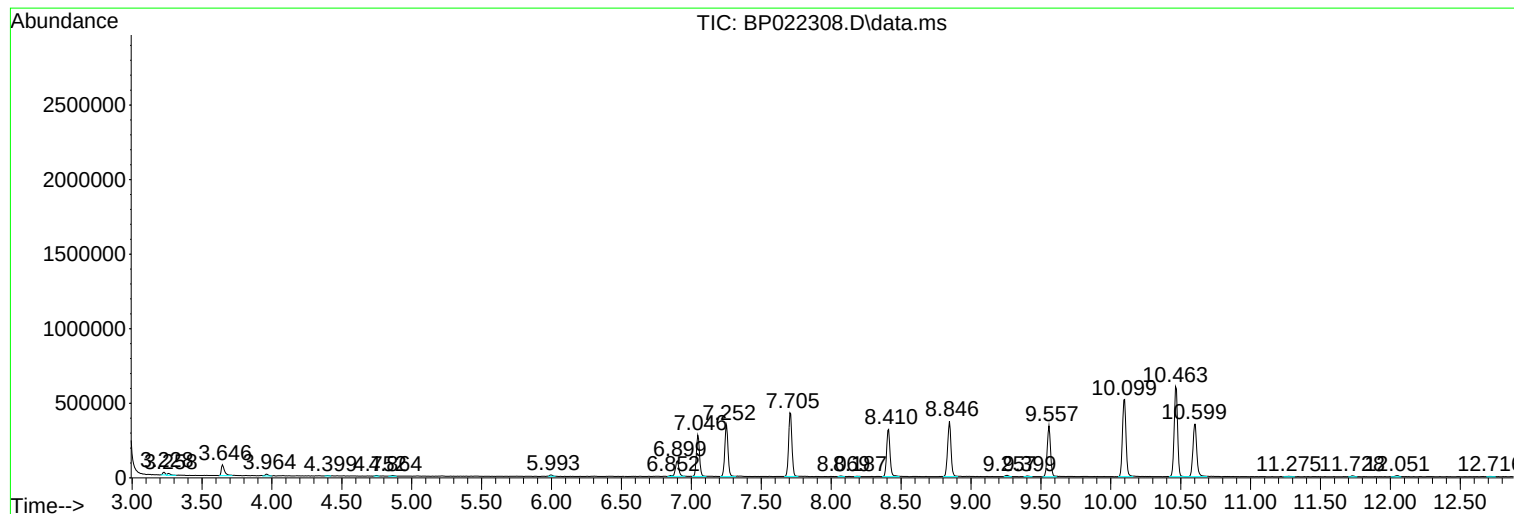

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022308.D
Acq On : 10 Oct 2024 03:57
Operator : RC/JU
Sample : P4207-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY052

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100924\
Data File : BP022308.D
Acq On : 10 Oct 2024 03:57
Operator : RC/JU
Sample : P4207-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EY052

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------